


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014784.D
Acq On : 09 Mar 2020 18:13
Operator : SY/MD
Sample : L1835-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DJ1

Manual Integrations
APPROVED

MMDadoda
3/11/2020 9:41:39 AM

Quant Time: Mar 10 16:58:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 10 14:44:37 2020
Response via : Initial Calibration

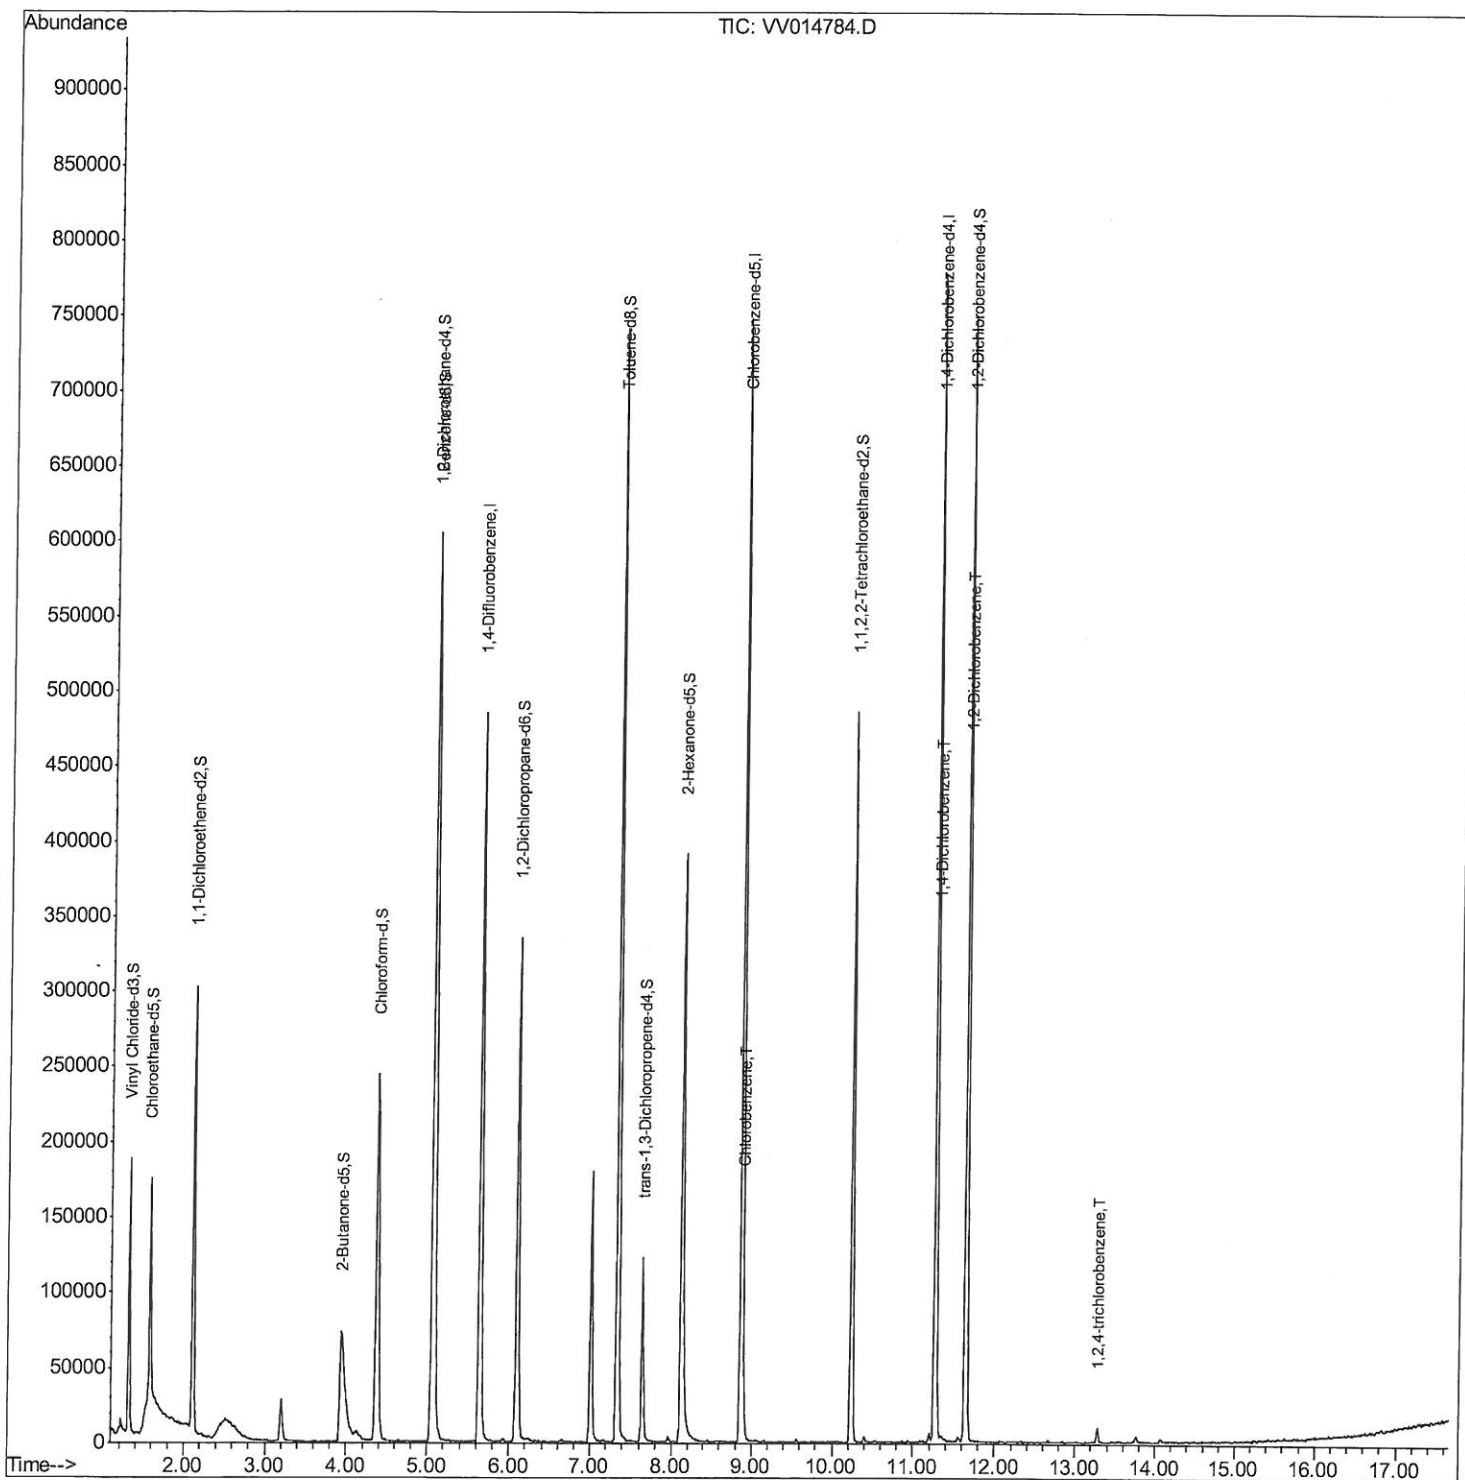

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014784.D
 Acq On : 09 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1835-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ1

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:39 AM

Quant Time: Mar 10 14:50:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

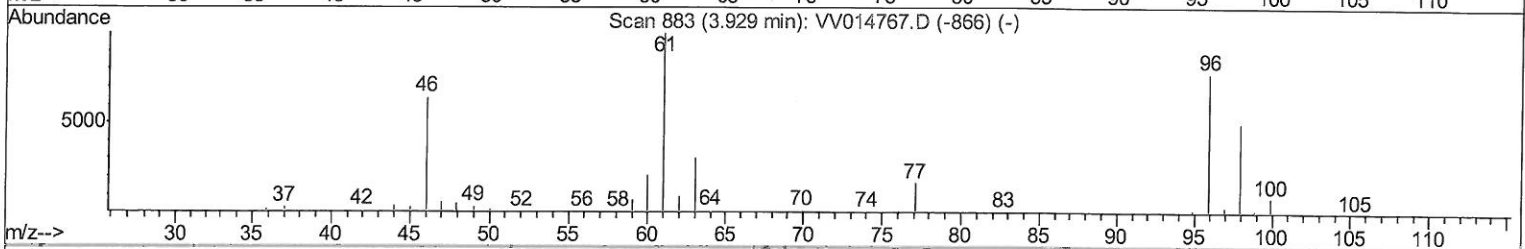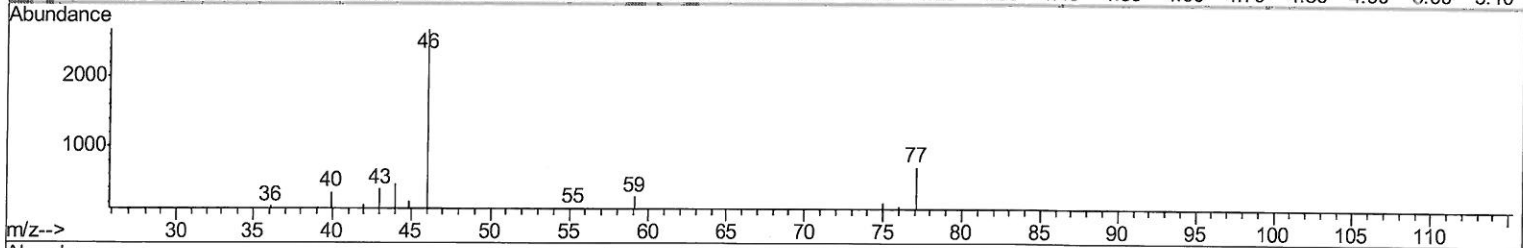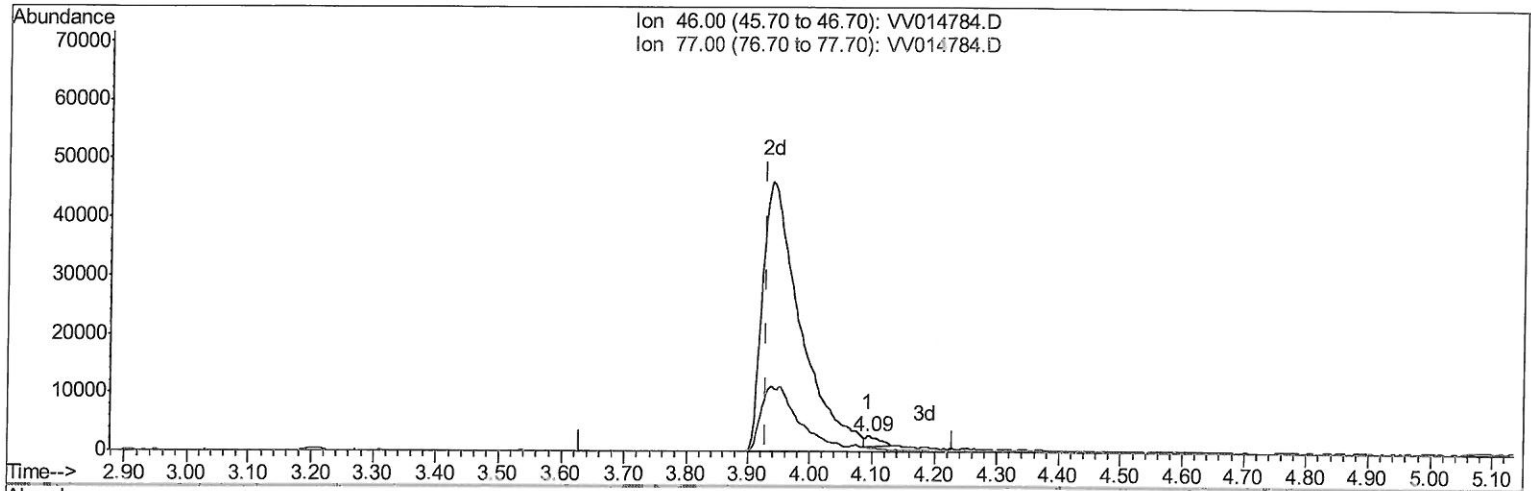

TIC: VV014784.D

(21) 2-Butanone-d5 (S)
 4.093min (+0.164) 1.29ug/L
 response 2740

Ion	Exp%	Act%
46.00	100	100
77.00	23.30	22.59
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014784.D
 Acq On : 09 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1835-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0DJ1

Manual Integrations
APPROVED

MMDadoda
 3/11/2020 9:41:39 AM

Quant Time: Mar 10 14:50:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

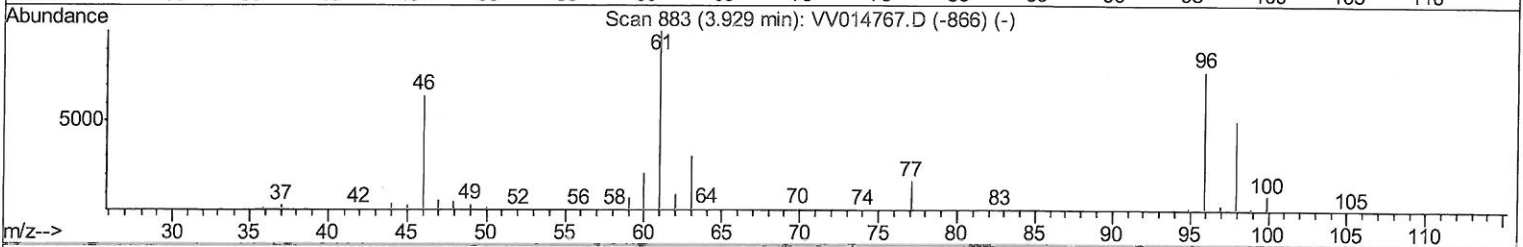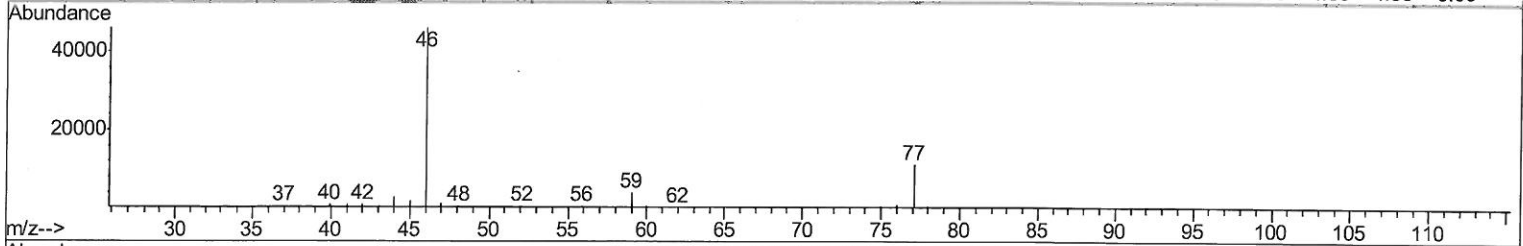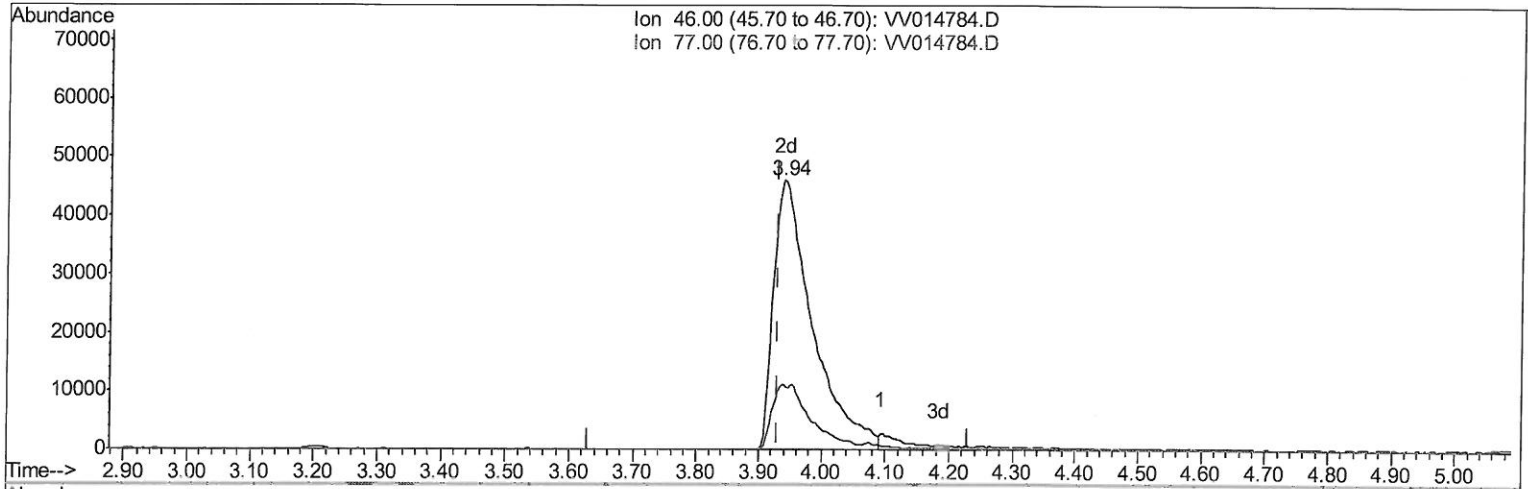

TIC: VV014784.D

(21) 2-Butanone-d5 (S)

3.939min (+0.010) 93.09ug/L m

response 197849

Ion	Exp%	Act%
46.00	100	100
77.00	23.30	0.31#
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
3/11/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014784.D
 Acq On : 09 Mar 2020 18:13
 Operator : SY/MD
 Sample : L1835-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ1

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:39 AM

Quant Time: Mar 10 16:58:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	421092	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	412045	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	203323	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	116525	40.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.78%
7) Chloroethane-d5	1.58	69	98584	43.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.52%
11) 1,1-Dichloroethene-d2	2.12	63	154252	32.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.16%
21) 2-Butanone-d5	3.94	46	197849m	93.09	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.09%
24) Chloroform-d	4.38	84	257483	47.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.44%
26) 1,2-Dichloroethane-d4	5.06	65	169562	46.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.52%
32) Benzene-d6	5.08	84	518284	47.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.28%
36) 1,2-Dichloropropane-d6	6.10	67	162920	45.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.36%
41) Toluene-d8	7.34	98	491389	46.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.24%
43) trans-1,3-Dichloropropene-	7.64	79	70342	39.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.90%
47) 2-Hexanone-d5	8.12	63	159302	99.50	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.50%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	225208	45.40	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	197694	49.06	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.12%

Target Compounds

					Qvalue
51) Chlorobenzene	8.90	112	7312	0.86	ug/L 94
63) 1,4-Dichlorobenzene	11.29	146	10989	1.66	ug/L 95
65) 1,2-Dichlorobenzene	11.67	146	8784	1.34	ug/L 92
68) 1,2,4-trichlorobenzene	13.29	180	3430	0.73	ug/L 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed