

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014769.D
 Acq On : 09 Mar 2020 12:17
 Operator : SY/MD
 Sample : L1834-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	91	rVB	211892	224981	14.11%	1.812%
2	1.579	145	152	166	rVB	154044	187991	11.79%	1.514%
3	2.119	310	320	333	rBV	324320	463420	29.07%	3.731%
4	2.981	585	588	589	rBV2	587	361	0.02%	0.003%
5	3.032	602	604	605	rBV2	305	119	0.01%	0.001%
6	3.077	617	618	621	rBV2	431	190	0.01%	0.002%
7	3.393	712	716	719	rVB2	555	488	0.03%	0.004%
8	3.409	719	721	722	rBV	479	226	0.01%	0.002%
9	3.421	722	725	728	rVV2	875	580	0.04%	0.005%
10	3.438	728	730	734	rVB3	660	396	0.02%	0.003%
11	3.483	742	744	746	rBV2	385	255	0.02%	0.002%
12	3.701	810	812	814	rBV2	658	359	0.02%	0.003%
13	3.765	829	832	834	rBV3	705	427	0.03%	0.003%
14	3.933	870	884	924	rBV3	91172	445652	27.96%	3.588%
15	4.376	1006	1022	1047	rVB	240446	615120	38.59%	4.953%
16	4.643	1102	1105	1106	rBV2	906	433	0.03%	0.003%
17	4.814	1156	1158	1160	rBV2	607	309	0.02%	0.002%
18	4.859	1167	1172	1178	rBV4	1178	1260	0.08%	0.010%
19	4.884	1178	1180	1183	rVB2	750	370	0.02%	0.003%
20	4.958	1199	1203	1206	rBV4	484	413	0.03%	0.003%
21	5.000	1214	1216	1219	rVB2	537	217	0.01%	0.002%
22	5.071	1219	1238	1268	rBV2	637807	1593933	100.00%	12.834%
23	5.338	1319	1321	1322	rBV2	819	368	0.02%	0.003%
24	5.463	1356	1360	1364	rVB6	1217	991	0.06%	0.008%
25	5.534	1380	1382	1385	rBV2	743	432	0.03%	0.003%
26	5.640	1402	1415	1435	rBV	522176	1020288	64.01%	8.215%
27	6.000	1522	1527	1530	rBV3	629	581	0.04%	0.005%
28	6.032	1536	1537	1539	rBV	417	229	0.01%	0.002%
29	6.093	1541	1556	1586	rVV	351407	715761	44.91%	5.763%
30	6.447	1664	1666	1668	rBV3	684	380	0.02%	0.003%
31	6.482	1675	1677	1681	rBV2	736	423	0.03%	0.003%
32	6.502	1681	1683	1685	rVB	355	112	0.01%	0.001%
33	6.540	1693	1695	1696	rBV	211	63	0.00%	0.001%
34	6.556	1696	1700	1707	rVB5	646	818	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014769.D
 Acq On : 09 Mar 2020 12:17
 Operator : SY/MD
 Sample : L1834-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.585	1707	1709	1711	rBV3	673	362	0.02%	0.003%
36	6.614	1715	1718	1719	rBV2	565	300	0.02%	0.002%
37	6.701	1743	1745	1746	rBV	538	248	0.02%	0.002%
38	6.762	1759	1764	1767	rBV3	661	825	0.05%	0.007%
39	6.852	1790	1792	1793	rBV3	533	208	0.01%	0.002%
40	6.865	1794	1796	1798	rVV2	509	276	0.02%	0.002%
41	7.007	1827	1840	1861	rBV	212537	380275	23.86%	3.062%
42	7.338	1929	1943	1962	rBV	783287	1366258	85.72%	11.001%
43	7.543	2005	2007	2009	rBV2	613	242	0.02%	0.002%
44	7.640	2026	2037	2059	rBV	152339	257567	16.16%	2.074%
45	7.839	2095	2099	2100	rBV2	762	554	0.03%	0.004%
46	7.849	2100	2102	2106	rVB3	1061	549	0.03%	0.004%
47	7.871	2106	2109	2113	rBV2	611	441	0.03%	0.004%
48	7.958	2128	2136	2151	rVB2	10246	19819	1.24%	0.160%
49	8.064	2167	2169	2172	rVB2	944	386	0.02%	0.003%
50	8.116	2172	2185	2217	rBV	364019	747933	46.92%	6.022%
51	8.392	2269	2271	2273	rBV	646	292	0.02%	0.002%
52	8.682	2359	2361	2365	rBV2	566	293	0.02%	0.002%
53	8.797	2395	2397	2400	rBV3	518	278	0.02%	0.002%
54	8.830	2403	2407	2408	rBV4	819	501	0.03%	0.004%
55	8.875	2408	2421	2422	rBV	867277	994285	62.38%	8.006%
56	9.450	2598	2600	2601	rBV2	698	285	0.02%	0.002%
57	9.502	2613	2616	2619	rBV2	646	428	0.03%	0.003%
58	9.534	2625	2626	2628	rBV2	373	177	0.01%	0.001%
59	9.553	2628	2632	2633	rBV2	622	414	0.03%	0.003%
60	9.797	2704	2708	2710	rBV2	398	381	0.02%	0.003%
61	10.067	2790	2792	2794	rBV	396	211	0.01%	0.002%
62	10.138	2812	2814	2815	rBV	515	239	0.01%	0.002%
63	10.238	2832	2845	2862	rBV	475408	750684	47.10%	6.045%
64	10.405	2887	2897	2906	rBV2	17025	27185	1.71%	0.219%
65	10.476	2918	2919	2923	rVB3	908	467	0.03%	0.004%
66	10.518	2929	2932	2933	rBV	496	302	0.02%	0.002%
67	10.675	2978	2981	2985	rBV2	735	601	0.04%	0.005%
68	10.836	3029	3031	3035	rBV3	646	372	0.02%	0.003%
69	10.923	3054	3058	3059	rBV	994	706	0.04%	0.006%
70	11.038	3092	3094	3096	rBV	717	253	0.02%	0.002%
71	11.270	3154	3166	3189	rBV	844091	1325947	83.19%	10.677%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014769.D
Acq On : 09 Mar 2020 12:17
Operator : SY/MD
Sample : L1834-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Title : VOC Analysis

72	11.524	3242	3245	3246	rBV	713	415	0.03%	0.003%
73	11.646	3271	3283	3302	rBV	801892	1257007	78.86%	10.122%
74	11.791	3326	3328	3331	rBV4	1016	652	0.04%	0.005%
75	12.042	3403	3406	3409	rBV4	767	662	0.04%	0.005%
76	12.119	3428	3430	3432	rBV	723	382	0.02%	0.003%
77	12.518	3552	3554	3557	rBV2	610	360	0.02%	0.003%
78	13.810	3952	3956	3959	rBV4	1255	1186	0.07%	0.010%


Sum of corrected areas: 12419154

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014769.D
Acq On : 09 Mar 2020 12:17
Operator : SY/MD
Sample : L1834-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

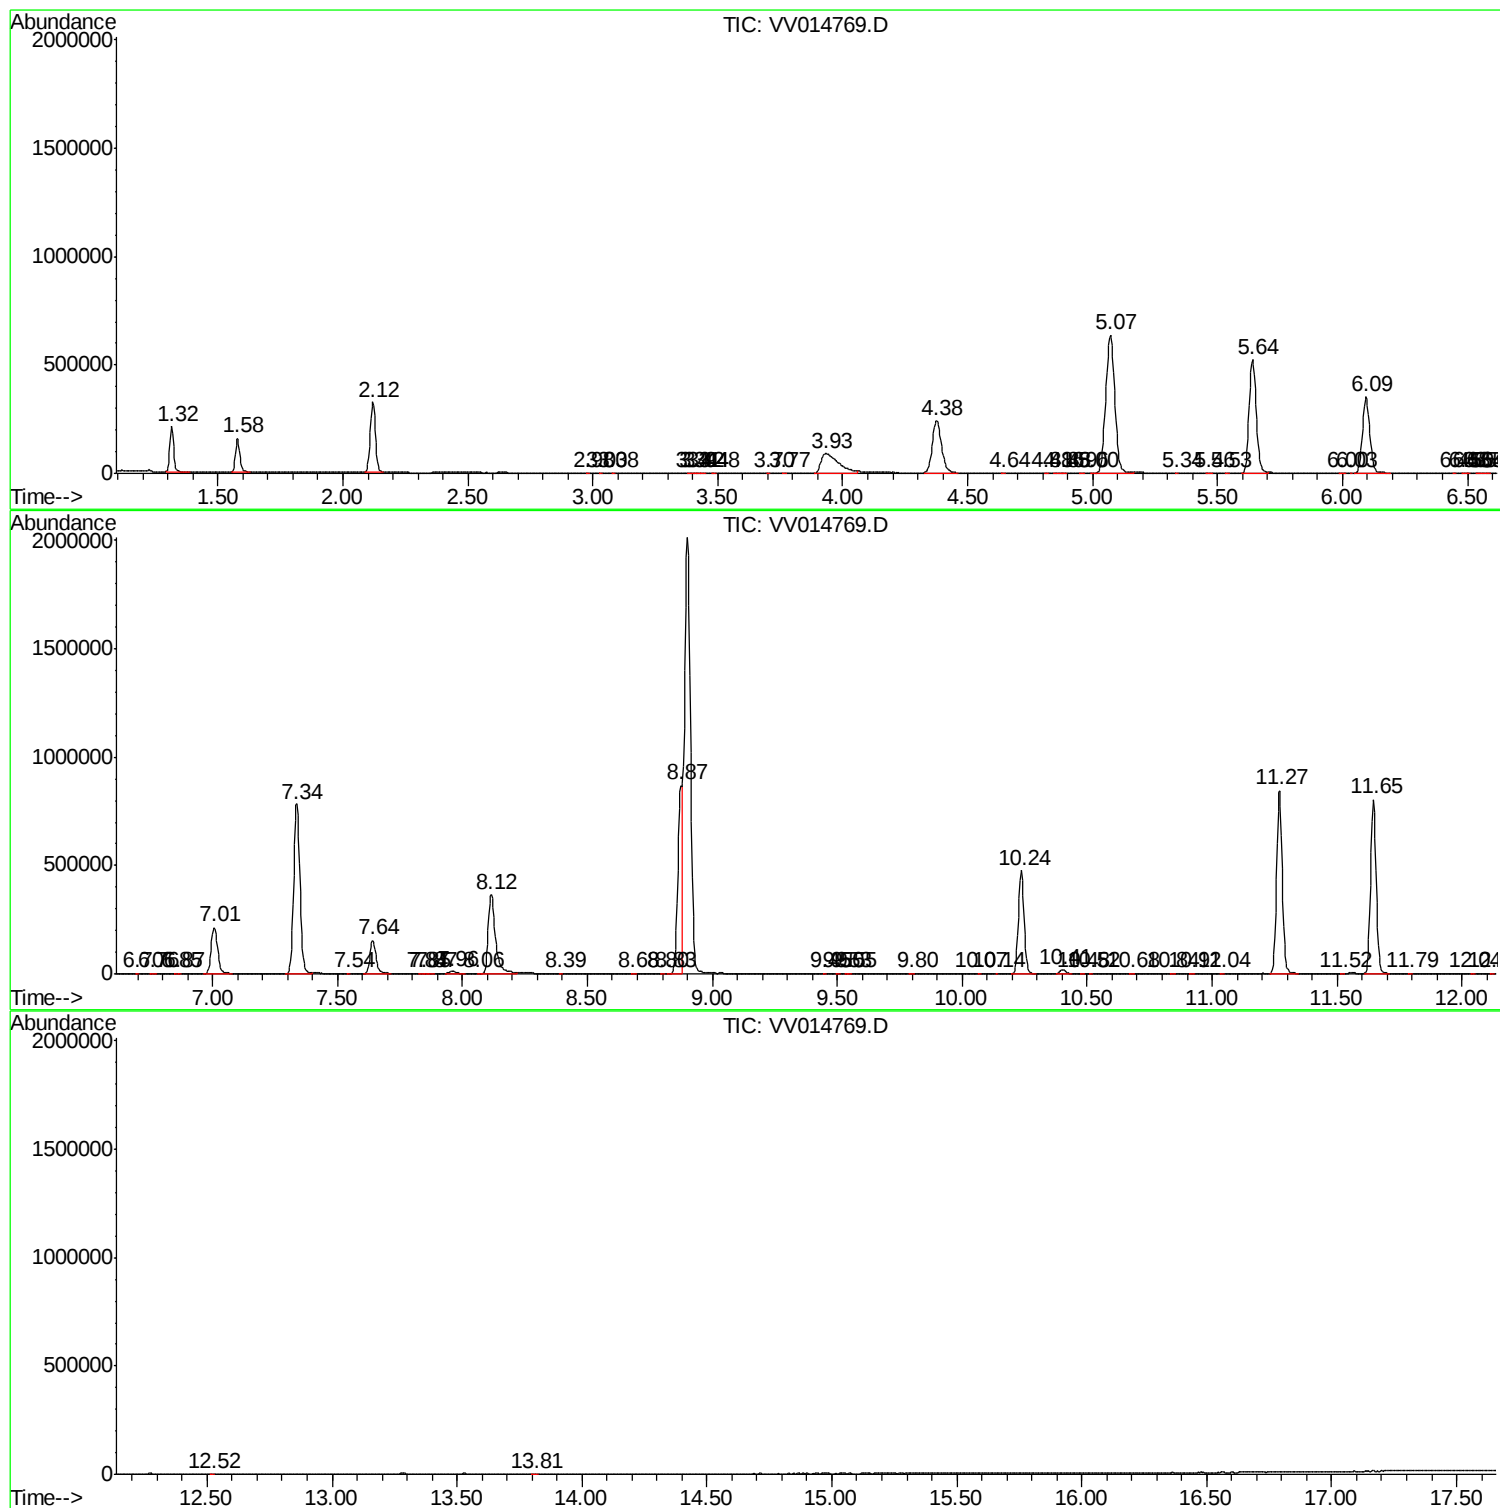

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014769.D
Acq On : 09 Mar 2020 12:17
Operator : SY/MD
Sample : L1834-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014769.D
Acq On : 09 Mar 2020 12:17
Operator : SY/MD
Sample : L1834-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc