

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014771.D
 Acq On : 09 Mar 2020 13:03
 Operator : SY/MD
 Sample : L1834-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	194274	208506	12.50%	1.635%
2	1.579	145	152	167	rVB	150862	179945	10.78%	1.411%
3	2.119	311	320	335	rBV	297803	424868	25.46%	3.332%
4	2.740	511	513	518	rBV4	845	569	0.03%	0.004%
5	2.878	553	556	558	rBV3	680	462	0.03%	0.004%
6	2.913	563	567	570	rBV2	707	610	0.04%	0.005%
7	2.955	576	580	586	rBV6	737	794	0.05%	0.006%
8	2.987	587	590	592	rBV2	802	459	0.03%	0.004%
9	3.151	635	641	644	rBV5	1304	1217	0.07%	0.010%
10	3.190	650	653	656	rVB3	566	393	0.02%	0.003%
11	3.222	660	663	665	rBV2	564	376	0.02%	0.003%
12	3.261	671	675	678	rBV2	654	618	0.04%	0.005%
13	3.299	684	687	689	rBV	395	298	0.02%	0.002%
14	3.476	739	742	746	rBV3	540	402	0.02%	0.003%
15	3.563	767	769	773	rBV2	557	431	0.03%	0.003%
16	3.582	773	775	781	rVB4	992	745	0.04%	0.006%
17	3.614	781	785	788	rBV3	614	588	0.04%	0.005%
18	3.634	788	791	797	rVB5	762	776	0.05%	0.006%
19	3.695	809	810	814	rVV3	476	283	0.02%	0.002%
20	3.733	819	822	825	rBV4	923	522	0.03%	0.004%
21	3.782	830	837	841	rBV7	1280	1472	0.09%	0.012%
22	3.801	841	843	847	rVB3	521	285	0.02%	0.002%
23	3.878	865	867	869	rBV	651	366	0.02%	0.003%
24	3.936	873	885	928	rVV	80295	322088	19.30%	2.526%
25	4.290	992	995	996	rBV2	625	373	0.02%	0.003%
26	4.380	1008	1023	1047	rBV	222512	579036	34.70%	4.541%
27	4.708	1121	1125	1131	rVB6	921	801	0.05%	0.006%
28	4.756	1135	1140	1142	rBV3	813	754	0.05%	0.006%
29	4.823	1158	1161	1164	rBV2	676	549	0.03%	0.004%
30	4.843	1165	1167	1170	rVV3	994	580	0.03%	0.005%
31	5.074	1221	1239	1248	rBV2	611158	1506681	90.29%	11.817%
32	5.524	1377	1379	1383	rBV3	604	359	0.02%	0.003%
33	5.643	1401	1416	1438	rBV	447166	894064	53.58%	7.012%
34	5.807	1464	1467	1471	rBV4	1498	1043	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014771.D
 Acq On : 09 Mar 2020 13:03
 Operator : SY/MD
 Sample : L1834-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	5.849	1477	1480	1482	rBV	747	474	0.03%	0.004%
36	5.900	1494	1496	1498	rBV3	599	295	0.02%	0.002%
37	6.026	1533	1535	1538	rBV3	607	347	0.02%	0.003%
38	6.097	1542	1557	1581	rBV	336106	681395	40.84%	5.344%
39	6.302	1619	1621	1623	rBV3	869	446	0.03%	0.003%
40	6.351	1634	1636	1640	rVB3	744	444	0.03%	0.003%
41	6.453	1666	1668	1670	rBV2	575	298	0.02%	0.002%
42	6.479	1675	1676	1679	rVV2	794	332	0.02%	0.003%
43	6.502	1681	1683	1686	rBV2	421	279	0.02%	0.002%
44	6.608	1715	1716	1718	rVB2	931	300	0.02%	0.002%
45	6.627	1719	1722	1723	rBV2	845	411	0.02%	0.003%
46	6.643	1724	1727	1729	rBV4	1126	670	0.04%	0.005%
47	6.695	1741	1743	1746	rVB3	800	440	0.03%	0.003%
48	6.756	1759	1762	1763	rBV2	663	330	0.02%	0.003%
49	6.836	1785	1787	1790	rVB4	980	494	0.03%	0.004%
50	6.875	1796	1799	1800	rBV	518	333	0.02%	0.003%
51	6.910	1805	1810	1812	rBV4	821	602	0.04%	0.005%
52	6.939	1816	1819	1822	rVB3	686	427	0.03%	0.003%
53	7.010	1828	1841	1862	rBV	199204	358517	21.49%	2.812%
54	7.174	1886	1892	1896	rBV8	1718	2042	0.12%	0.016%
55	7.338	1930	1943	1963	rBV	741402	1285229	77.02%	10.080%
56	7.643	2027	2038	2058	rVV	142611	241160	14.45%	1.891%
57	7.910	2119	2121	2126	rBV2	567	543	0.03%	0.004%
58	7.965	2126	2138	2148	rVV2	7211	13163	0.79%	0.103%
59	8.116	2173	2185	2218	rBV	381027	779992	46.74%	6.117%
60	8.424	2279	2281	2285	rBV4	831	650	0.04%	0.005%
61	8.498	2301	2304	2312	rBV6	989	949	0.06%	0.007%
62	8.633	2344	2346	2352	rBV5	431	411	0.02%	0.003%
63	8.807	2394	2400	2406	rBV4	905	1128	0.07%	0.009%
64	8.875	2409	2421	2424	rBV	735101	1055899	63.28%	8.281%
65	9.206	2521	2524	2526	rVB	780	354	0.02%	0.003%
66	9.424	2590	2592	2594	rBV2	626	306	0.02%	0.002%
67	9.457	2599	2602	2606	rBV3	654	577	0.03%	0.005%
68	9.559	2627	2634	2640	rBV6	901	1230	0.07%	0.010%
69	9.781	2701	2703	2708	rVB3	398	297	0.02%	0.002%
70	9.807	2709	2711	2714	rBV3	520	309	0.02%	0.002%
71	9.929	2746	2749	2750	rBV3	661	357	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014771.D
 Acq On : 09 Mar 2020 13:03
 Operator : SY/MD
 Sample : L1834-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.955	2755	2757	2759	rBV	805	331	0.02%	0.003%
73	10.170	2822	2824	2829	rVB	779	550	0.03%	0.004%
74	10.238	2833	2845	2861	rVV	472953	741468	44.44%	5.815%
75	10.331	2871	2874	2878	rBV3	670	569	0.03%	0.004%
76	10.402	2889	2896	2906	rVB2	10725	15681	0.94%	0.123%
77	10.530	2934	2936	2940	rVV3	800	473	0.03%	0.004%
78	10.556	2942	2944	2946	rVV2	796	379	0.02%	0.003%
79	10.582	2949	2952	2954	rVB3	654	305	0.02%	0.002%
80	10.621	2962	2964	2967	rBV2	737	473	0.03%	0.004%
81	10.685	2980	2984	2986	rBV2	652	516	0.03%	0.004%
82	10.820	3021	3026	3027	rBV2	559	416	0.02%	0.003%
83	10.926	3054	3059	3060	rBV4	1216	878	0.05%	0.007%
84	11.067	3100	3103	3105	rBV2	475	292	0.02%	0.002%
85	11.090	3107	3110	3111	rBV2	577	304	0.02%	0.002%
86	11.129	3120	3122	3128	rBV3	627	487	0.03%	0.004%
87	11.154	3128	3130	3132	rBV	589	330	0.02%	0.003%
88	11.202	3137	3145	3154	rVV3	30445	46640	2.80%	0.366%
89	11.270	3154	3166	3190	rVV2	777473	1668652	100.00%	13.087%
90	11.399	3204	3206	3207	rBV	866	389	0.02%	0.003%
91	11.646	3271	3283	3306	rBV2	838013	1657347	99.32%	12.998%
92	11.884	3355	3357	3360	rBV4	643	376	0.02%	0.003%
93	11.929	3365	3371	3373	rBV4	949	801	0.05%	0.006%
94	12.045	3404	3407	3409	rBV2	539	445	0.03%	0.003%
95	12.199	3451	3455	3456	rBV	446	303	0.02%	0.002%
96	12.209	3456	3458	3463	rVV3	1051	717	0.04%	0.006%
97	12.370	3502	3508	3513	rBV6	2977	3456	0.21%	0.027%
98	12.884	3663	3668	3673	rBV3	820	1015	0.06%	0.008%
99	13.212	3767	3770	3773	rBV2	774	497	0.03%	0.004%
100	13.283	3784	3792	3806	rVB3	28739	43796	2.62%	0.343%


Sum of corrected areas: 12750629

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014771.D
Acq On : 09 Mar 2020 13:03
Operator : SY/MD
Sample : L1834-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

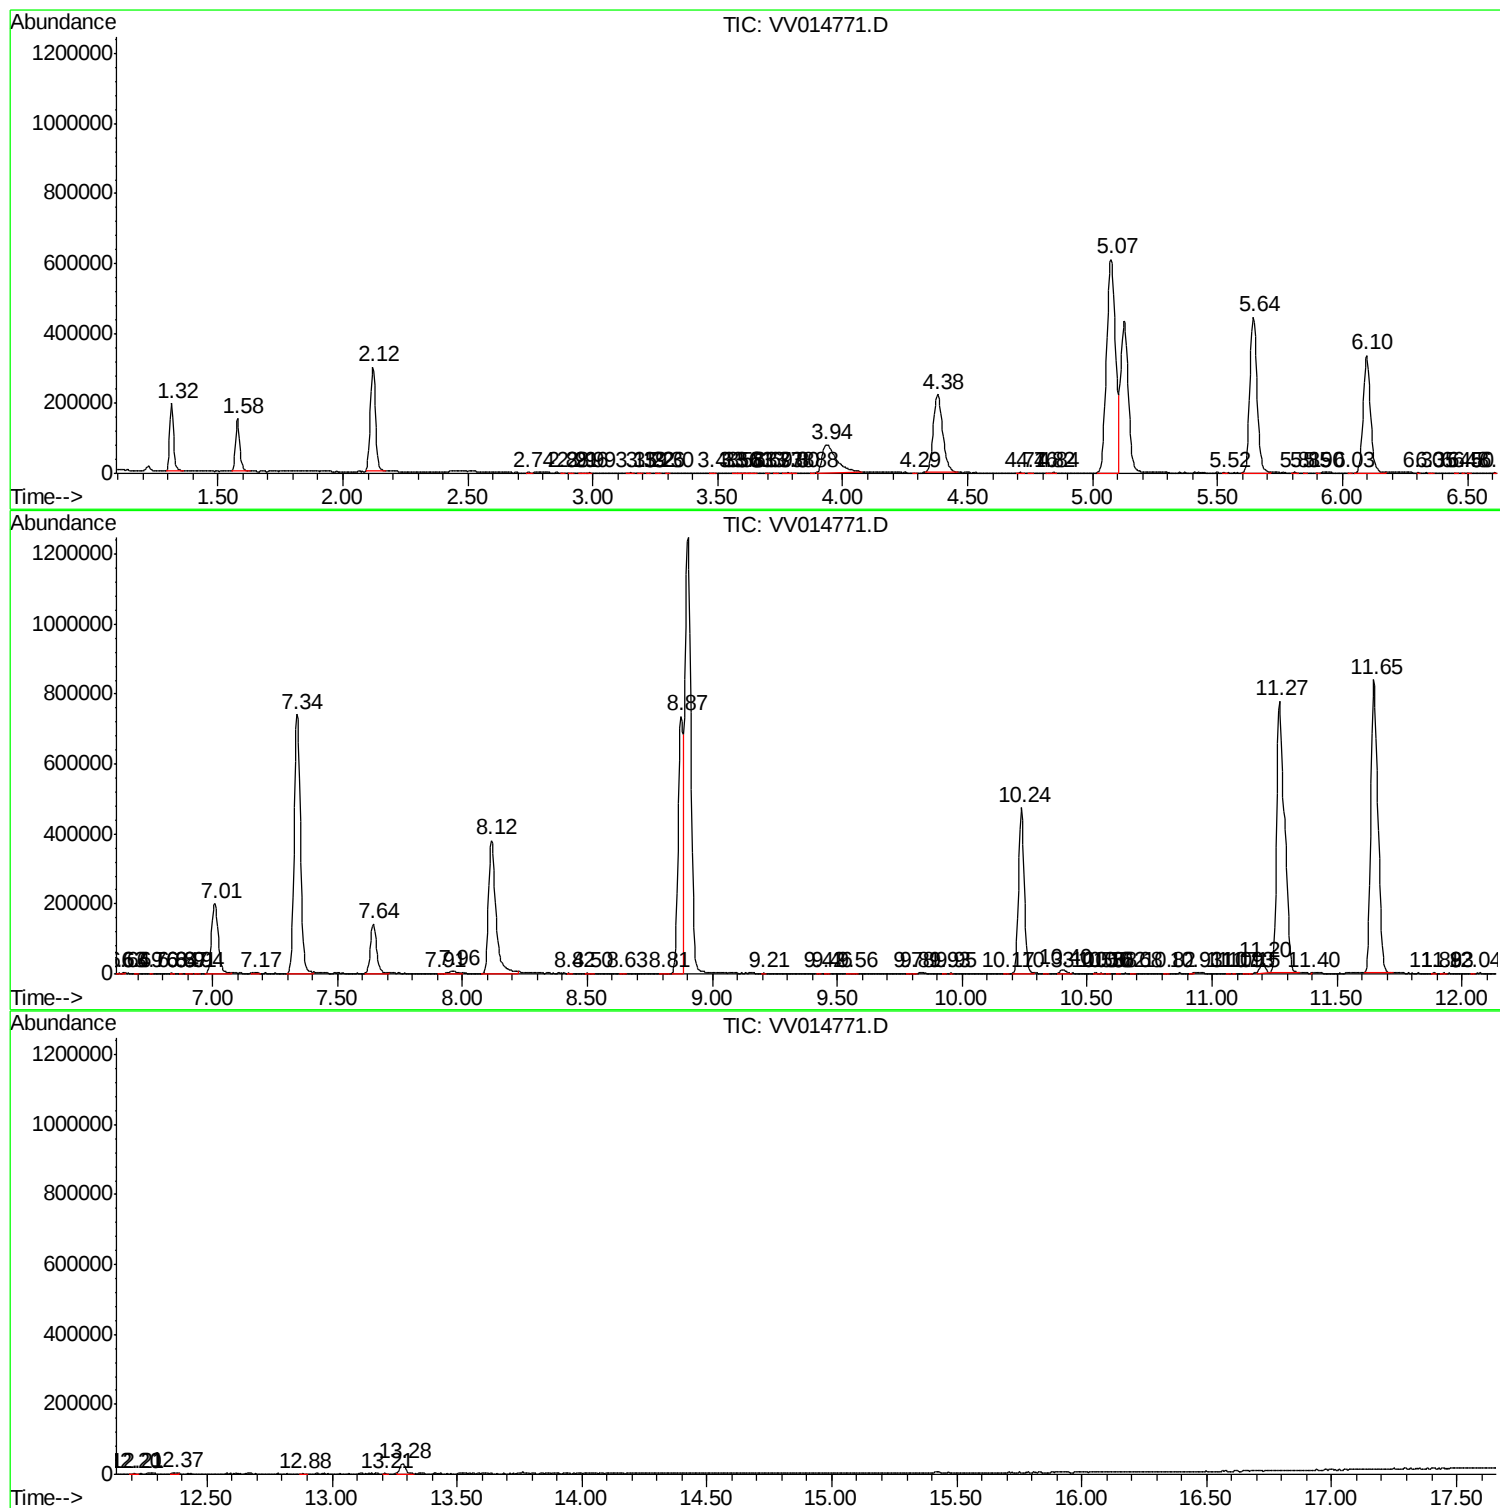

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014771.D
Acq On : 09 Mar 2020 13:03
Operator : SY/MD
Sample : L1834-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014771.D
Acq On : 09 Mar 2020 13:03
Operator : SY/MD
Sample : L1834-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc