

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014775.D
 Acq On : 09 Mar 2020 14:36
 Operator : SY/MD
 Sample : L1834-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	84	rVB	195324	205990	0.50%	0.201%
2	1.576	145	151	165	rBV	152075	188708	0.46%	0.184%
3	2.119	311	320	338	rVB	322537	463516	1.12%	0.453%
4	2.949	576	578	582	rBV3	685	375	0.00%	0.000%
5	3.010	595	597	600	rBV	437	231	0.00%	0.000%
6	3.106	625	627	630	rVB2	459	251	0.00%	0.000%
7	3.132	631	635	637	rBV2	734	482	0.00%	0.000%
8	3.148	637	640	642	rBV3	373	217	0.00%	0.000%
9	3.167	644	646	648	rBV2	628	319	0.00%	0.000%
10	3.341	696	700	702	rBV3	644	445	0.00%	0.000%
11	3.360	702	706	709	rBV3	591	298	0.00%	0.000%
12	3.380	709	712	714	rBV2	567	269	0.00%	0.000%
13	3.434	724	729	731	rVB2	916	670	0.00%	0.001%
14	3.460	734	737	738	rBV2	594	280	0.00%	0.000%
15	3.499	746	749	751	rBV2	633	377	0.00%	0.000%
16	3.524	754	757	759	rVV2	452	285	0.00%	0.000%
17	3.540	761	762	766	rVB3	738	444	0.00%	0.000%
18	3.566	766	770	774	rVB5	629	517	0.00%	0.001%
19	3.602	779	781	787	rVB5	828	665	0.00%	0.001%
20	3.650	795	796	798	rBV	488	238	0.00%	0.000%
21	3.737	820	823	824	rBV2	740	354	0.00%	0.000%
22	3.878	864	867	871	rBV	789	712	0.00%	0.001%
23	3.930	871	883	921	rBV	86915	341115	0.82%	0.333%
24	4.380	1007	1023	1053	rVB2	254044	691203	1.67%	0.675%
25	4.692	1112	1120	1122	rBV8	2091	2047	0.00%	0.002%
26	4.856	1158	1171	1183	rBV3	9471	22142	0.05%	0.022%
27	4.929	1192	1194	1196	rBV3	391	256	0.00%	0.000%
28	4.971	1203	1207	1208	rBV3	609	451	0.00%	0.000%
29	5.074	1218	1239	1244	rBV2	652046	1435812	3.47%	1.403%
30	5.547	1381	1386	1389	rBV5	1339	1309	0.00%	0.001%
31	5.643	1402	1416	1439	rBV	488979	960012	2.32%	0.938%
32	5.865	1482	1485	1489	rBV4	731	539	0.00%	0.001%
33	5.884	1489	1491	1493	rBV3	722	259	0.00%	0.000%
34	5.974	1517	1519	1521	rVB	573	259	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014775.D
 Acq On : 09 Mar 2020 14:36
 Operator : SY/MD
 Sample : L1834-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.097	1542	1557	1574	rBV	356098	716221	1.73%	0.700%
36	6.341	1631	1633	1636	rBV3	574	428	0.00%	0.000%
37	6.370	1640	1642	1643	rBV	469	196	0.00%	0.000%
38	6.550	1696	1698	1702	rVB4	1028	678	0.00%	0.001%
39	6.579	1702	1707	1710	rVB5	949	621	0.00%	0.001%
40	6.601	1710	1714	1715	rBV3	559	359	0.00%	0.000%
41	6.743	1756	1758	1760	rBV	453	216	0.00%	0.000%
42	6.753	1760	1761	1763	rVV2	535	224	0.00%	0.000%
43	6.794	1772	1774	1776	rBV2	562	284	0.00%	0.000%
44	6.823	1780	1783	1785	rBV4	625	362	0.00%	0.000%
45	6.910	1807	1810	1813	rBV4	982	677	0.00%	0.001%
46	6.949	1820	1822	1826	rBV3	503	260	0.00%	0.000%
47	7.010	1828	1841	1859	rBV	204159	365379	0.88%	0.357%
48	7.338	1927	1943	1961	rBV	804172	1383049	3.34%	1.351%
49	7.518	1997	1999	2003	rBV2	876	823	0.00%	0.001%
50	7.569	2014	2015	2022	rVB6	651	522	0.00%	0.001%
51	7.643	2027	2038	2060	rVV	143685	242441	0.59%	0.237%
52	7.888	2110	2114	2119	rBV2	631	804	0.00%	0.001%
53	7.910	2119	2121	2124	rVB2	406	202	0.00%	0.000%
54	7.958	2131	2136	2139	rBV3	1961	2271	0.01%	0.002%
55	8.116	2173	2185	2214	rBV	403686	806075	1.95%	0.788%
56	8.437	2283	2285	2287	rBV2	515	213	0.00%	0.000%
57	8.572	2322	2327	2328	rBV3	559	351	0.00%	0.000%
58	8.614	2338	2340	2343	rVB2	687	351	0.00%	0.000%
59	8.669	2354	2357	2360	rBV2	493	258	0.00%	0.000%
60	8.727	2373	2375	2376	rBV2	547	231	0.00%	0.000%
61	8.762	2384	2386	2390	rVB3	653	417	0.00%	0.000%
62	8.904	2406	2430	2466	rBV	10051255	17151887	41.46%	16.758%
63	9.241	2533	2535	2537	rBV3	880	417	0.00%	0.000%
64	9.399	2582	2584	2587	rBV2	632	351	0.00%	0.000%
65	9.527	2622	2624	2627	rBV2	643	497	0.00%	0.000%
66	9.624	2650	2654	2656	rBV2	691	595	0.00%	0.001%
67	9.752	2689	2694	2702	rVB6	1703	2074	0.01%	0.002%
68	9.785	2702	2704	2707	rBV	398	265	0.00%	0.000%
69	9.881	2731	2734	2739	rVB3	843	685	0.00%	0.001%
70	9.907	2739	2742	2744	rBV2	410	256	0.00%	0.000%
71	9.977	2762	2764	2766	rBV	388	224	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014775.D
 Acq On : 09 Mar 2020 14:36
 Operator : SY/MD
 Sample : L1834-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.039	2780	2783	2787	rVB3	1015	660	0.00%	0.001%
73	10.058	2787	2789	2791	rBV2	1013	486	0.00%	0.000%
74	10.090	2797	2799	2800	rBV2	601	236	0.00%	0.000%
75	10.238	2832	2845	2861	rBV	506649	790087	1.91%	0.772%
76	10.363	2882	2884	2888	rVB	618	322	0.00%	0.000%
77	10.402	2888	2896	2902	rBV3	3804	5439	0.01%	0.005%
78	10.637	2967	2969	2973	rVB2	597	350	0.00%	0.000%
79	10.656	2973	2975	2978	rBV2	614	438	0.00%	0.000%
80	10.682	2981	2983	2988	rVB2	596	443	0.00%	0.000%
81	10.781	3011	3014	3016	rBV2	743	476	0.00%	0.000%
82	10.846	3029	3034	3040	rBV3	1507	1573	0.00%	0.002%
83	10.875	3040	3043	3045	rBV	716	553	0.00%	0.001%
84	10.897	3048	3050	3052	rVV	522	264	0.00%	0.000%
85	10.932	3056	3061	3065	rBV5	845	959	0.00%	0.001%
86	10.974	3072	3074	3078	rVB2	605	342	0.00%	0.000%
87	11.003	3078	3083	3085	rBV	555	468	0.00%	0.000%
88	11.138	3122	3125	3127	rVB2	603	291	0.00%	0.000%
89	11.151	3127	3129	3131	rBV2	456	250	0.00%	0.000%
90	11.199	3131	3144	3156	rBV	2340042	3528120	8.53%	3.447%
91	11.296	3157	3174	3201	rVB	14967911	23807730	57.54%	23.261%
92	11.669	3271	3290	3312	rBV	25799021	41373190	100.00%	40.423%
93	12.418	3514	3523	3532	rVB3	15136	23652	0.06%	0.023%
94	12.595	3566	3578	3579	rBV7	3792	5041	0.01%	0.005%
95	12.659	3589	3598	3611	rVB	39098	63487	0.15%	0.062%
96	13.074	3725	3727	3729	rBV3	836	386	0.00%	0.000%
97	13.283	3779	3792	3810	rBV	3568020	5431891	13.13%	5.307%
98	13.765	3929	3942	3960	rBV	1290390	2002743	4.84%	1.957%
99	14.842	4264	4277	4289	rVB2	59212	100890	0.24%	0.099%
100	15.418	4447	4456	4471	rBV2	129455	207423	0.50%	0.203%


Sum of corrected areas: 102350401

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014775.D
Acq On : 09 Mar 2020 14:36
Operator : SY/MD
Sample : L1834-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

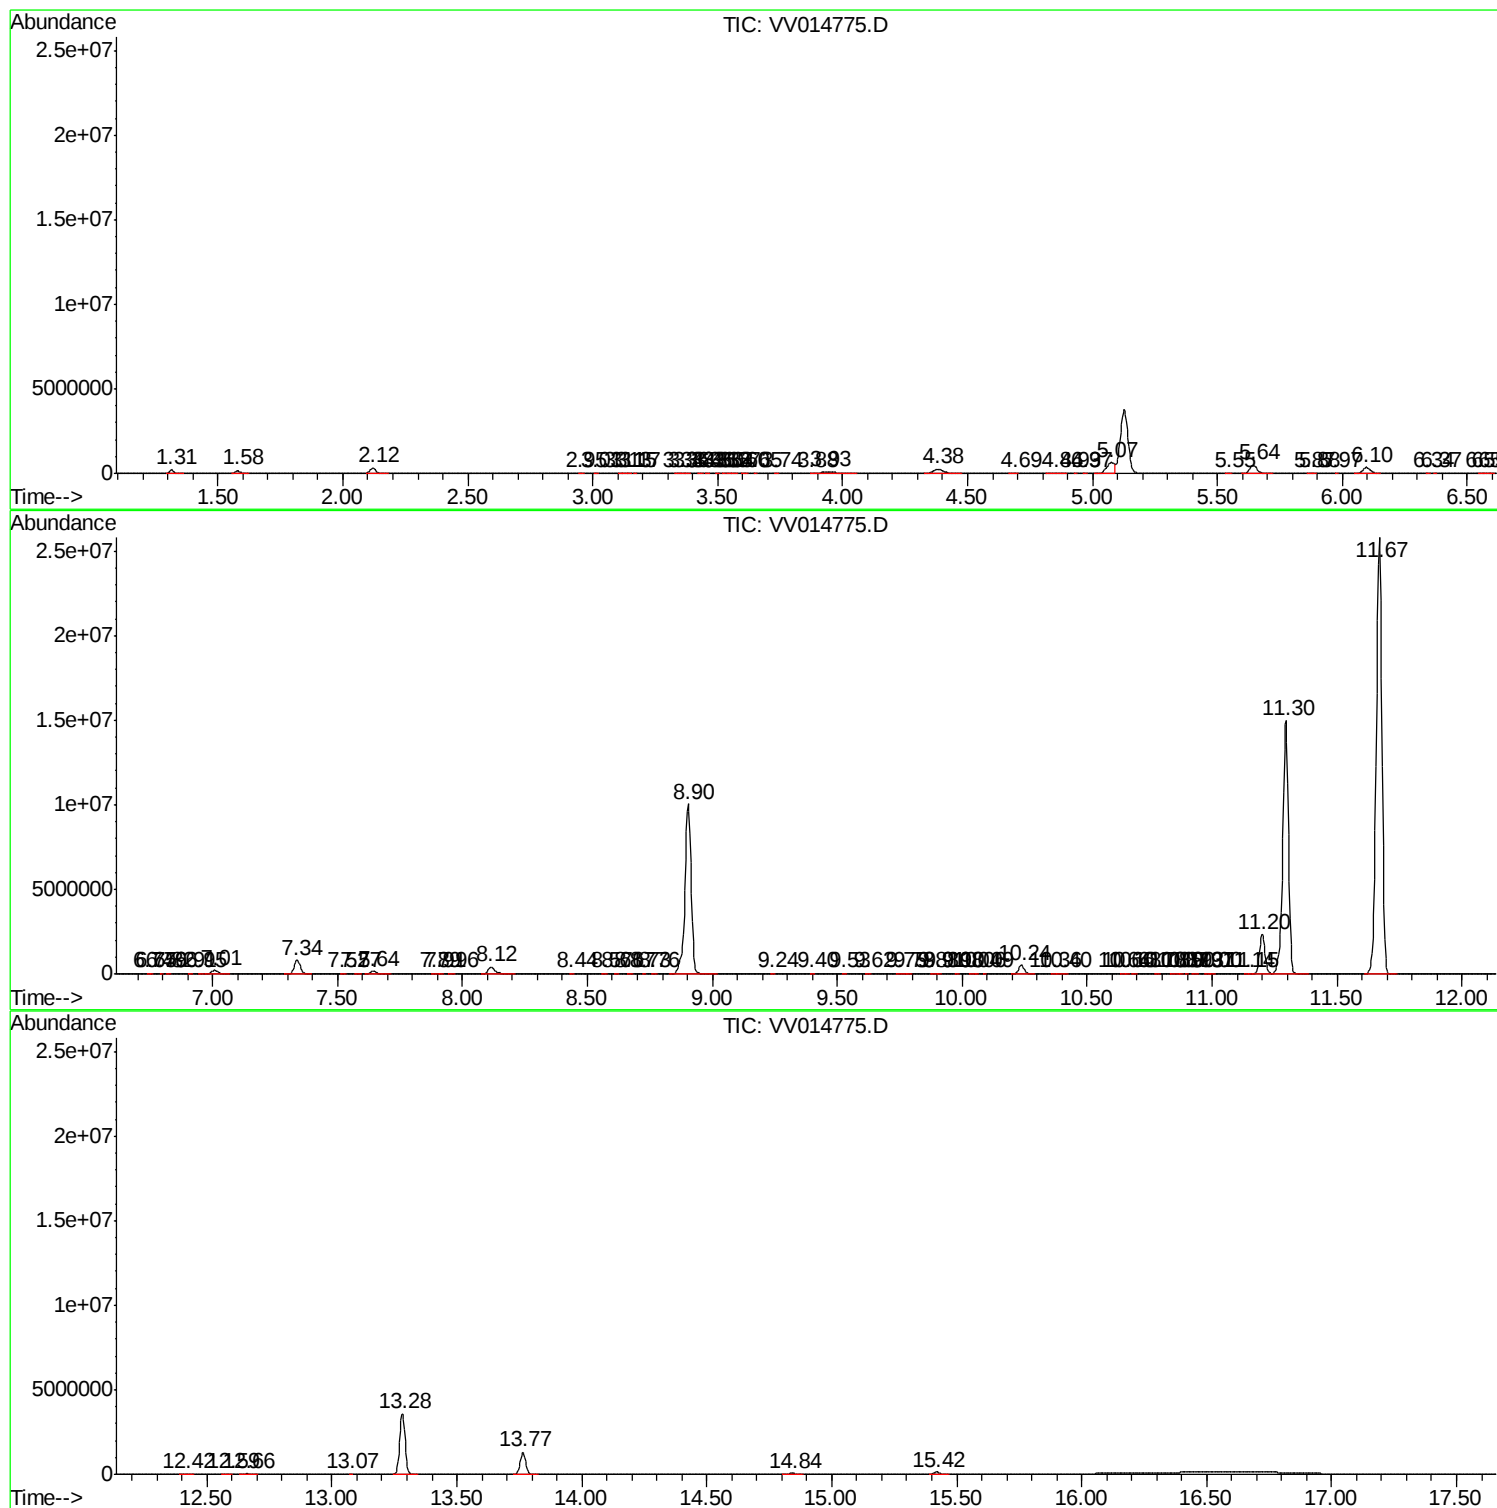

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014775.D
Acq On : 09 Mar 2020 14:36
Operator : SY/MD
Sample : L1834-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014775.D
Acq On : 09 Mar 2020 14:36
Operator : SY/MD
Sample : L1834-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc