

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014776.D
 Acq On : 09 Mar 2020 15:00
 Operator : SY/MD
 Sample : L1834-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	88	rVB	194730	211948	0.49%	0.174%
2	1.579	145	152	171	rVB	155238	190150	0.44%	0.156%
3	2.122	312	321	341	rVB	313951	461403	1.06%	0.378%
4	2.868	550	553	554	rBV2	722	476	0.00%	0.000%
5	2.894	559	561	563	rBV4	572	264	0.00%	0.000%
6	3.013	595	598	601	rBV2	999	635	0.00%	0.001%
7	3.094	622	623	625	rVB2	716	243	0.00%	0.000%
8	3.277	678	680	682	rBV2	475	263	0.00%	0.000%
9	3.386	712	714	717	rBV4	892	488	0.00%	0.000%
10	3.415	719	723	726	rVV2	801	524	0.00%	0.000%
11	3.434	726	729	730	rBV2	410	223	0.00%	0.000%
12	3.479	740	743	744	rBV	551	350	0.00%	0.000%
13	3.563	766	769	775	rBV5	994	959	0.00%	0.001%
14	3.653	793	797	801	rBV2	486	452	0.00%	0.000%
15	3.682	801	806	808	rBV4	777	673	0.00%	0.001%
16	3.695	808	810	812	rBV2	418	232	0.00%	0.000%
17	3.727	817	820	822	rVB	453	230	0.00%	0.000%
18	3.759	828	830	832	rBV	1010	623	0.00%	0.001%
19	3.859	859	861	870	rVB4	1003	807	0.00%	0.001%
20	3.936	871	885	936	rBV2	83982	363184	0.83%	0.297%
21	4.389	1007	1026	1055	rBV4	309812	1073865	2.46%	0.879%
22	4.544	1072	1074	1076	rBV	864	489	0.00%	0.000%
23	4.775	1140	1146	1149	rBV5	1172	1213	0.00%	0.001%
24	4.798	1151	1153	1156	rVB3	819	405	0.00%	0.000%
25	4.859	1156	1172	1188	rBV2	16559	40264	0.09%	0.033%
26	4.949	1198	1200	1202	rBV2	567	295	0.00%	0.000%
27	4.978	1206	1209	1212	rBV2	1145	711	0.00%	0.001%
28	5.077	1221	1240	1243	rBV2	645574	1304258	2.99%	1.068%
29	5.643	1402	1416	1439	rBV	510233	1003130	2.30%	0.821%
30	5.936	1499	1507	1508	rBV6	3246	3524	0.01%	0.003%
31	6.097	1543	1557	1586	rBV	348554	718774	1.65%	0.589%
32	6.383	1644	1646	1647	rBV2	655	232	0.00%	0.000%
33	6.499	1675	1682	1684	rBV6	566	585	0.00%	0.000%
34	6.598	1709	1713	1715	rBV2	412	301	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014776.D
 Acq On : 09 Mar 2020 15:00
 Operator : SY/MD
 Sample : L1834-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.746	1757	1759	1763	rVV3	596	320	0.00%	0.000%
36	6.785	1769	1771	1773	rVB2	694	299	0.00%	0.000%
37	6.801	1773	1776	1778	rBV3	651	441	0.00%	0.000%
38	6.826	1782	1784	1789	rVB3	1352	709	0.00%	0.001%
39	6.881	1798	1801	1803	rBV3	522	322	0.00%	0.000%
40	6.917	1810	1812	1813	rBV2	499	232	0.00%	0.000%
41	6.958	1821	1825	1827	rBV4	620	482	0.00%	0.000%
42	7.010	1829	1841	1860	rVV2	207907	372549	0.85%	0.305%
43	7.254	1914	1917	1919	rBV2	874	447	0.00%	0.000%
44	7.338	1930	1943	1964	rBV	809720	1386764	3.18%	1.136%
45	7.531	2001	2003	2006	rVB3	1297	608	0.00%	0.000%
46	7.553	2006	2010	2012	rBV4	771	556	0.00%	0.000%
47	7.643	2025	2038	2055	rBV	148068	255813	0.59%	0.209%
48	7.801	2085	2087	2090	rVB3	994	527	0.00%	0.000%
49	7.843	2097	2100	2103	rBV4	1022	837	0.00%	0.001%
50	7.994	2143	2147	2148	rBV4	1972	1555	0.00%	0.001%
51	8.039	2157	2161	2165	rVB4	961	780	0.00%	0.001%
52	8.064	2166	2169	2171	rBV2	662	434	0.00%	0.000%
53	8.116	2174	2185	2221	rVV	426832	850855	1.95%	0.697%
54	8.502	2302	2305	2308	rBV3	749	501	0.00%	0.000%
55	8.531	2311	2314	2317	rBV2	531	288	0.00%	0.000%
56	8.543	2317	2318	2322	rVB3	818	493	0.00%	0.000%
57	8.566	2322	2325	2327	rBV3	575	358	0.00%	0.000%
58	8.585	2327	2331	2333	rBV2	546	460	0.00%	0.000%
59	8.617	2337	2341	2342	rBV	406	229	0.00%	0.000%
60	8.646	2347	2350	2351	rBV2	508	318	0.00%	0.000%
61	8.691	2361	2364	2367	rBV3	444	232	0.00%	0.000%
62	8.769	2384	2388	2392	rBV4	841	696	0.00%	0.001%
63	8.785	2392	2393	2397	rVB2	424	287	0.00%	0.000%
64	8.904	2408	2430	2463	rBV	13961387	23448952	53.76%	19.203%
65	9.447	2597	2599	2602	rBV3	794	408	0.00%	0.000%
66	9.511	2617	2619	2626	rVB6	805	474	0.00%	0.000%
67	9.566	2631	2636	2638	rBV3	1444	1342	0.00%	0.001%
68	9.688	2672	2674	2676	rBV3	539	275	0.00%	0.000%
69	9.717	2679	2683	2685	rBV	530	286	0.00%	0.000%
70	9.730	2685	2687	2689	rBV2	688	296	0.00%	0.000%
71	9.752	2689	2694	2696	rBV3	1593	1513	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014776.D
 Acq On : 09 Mar 2020 15:00
 Operator : SY/MD
 Sample : L1834-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.791	2704	2706	2710	rBV2	601	426	0.00%	0.000%
73	9.878	2728	2733	2734	rBV3	485	437	0.00%	0.000%
74	9.932	2746	2750	2752	rBV3	618	446	0.00%	0.000%
75	9.945	2752	2754	2756	rVV	1019	468	0.00%	0.000%
76	9.961	2756	2759	2761	rVB3	612	419	0.00%	0.000%
77	10.103	2798	2803	2804	rBV2	818	545	0.00%	0.000%
78	10.148	2815	2817	2818	rBV	515	214	0.00%	0.000%
79	10.238	2830	2845	2861	rBV	525628	825408	1.89%	0.676%
80	10.402	2889	2896	2904	rBV4	3838	5691	0.01%	0.005%
81	10.498	2923	2926	2929	rBV2	1141	719	0.00%	0.001%
82	10.611	2959	2961	2965	rBV3	823	559	0.00%	0.000%
83	10.640	2968	2970	2974	rVB2	520	273	0.00%	0.000%
84	10.659	2974	2976	2981	rVB4	481	367	0.00%	0.000%
85	10.772	3009	3011	3014	rBV2	600	286	0.00%	0.000%
86	10.788	3014	3016	3021	rVB3	788	496	0.00%	0.000%
87	10.830	3025	3029	3030	rBV2	666	519	0.00%	0.000%
88	10.900	3049	3051	3055	rBV	574	499	0.00%	0.000%
89	11.006	3082	3084	3086	rBV3	445	256	0.00%	0.000%
90	11.203	3128	3145	3157	rBV	4364319	6651026	15.25%	5.447%
91	11.296	3157	3174	3201	rVB	18644254	29113428	66.75%	23.842%
92	11.669	3271	3290	3309	rBV	27438414	43618236	100.00%	35.720%
93	12.418	3513	3523	3536	rVB2	27269	43151	0.10%	0.035%
94	12.659	3587	3598	3615	rBV	200863	323575	0.74%	0.265%
95	13.013	3704	3708	3711	rBV5	2209	2125	0.00%	0.002%
96	13.112	3734	3739	3749	rVB8	6819	9873	0.02%	0.008%
97	13.283	3778	3792	3813	rBV	4233701	6473195	14.84%	5.301%
98	13.765	3928	3942	3961	rBV	2006327	3111031	7.13%	2.548%
99	14.170	4060	4068	4081	rVB3	37199	60178	0.14%	0.049%
100	15.418	4447	4456	4471	rVB	98714	154033	0.35%	0.126%


Sum of corrected areas: 122111990

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014776.D
Acq On : 09 Mar 2020 15:00
Operator : SY/MD
Sample : L1834-18
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

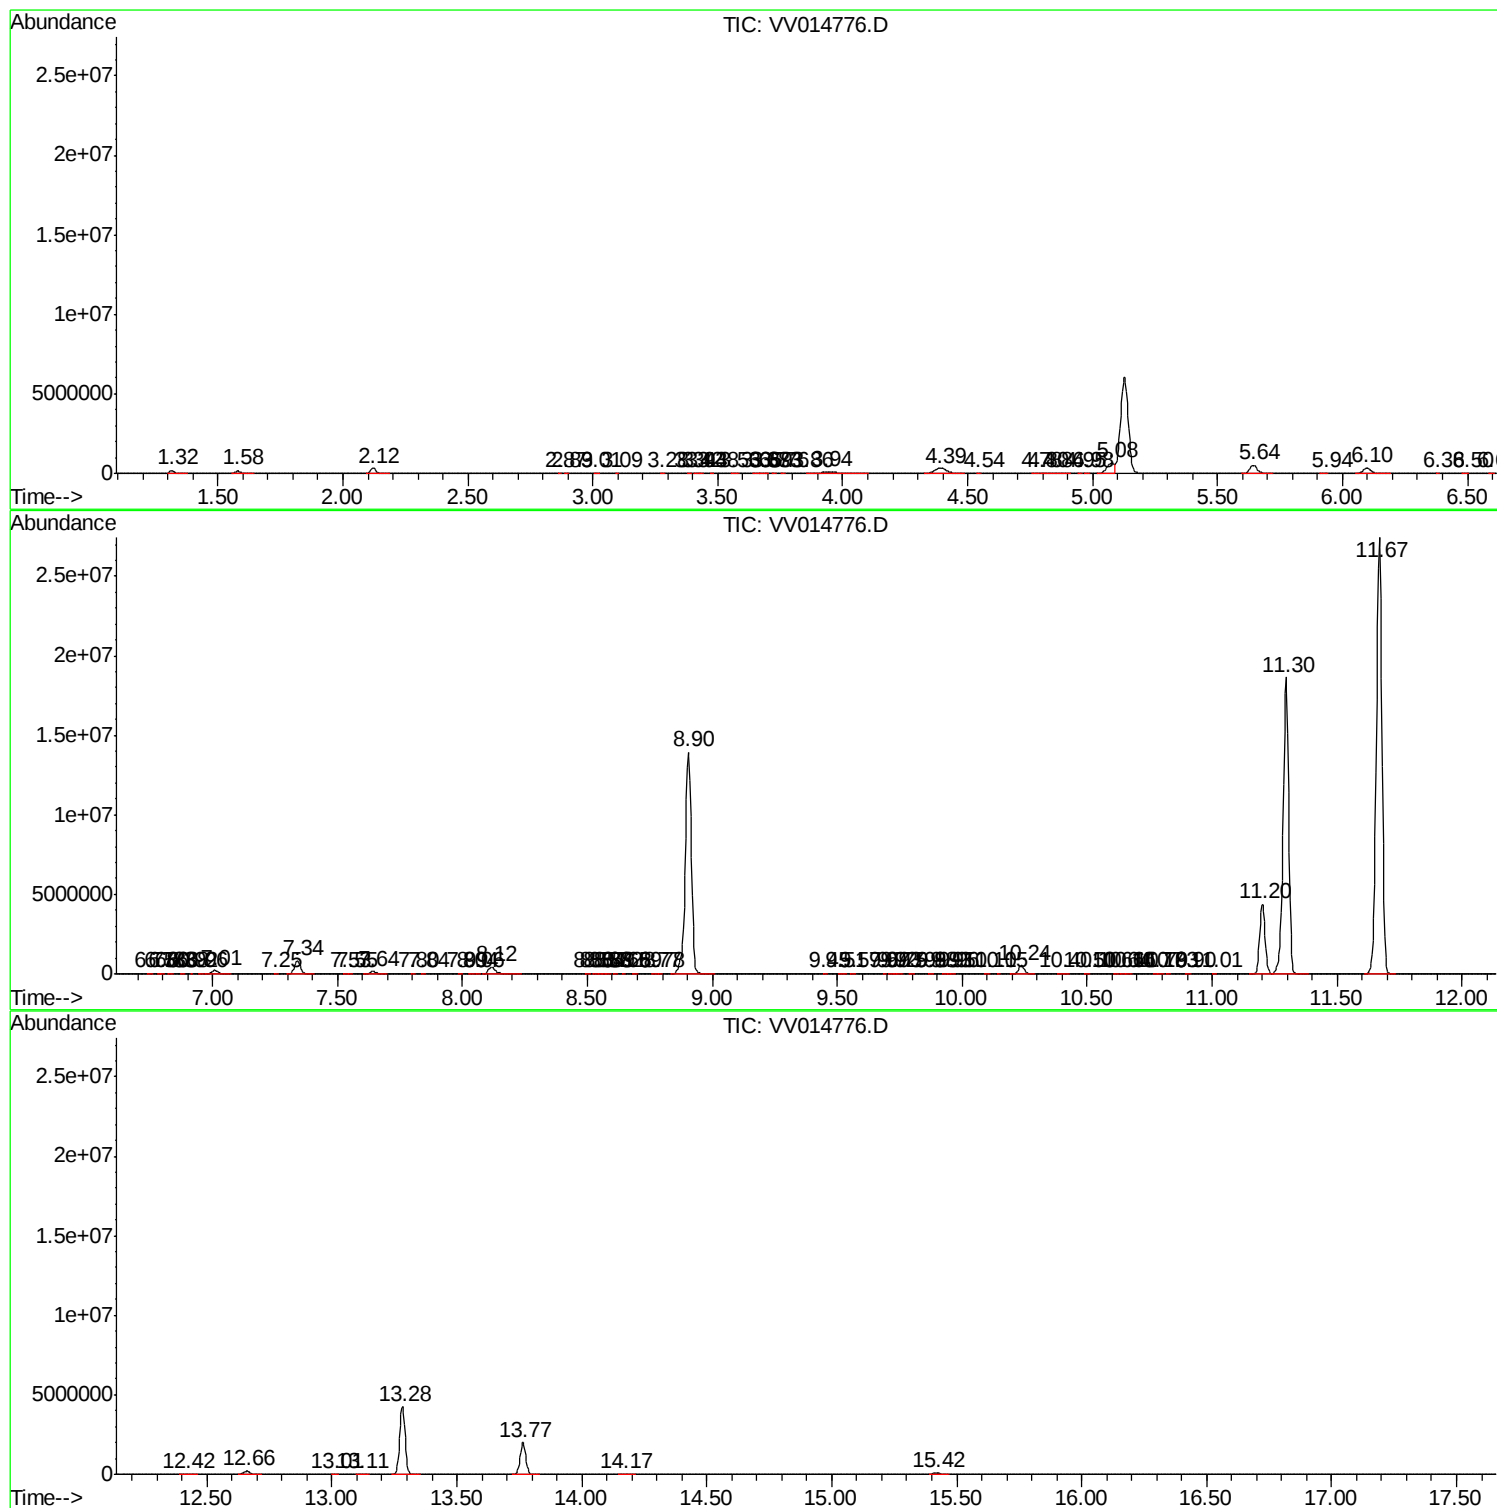

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014776.D
Acq On : 09 Mar 2020 15:00
Operator : SY/MD
Sample : L1834-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014776.D
Acq On : 09 Mar 2020 15:00
Operator : SY/MD
Sample : L1834-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc