

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014779.D
 Acq On : 09 Mar 2020 16:12
 Operator : SY/MD
 Sample : L1835-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	190585	205519	12.99%	1.633%
2	1.579	145	152	173	rVB	148463	190376	12.03%	1.512%
3	2.119	311	320	338	rVB	315210	449056	28.37%	3.568%
4	2.942	574	576	580	rBV2	592	352	0.02%	0.003%
5	2.978	586	587	592	rVB4	792	504	0.03%	0.004%
6	3.077	615	618	624	rVB4	718	577	0.04%	0.005%
7	3.106	624	627	630	rBV3	767	605	0.04%	0.005%
8	3.425	722	726	729	rBV3	817	729	0.05%	0.006%
9	3.447	731	733	736	rVB2	689	372	0.02%	0.003%
10	3.643	791	794	797	rBV3	605	400	0.03%	0.003%
11	3.798	838	842	844	rVB4	534	380	0.02%	0.003%
12	3.846	853	857	860	rBV2	748	692	0.04%	0.005%
13	3.942	870	887	928	rBV	79146	379747	23.99%	3.017%
14	4.380	1008	1023	1047	rVB	249992	613867	38.79%	4.877%
15	4.589	1085	1088	1091	rVB3	643	423	0.03%	0.003%
16	4.624	1096	1099	1100	rBV2	649	373	0.02%	0.003%
17	4.759	1137	1141	1144	rBV	985	934	0.06%	0.007%
18	4.782	1146	1148	1153	rVB3	627	521	0.03%	0.004%
19	4.836	1161	1165	1167	rVB4	1108	793	0.05%	0.006%
20	4.884	1175	1180	1182	rBV4	649	432	0.03%	0.003%
21	4.929	1190	1194	1196	rBV3	916	604	0.04%	0.005%
22	5.074	1220	1239	1263	rBV2	635536	1582619	100.00%	12.574%
23	5.415	1338	1345	1348	rBV4	545	555	0.04%	0.004%
24	5.495	1364	1370	1371	rBV5	926	678	0.04%	0.005%
25	5.528	1378	1380	1383	rVB3	986	533	0.03%	0.004%
26	5.573	1391	1394	1397	rBV3	749	550	0.03%	0.004%
27	5.643	1402	1416	1443	rBV	518182	1034060	65.34%	8.215%
28	5.929	1499	1505	1511	rVB8	1930	2910	0.18%	0.023%
29	6.000	1523	1527	1531	rBV2	716	694	0.04%	0.006%
30	6.097	1543	1557	1578	rBV	350043	707313	44.69%	5.619%
31	6.380	1642	1645	1648	rBV3	767	390	0.02%	0.003%
32	6.402	1650	1652	1655	rBV3	678	397	0.03%	0.003%
33	6.592	1707	1711	1712	rBV2	772	444	0.03%	0.004%
34	6.630	1720	1723	1724	rBV3	1200	737	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014779.D
 Acq On : 09 Mar 2020 16:12
 Operator : SY/MD
 Sample : L1835-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.682	1736	1739	1743	rVB4	624	525	0.03%	0.004%
36	6.704	1743	1746	1748	rBV2	781	367	0.02%	0.003%
37	6.756	1759	1762	1764	rBV2	641	452	0.03%	0.004%
38	6.775	1764	1768	1772	rBV3	633	571	0.04%	0.005%
39	6.894	1803	1805	1808	rBV2	721	437	0.03%	0.003%
40	6.923	1811	1814	1819	rBV3	576	702	0.04%	0.006%
41	7.010	1827	1841	1864	rBV	204199	364745	23.05%	2.898%
42	7.145	1881	1883	1887	rBV3	968	669	0.04%	0.005%
43	7.167	1887	1890	1896	rVV5	1303	1157	0.07%	0.009%
44	7.251	1914	1916	1918	rBV2	689	445	0.03%	0.004%
45	7.293	1925	1929	1930	rBV2	1047	554	0.04%	0.004%
46	7.338	1930	1943	1960	rBV	787535	1342860	84.85%	10.669%
47	7.502	1991	1994	1996	rBV4	1095	662	0.04%	0.005%
48	7.569	2013	2015	2017	rBV2	853	500	0.03%	0.004%
49	7.643	2027	2038	2061	rVV	142192	247792	15.66%	1.969%
50	7.810	2085	2090	2095	rVB5	1231	1308	0.08%	0.010%
51	7.862	2105	2106	2111	rVB3	949	562	0.04%	0.004%
52	7.891	2111	2115	2118	rBV2	948	597	0.04%	0.005%
53	7.965	2130	2138	2145	rBV3	5037	8057	0.51%	0.064%
54	8.119	2173	2186	2217	rBV	395683	815379	51.52%	6.478%
55	8.331	2250	2252	2258	rBV4	796	765	0.05%	0.006%
56	8.492	2299	2302	2304	rBV2	810	406	0.03%	0.003%
57	8.637	2344	2347	2350	rBV3	1217	868	0.05%	0.007%
58	8.688	2361	2363	2367	rBV2	739	515	0.03%	0.004%
59	8.826	2399	2406	2408	rBV2	947	819	0.05%	0.007%
60	8.875	2408	2421	2444	rBV	773044	1276188	80.64%	10.139%
61	9.148	2504	2506	2508	rBV2	851	474	0.03%	0.004%
62	9.212	2522	2526	2528	rBV3	570	457	0.03%	0.004%
63	9.328	2558	2562	2567	rBV2	1142	1001	0.06%	0.008%
64	9.383	2576	2579	2581	rBV3	468	355	0.02%	0.003%
65	9.402	2583	2585	2588	rVB3	1071	460	0.03%	0.004%
66	9.450	2599	2600	2605	rVB3	924	499	0.03%	0.004%
67	9.479	2605	2609	2613	rBV4	856	925	0.06%	0.007%
68	9.508	2617	2618	2623	rBV2	740	433	0.03%	0.003%
69	9.531	2623	2625	2627	rBV2	975	426	0.03%	0.003%
70	9.563	2631	2635	2636	rBV2	742	544	0.03%	0.004%
71	9.585	2638	2642	2644	rBV2	684	410	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030920\
 Data File : VV014779.D
 Acq On : 09 Mar 2020 16:12
 Operator : SY/MD
 Sample : L1835-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.749	2691	2693	2697	rBV2	757	510	0.03%	0.004%
73	9.878	2730	2733	2737	rVB2	521	454	0.03%	0.004%
74	9.897	2737	2739	2742	rBV3	503	366	0.02%	0.003%
75	10.238	2833	2845	2862	rBV	495623	777388	49.12%	6.176%
76	10.402	2888	2896	2907	rVB4	8609	13870	0.88%	0.110%
77	10.447	2907	2910	2911	rBV2	613	371	0.02%	0.003%
78	10.521	2930	2933	2934	rBV	833	427	0.03%	0.003%
79	10.614	2958	2962	2967	rBV3	780	764	0.05%	0.006%
80	10.669	2976	2979	2985	rBV3	574	479	0.03%	0.004%
81	10.701	2985	2989	2992	rBV2	562	450	0.03%	0.004%
82	10.749	3000	3004	3006	rVB2	688	447	0.03%	0.004%
83	10.788	3013	3016	3023	rVB3	644	420	0.03%	0.003%
84	10.862	3033	3039	3040	rBV2	713	613	0.04%	0.005%
85	10.894	3047	3049	3051	rBV3	735	432	0.03%	0.003%
86	10.968	3070	3072	3075	rVV2	662	472	0.03%	0.004%
87	10.984	3075	3077	3080	rVB2	1106	544	0.03%	0.004%
88	11.180	3131	3138	3140	rBV7	1831	2180	0.14%	0.017%
89	11.267	3153	3165	3185	rBV	809529	1267837	80.11%	10.073%
90	11.463	3224	3226	3228	rBV3	844	467	0.03%	0.004%
91	11.646	3271	3283	3304	rVB	785849	1239472	78.32%	9.847%
92	12.067	3411	3414	3420	rBV5	673	714	0.05%	0.006%
93	12.145	3435	3438	3442	rBV2	852	550	0.03%	0.004%
94	12.373	3502	3509	3515	rVB7	3739	5000	0.32%	0.040%
95	12.569	3567	3570	3573	rBV2	728	616	0.04%	0.005%
96	12.659	3593	3598	3601	rBV4	1626	1467	0.09%	0.012%
97	12.723	3614	3618	3620	rBV3	657	538	0.03%	0.004%
98	13.116	3738	3740	3746	rVB4	795	652	0.04%	0.005%
99	13.283	3782	3792	3802	rBV5	7764	12068	0.76%	0.096%
100	13.765	3935	3942	3949	rBV8	3375	4327	0.27%	0.034%


Sum of corrected areas: 12586917

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030920\
Data File : VV014779.D
Acq On : 09 Mar 2020 16:12
Operator : SY/MD
Sample : L1835-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

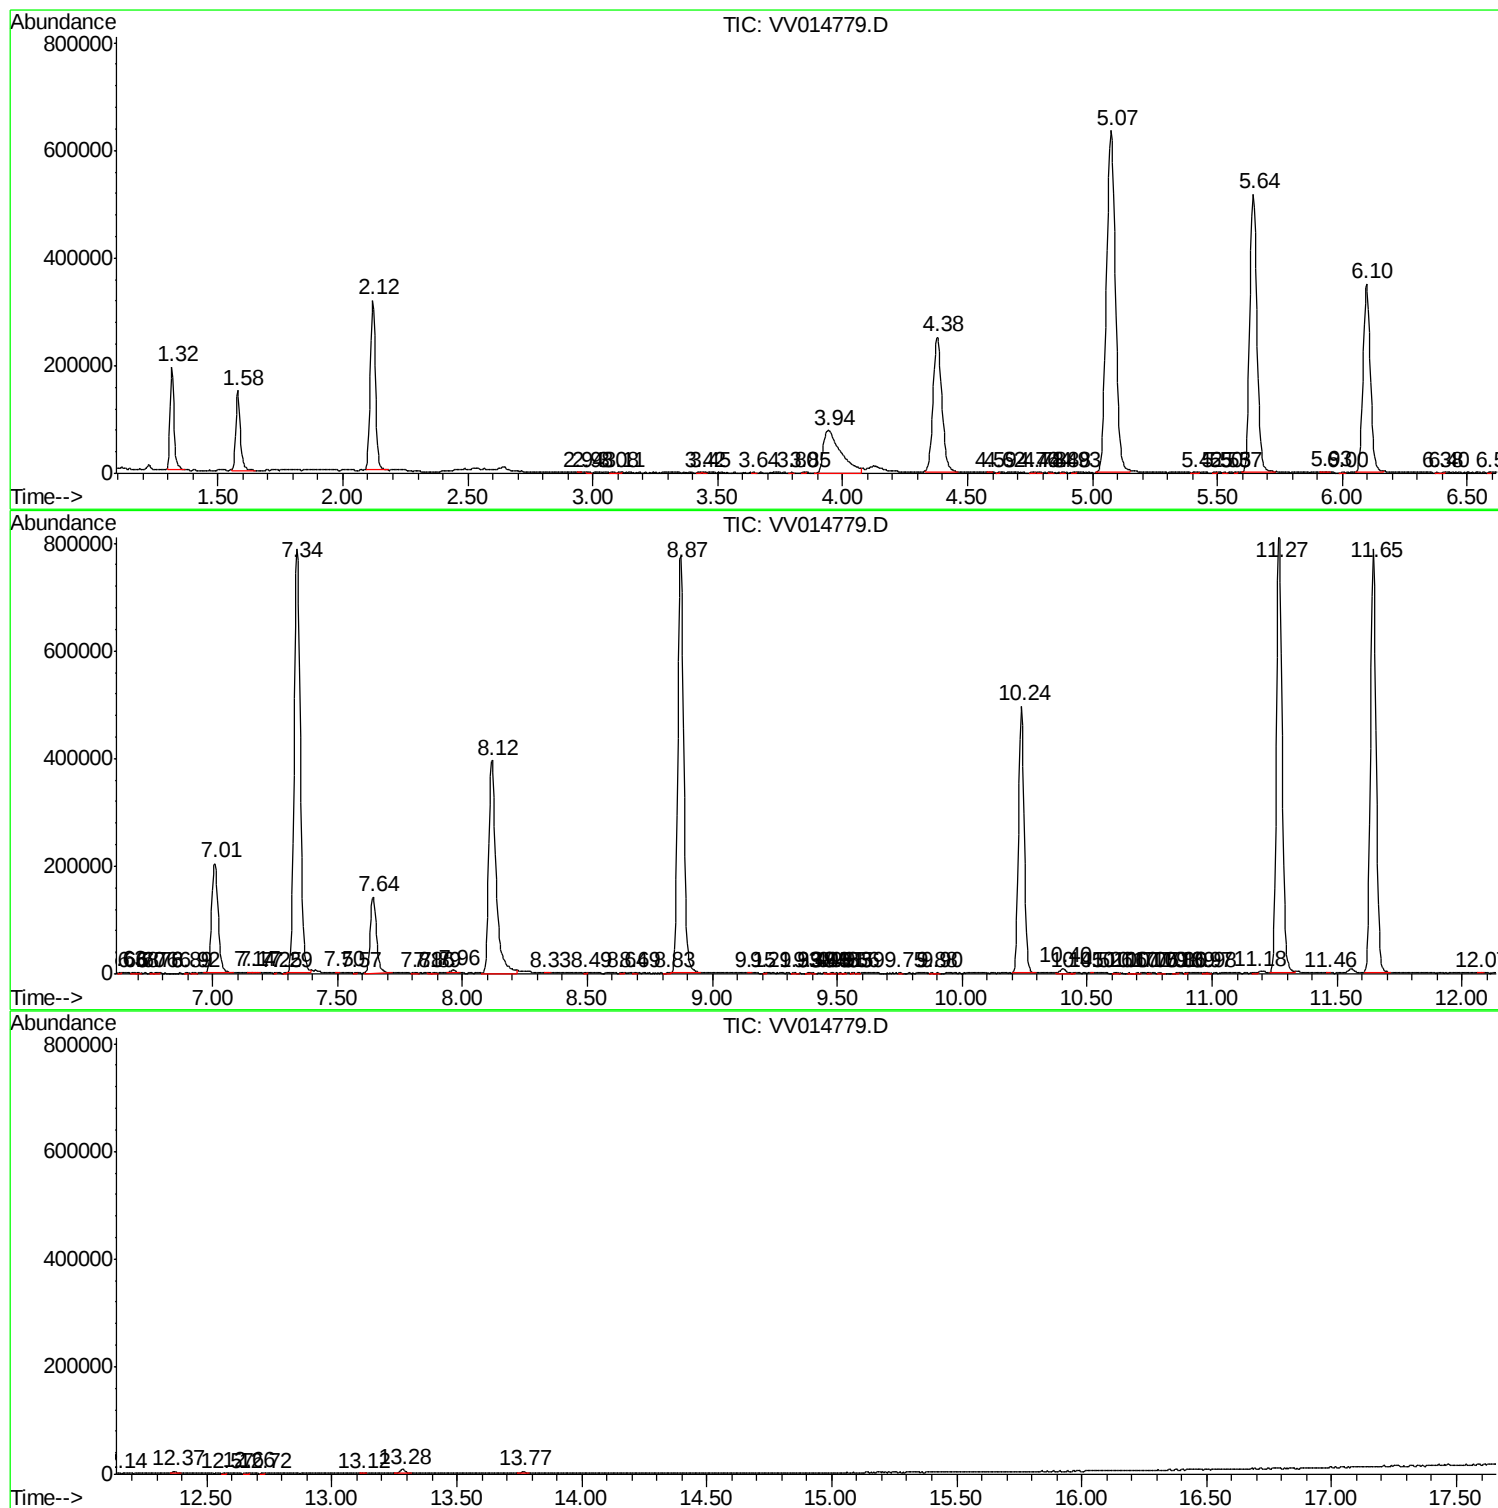

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014779.D
Acq On : 09 Mar 2020 16:12
Operator : SY/MD
Sample : L1835-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014779.D
Acq On : 09 Mar 2020 16:12
Operator : SY/MD
Sample : L1835-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DM6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc