


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030920\
 Data File : VV014766.D
 Acq On : 09 Mar 2020 09:31
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB98

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 11 12:33:27 2020

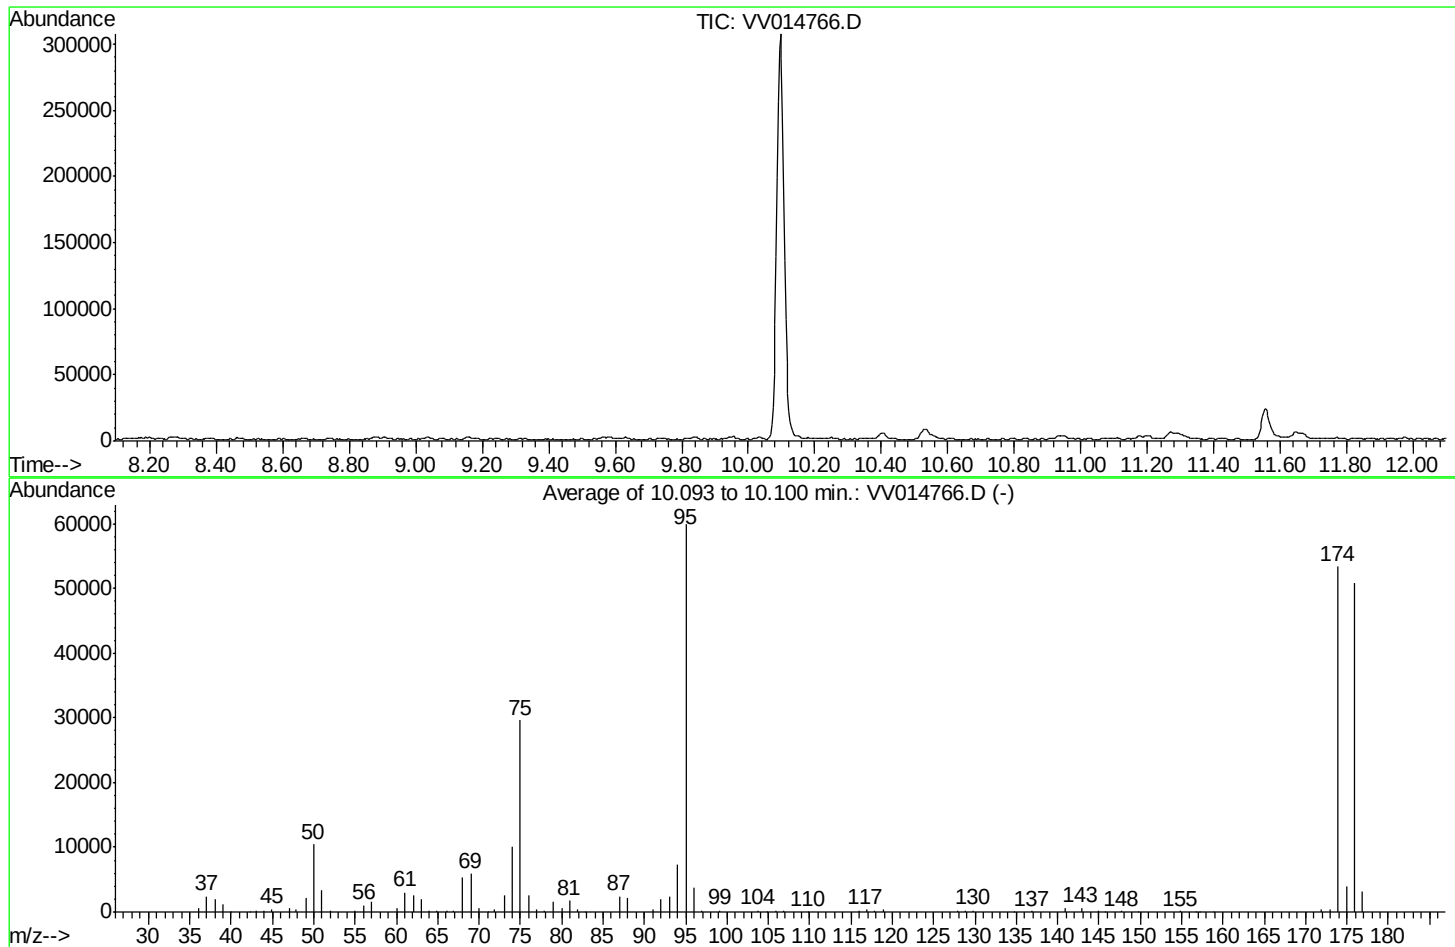

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	10463	PASS
75	95	30	80	49.5	29653	PASS
95	95	100	100	100.0	59906	PASS
96	95	5	9	6.4	3854	PASS
173	174	0.00	2	0.9	474	PASS
174	95	50	120	89.0	53328	PASS
175	174	5	9	7.3	3893	PASS
176	174	95	101	95.5	50933	PASS
177	176	5	9	6.2	3138	PASS

Scan 2788 (10.055 min): VV014766.D
BFB98

m/z	Abundance
39.90	579.0
40.90	111.0
44.00	475.0
44.80	123.0
54.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	609.0
37.00	2548.0
38.00	2038.0
38.90	1064.0
39.90	626.0
40.90	133.0
42.20	105.0
42.90	218.0
43.90	722.0
45.00	611.0
47.00	695.0
47.90	371.0
49.00	2315.0
50.00	10434.0
51.00	3383.0
51.90	176.0
54.90	259.0
56.00	1011.0
57.00	1655.0
60.10	740.0
61.00	3124.0
62.00	2490.0
63.00	2102.0
63.90	319.0
64.90	321.0
66.10	100.0
66.80	230.0
68.00	5535.0
69.00	6277.0
70.00	529.0
71.80	366.0
73.00	2706.0
74.00	10080.0
75.00	29736.0
76.00	2852.0
77.00	479.0
77.80	337.0
78.90	1611.0
80.00	628.0
80.90	1689.0
81.90	416.0
87.00	2671.0
87.90	2199.0
91.00	288.0
92.00	1935.0
93.00	2472.0
94.00	7338.0
95.00	58944.0
96.00	3873.0
96.90	166.0
99.10	293.0
103.80	187.0
104.80	153.0
105.80	236.0
106.80	139.0
109.80	106.0
115.90	198.0
116.90	391.0
117.90	206.0
119.00	342.0
127.90	238.0
128.80	151.0
129.80	216.0
137.00	103.0
140.90	600.0
142.90	704.0
145.00	127.0
147.70	168.0
149.80	116.0
155.00	188.0
156.70	105.0
158.80	150.0
171.90	324.0
172.90	477.0
173.90	52120.0
175.00	3876.0
175.90	49616.0
176.90	2894.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	610.0
37.00	2468.0
38.00	2137.0
39.00	1175.0
39.90	614.0
40.90	101.0
43.00	184.0
43.90	724.0
45.00	594.0
47.10	666.0
47.80	383.0
49.00	2198.0
50.00	10824.0
51.00	3645.0
52.00	181.0
54.90	263.0
56.00	1090.0
57.00	1566.0
60.00	729.0
61.00	3121.0
62.00	2666.0
63.00	2103.0
63.90	311.0
64.80	297.0
66.00	118.0
66.80	243.0
68.00	5611.0
69.00	5969.0
70.00	562.0
71.00	102.0
71.80	359.0
73.00	2717.0
74.00	10345.0
75.00	30568.0
76.00	2695.0
77.00	492.0
77.80	308.0
78.90	1576.0
80.00	627.0
80.90	1814.0
81.90	477.0
82.90	121.0
86.90	2478.0
87.90	2244.0
91.00	355.0
92.00	2016.0
93.00	2492.0
94.00	7560.0
95.00	62072.0
96.00	3949.0
96.90	142.0
99.10	238.0
103.80	258.0
105.90	197.0
106.80	134.0
115.90	217.0
116.90	380.0
117.90	167.0
119.00	360.0
127.90	272.0
128.90	119.0
129.80	270.0
137.00	159.0
140.90	626.0
142.80	676.0
145.00	138.0
145.70	105.0
147.80	186.0
154.90	167.0
158.80	129.0
171.90	329.0
173.00	493.0
173.90	55288.0
174.90	3979.0
175.90	52976.0
176.90	3302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	534.0
37.00	2323.0
38.00	2024.0
39.00	1177.0
39.90	591.0
43.10	167.0
43.90	666.0
44.90	493.0
47.10	602.0
47.80	347.0
49.00	1911.0
50.00	10133.0
51.00	3293.0
52.00	150.0
54.90	272.0
56.10	1100.0
57.00	1351.0
60.00	617.0
61.00	2827.0
62.10	2733.0
63.00	1973.0
64.00	280.0
64.80	269.0
66.00	129.0
66.90	189.0
68.00	5159.0
69.00	5440.0
69.90	480.0
71.00	106.0
71.90	343.0
73.00	2397.0
74.00	9821.0
75.00	28656.0
76.00	2435.0
77.00	464.0
77.90	247.0
78.90	1378.0
80.00	565.0
80.90	1686.0
81.90	442.0
82.90	149.0
86.90	2138.0
87.90	2033.0
91.00	297.0
92.00	1758.0
93.00	2294.0
94.00	7012.0
95.00	58704.0
96.00	3740.0
96.90	140.0
99.00	177.0
103.80	299.0
105.90	188.0
106.80	101.0
115.90	209.0
116.90	371.0
117.90	167.0
118.90	276.0
127.90	241.0
128.90	127.0
129.80	279.0
134.70	137.0
136.90	164.0
140.90	625.0
142.90	545.0
144.90	157.0
147.80	158.0
154.80	168.0
157.10	109.0
171.90	337.0
173.00	453.0
173.90	52576.0
174.90	3825.0
175.90	50208.0
176.90	3219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98