

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030921\
Data File : VV020475.D
Acq On : 09 Mar 2021 16:54
Operator : SY/MD
Sample : M1617-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG0M7

Manual Integrations
APPROVED

MMDadoda
3/10/2021 1:42:17 PM

Quant Time: Mar 10 00:20:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 10 00:20:01 2021
Response via : Initial Calibration

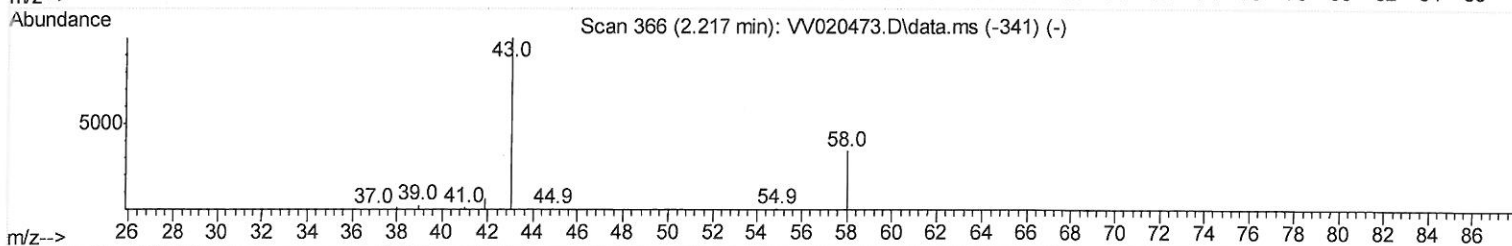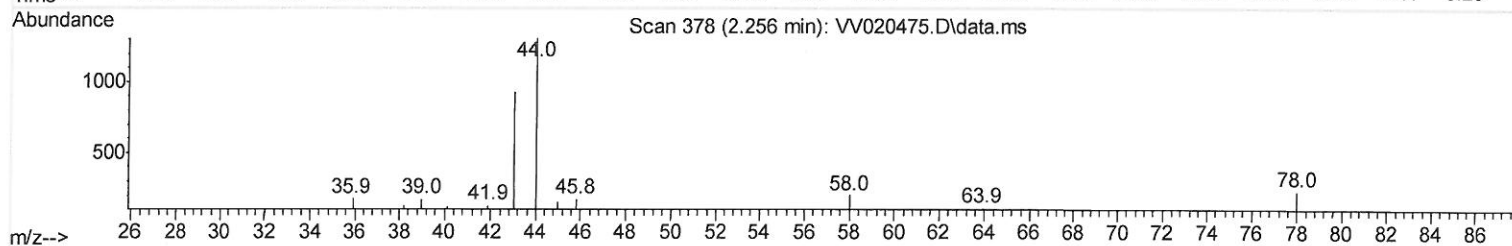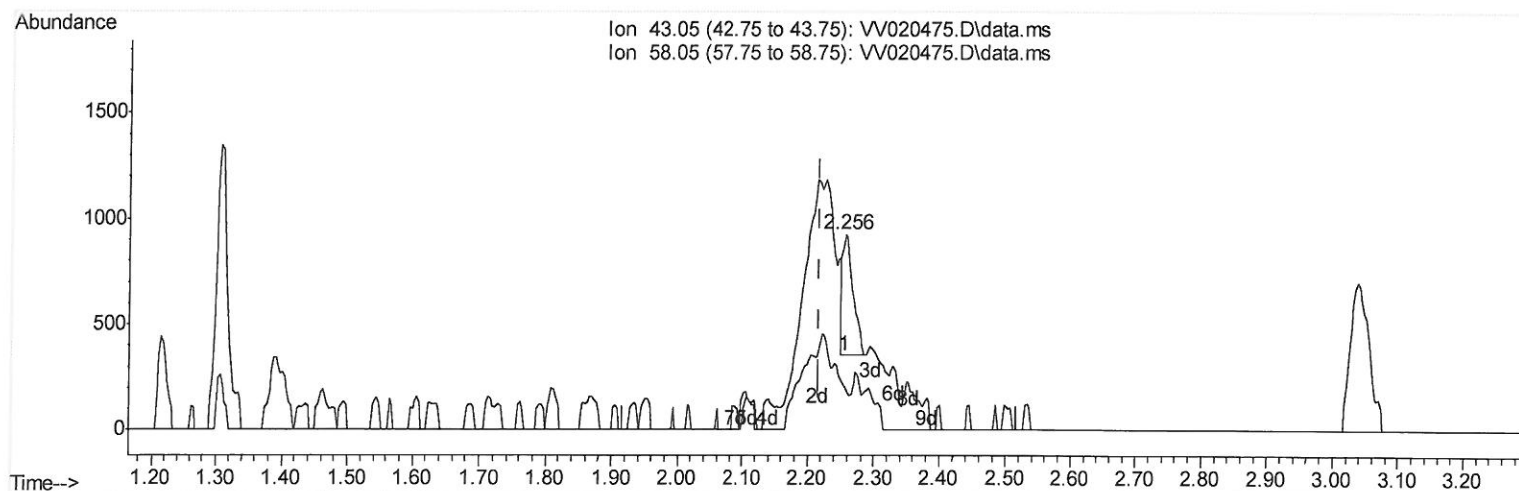

TIC: VV020475.D\data.ms

(13) Acetone (T)

2.256min (+ 0.039) 0.18 ug/L

response 605

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	15.37
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030921\
 Data File : VW020475.D
 Acq On : 09 Mar 2021 16:54
 Operator : SY/MD
 Sample : M1617-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0M7

Manual Integrations
 APPROVED

MMDadoda
 3/10/2021 1:42:17 PM

Quant Time: Mar 10 00:20:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 10 00:20:01 2021
 Response via : Initial Calibration

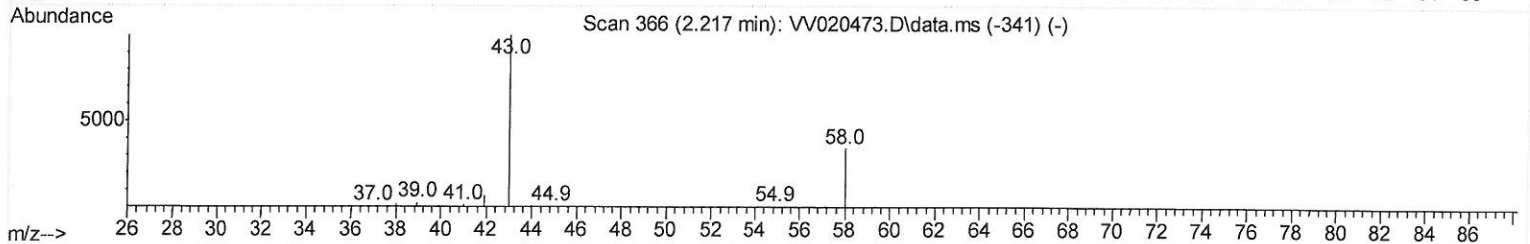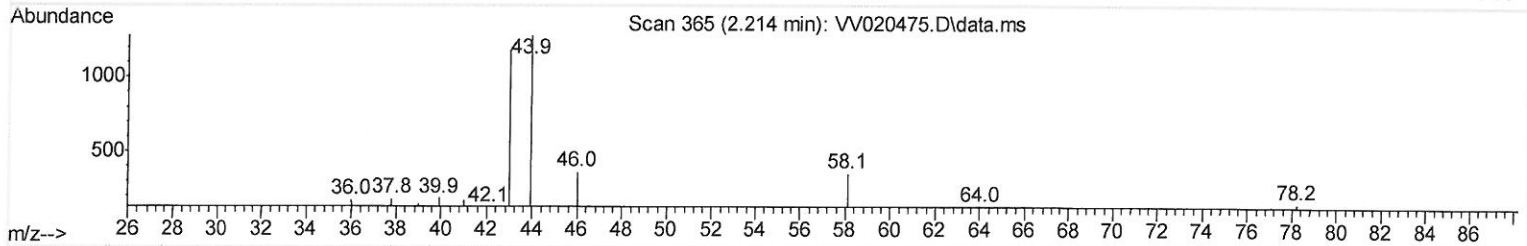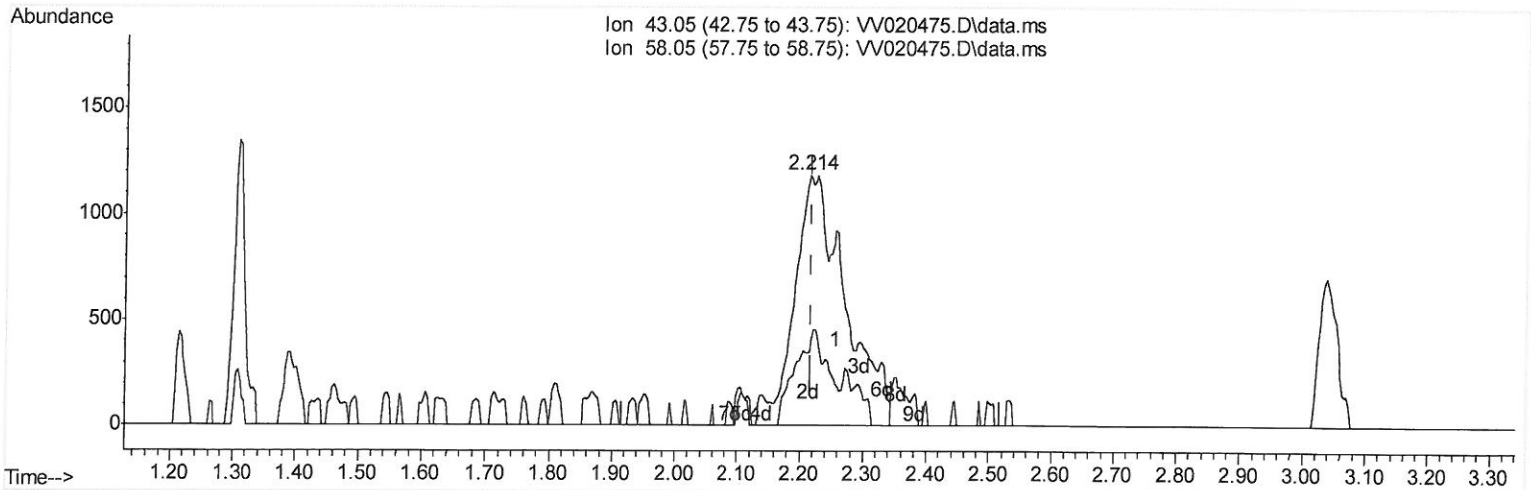

TIC: VW020475.D\data.ms

(13) Acetone (T)

2.214min (-0.003) 2.00 ug/L m

response 6686

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	1.39
0.00	0.00	0.00
0.00	0.00	0.00

203/12/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\W030921\
 Data File : W020475.D
 Acq On : 09 Mar 2021 16:54
 Operator : SY/MD
 Sample : M1617-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0M7

Manual Integrations
 APPROVED

MMDadoda
 3/10/2021 1:42:17 PM

Quant Time: Mar 10 00:20:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR02221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 10 00:20:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	301559	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	298514	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	143018	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	93306	4.39	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery =	87.80%		
7) Chloroethane-d5	1.568	69	74651	4.47	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery =	89.40%		
11) 1,1-Dichloroethene-d2	2.108	63	124854	3.02	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery =	60.40%		
20) 2-Butanone-d5	3.918	46	144344	39.24	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery =	78.48%		
24) Chloroform-d	4.349	84	159226	4.19	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	83.80%		
26) 1,2-Dichloroethane-d4	5.034	65	77249	4.18	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	83.60%		
32) Benzene-d6	5.050	84	326912	4.37	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	87.40%		
36) 1,2-Dichloropropane-d6	6.069	67	92304	4.17	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery =	83.40%		
41) Toluene-d8	7.317	98	301606	4.18	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	83.60%		
45) trans-1,3-Dichloroprop...	7.625	79	32930	3.89	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery =	77.80%		
48) 2-Hexanone-d5	8.095	63	89408	30.14	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery =	60.28%		
59) 1,1,2,2-Tetrachloroeth...	10.223	84	49262	3.13	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery =	62.60%#		
65) 1,2-Dichlorobenzene-d4	11.632	152	120314	4.74	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery =	94.80%		
Target Compounds						
13) Acetone	2.214	43	6686m	2.00	ug/L	Qvalue 03/12/21 SY
16) Methylene chloride	2.507	84	5734	0.21	ug/L	100
25) Chloroform	4.378	83	7215	0.14	ug/L	98
50) 2-Hexanone	8.146	43	20023	2.23	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030921\
Data File : VW020475.D
Acq On : 09 Mar 2021 16:54
Operator : SY/MD
Sample : M1617-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0M7

Manual Integrations
APPROVED

MMDadoda
3/10/2021 1:42:17 PM

Quant Time: Mar 10 00:20:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 10 00:20:01 2021
Response via : Initial Calibration

