

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V030921\
 Data File : V020487.D
 Acq On : 09 Mar 2021 22:35
 Operator : SY/MD
 Sample : M1617-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 3/10/2021 1:42:19 PM

Quant Time: Mar 10 01:02:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 10 01:00:54 2021
 Response via : Initial Calibration

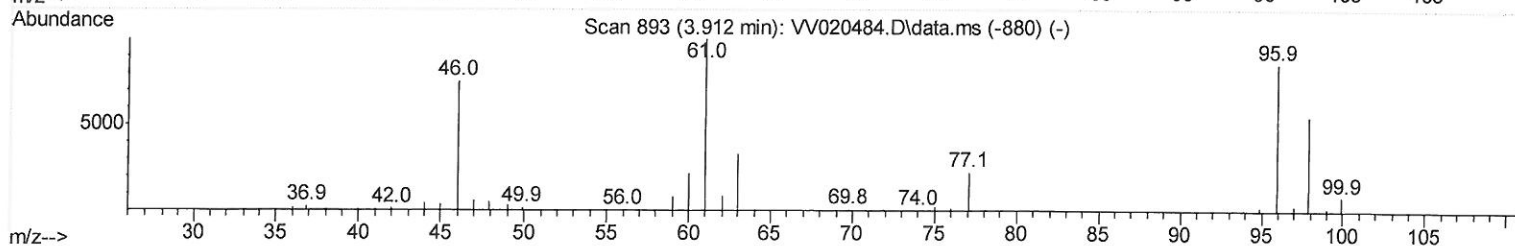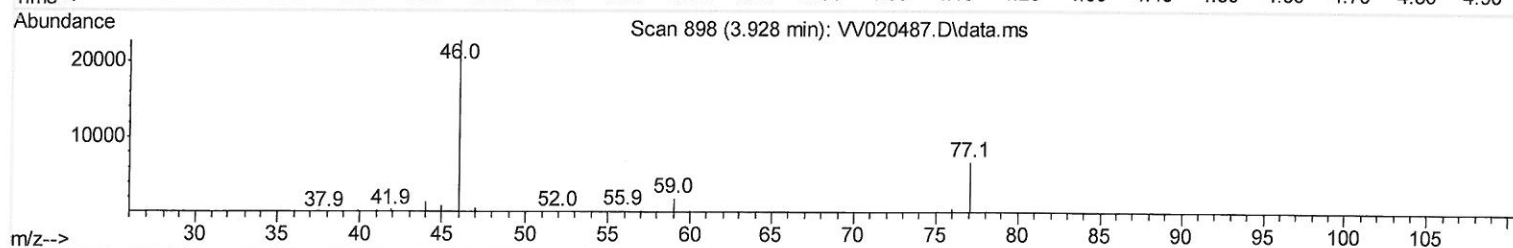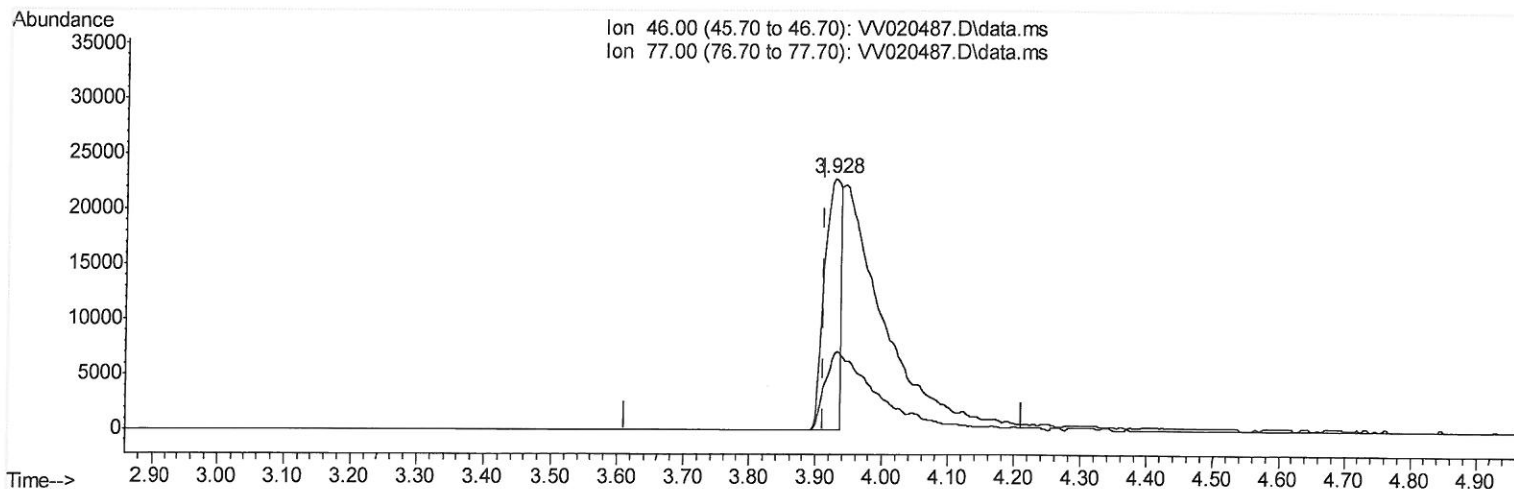

TIC: VV020487.D\data.ms

(20) 2-Butanone-d5 (S)

3.928min (+ 0.016) 11.79 ug/L

response 40256

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.20	83.25#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030921\
 Data File : VV020487.D
 Acq On : 09 Mar 2021 22:35
 Operator : SY/MD
 Sample : M1617-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 3/10/2021 1:42:19 PM

Quant Time: Mar 10 01:02:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 10 01:00:54 2021
 Response via : Initial Calibration

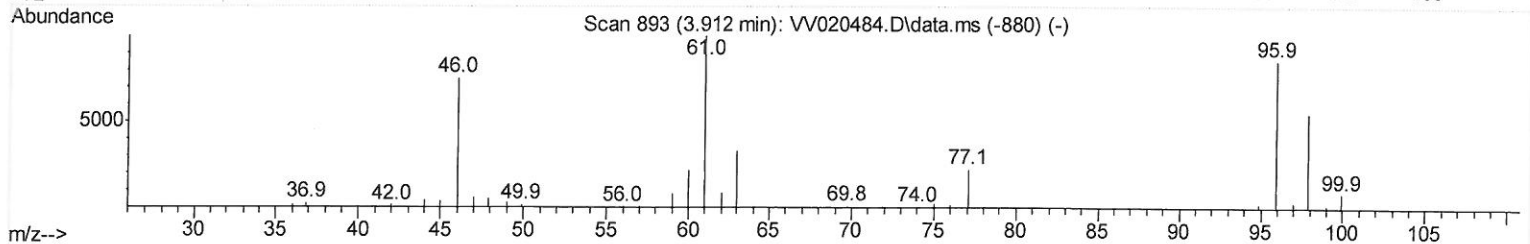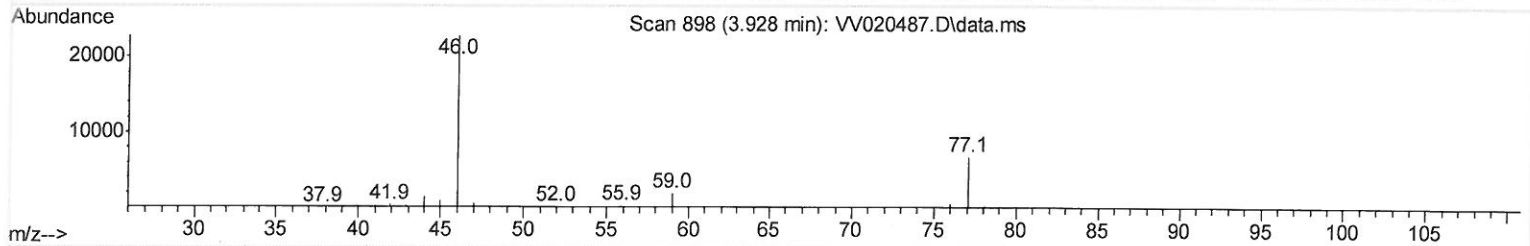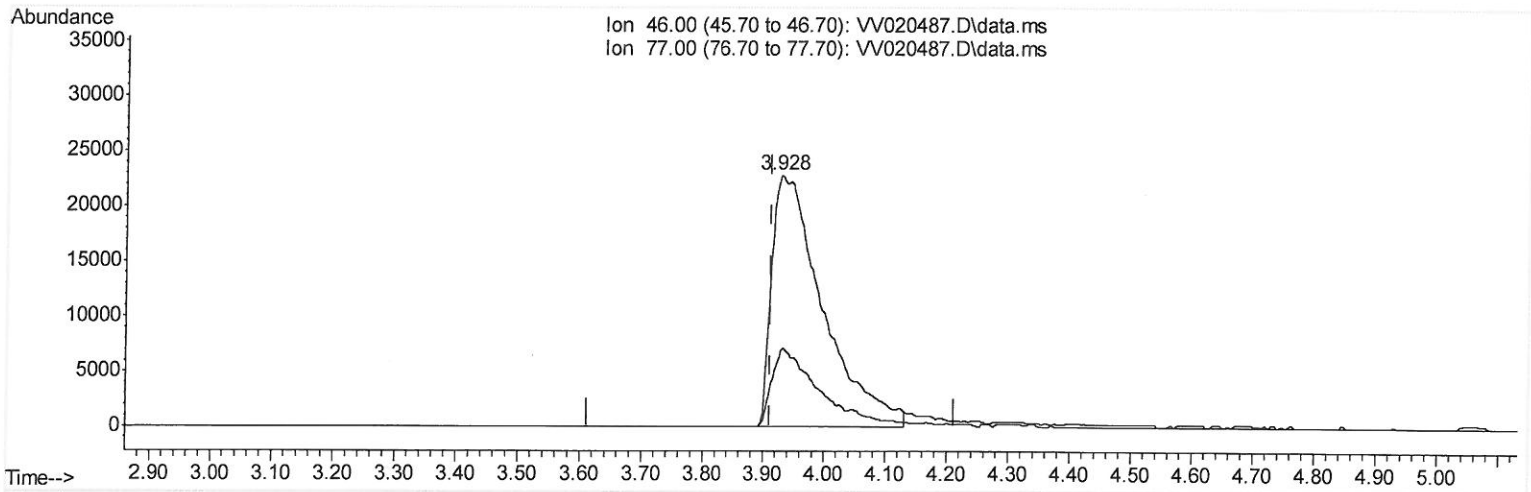

TIC: VV020487.D\data.ms

(20) 2-Butanone-d5 (S)

3.928min (+ 0.016) 38.69 ug/L m

response 132105

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.20	25.37#
0.00	0.00	0.00
0.00	0.00	0.00

03/12/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030921\
 Data File : VW020487.D
 Acq On : 09 Mar 2021 22:35
 Operator : SY/MD
 Sample : M1617-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 3/10/2021 1:42:19 PM

Quant Time: Mar 10 01:02:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 10 01:00:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	279955	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	281150	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	131440	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	85693	4.35	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	87.00%		
7) Chloroethane-d5	1.568	69	67945	4.39	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	87.80%		
11) 1,1-Dichloroethene-d2	2.105	63	113584	2.96	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	59.20%#		
20) 2-Butanone-d5	3.928	46	132105m	38.69	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	77.38%		
24) Chloroform-d	4.352	84	147081	4.17	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	83.40%		
26) 1,2-Dichloroethane-d4	5.037	65	71019	4.14	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	82.80%		
32) Benzene-d6	5.053	84	306272	4.35	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	87.00%		
36) 1,2-Dichloropropane-d6	6.075	67	85518	4.10	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	82.00%		
41) Toluene-d8	7.320	98	278768	4.10	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	82.00%		
45) trans-1,3-Dichloroprop...	7.628	79	29801	3.74	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	74.80%		
48) 2-Hexanone-d5	8.098	63	89742	32.13	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	64.26%		
59) 1,1,2,2-Tetrachloroeth...	10.223	84	50992	3.44	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	68.80%		
65) 1,2-Dichlorobenzene-d4	11.631	152	112679	4.83	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	96.60%		
Target Compounds						
25) Chloroform	4.384	83	5795	0.12	ug/L	94
50) 2-Hexanone	8.153	43	14563	1.72	ug/L #	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/12/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030921\
Data File : VW020487.D
Acq On : 09 Mar 2021 22:35
Operator : SY/MD
Sample : M1617-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
3/10/2021 1:42:19 PM

Quant Time: Mar 10 01:02:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 10 01:00:54 2021
Response via : Initial Calibration

