


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030921\
Data File : VV020472.D
Acq On : 09 Mar 2021 08:55
Operator : SY/MD
Sample : BFB34
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 10 01:00:54 2021

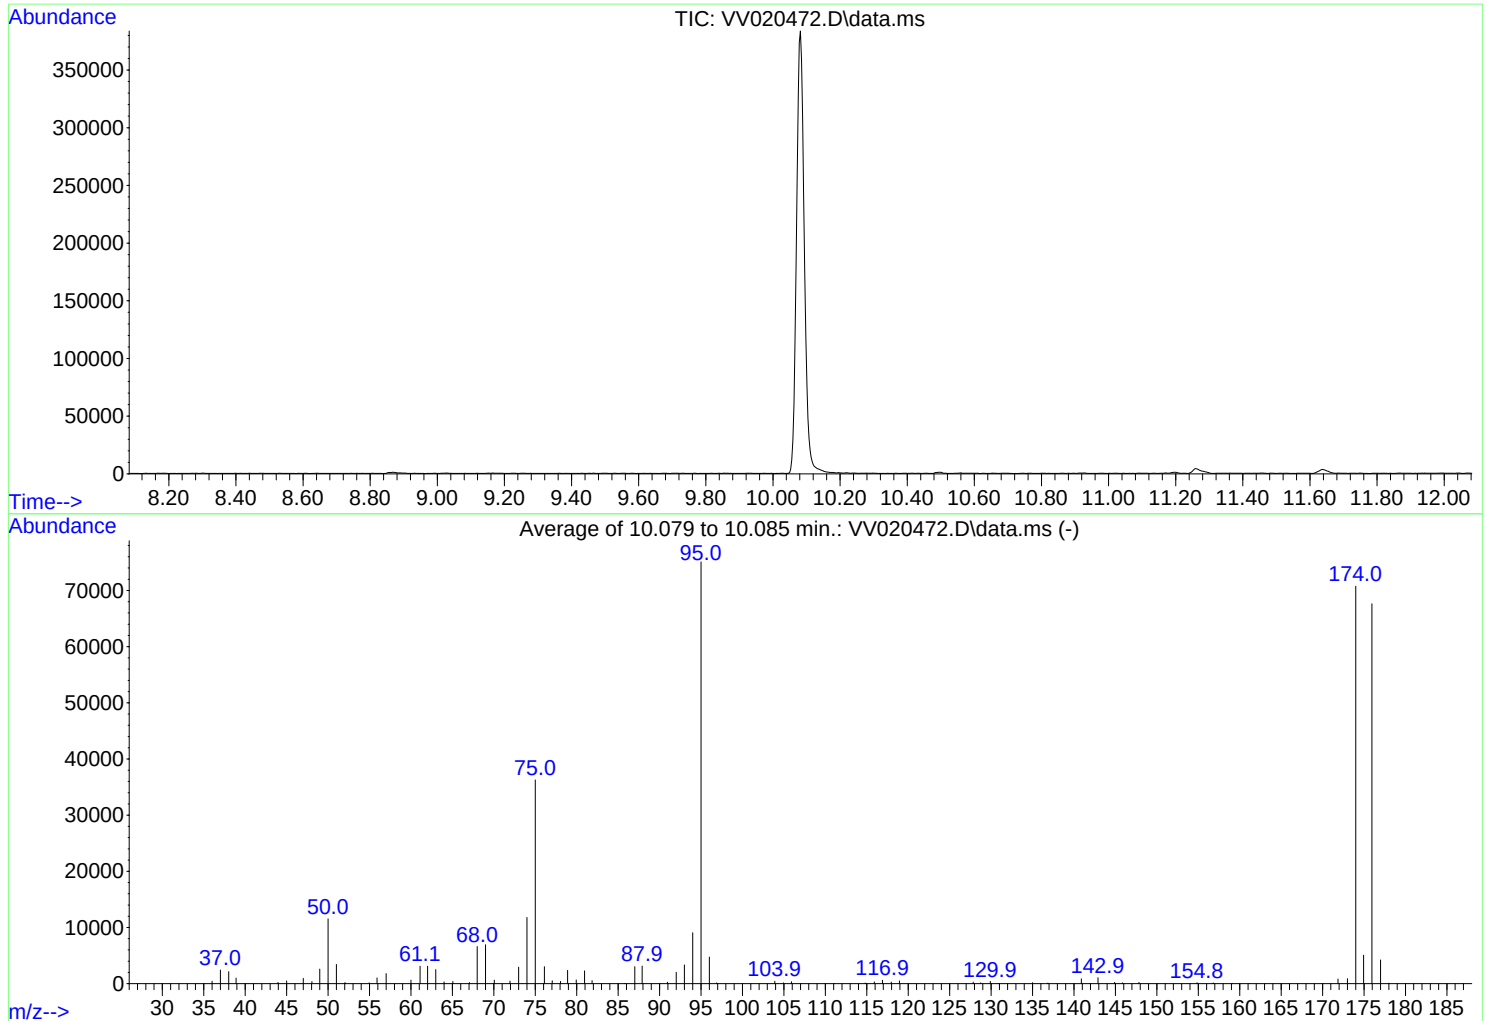

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2798

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	11543	PASS
75	95	30	80	48.3	36272	PASS
95	95	100	100	100.0	75101	PASS
96	95	5	9	6.3	4728	PASS
173	174	0.00	2	1.3	896	PASS
174	95	50	120	94.2	70760	PASS
175	174	5	9	7.2	5078	PASS
176	174	95	101	95.6	67645	PASS
177	176	5	9	6.2	4221	PASS

m/z	Abundance
36.00	401.0
37.00	2468.0
38.00	2206.0
38.90	1073.0
40.10	120.0
43.90	554.0
45.00	489.0
47.00	1006.0
48.10	417.0
49.00	2592.0
50.00	12071.0
51.00	3407.0
52.10	185.0
54.90	141.0
55.90	1057.0
57.00	1803.0
60.00	595.0
61.10	3241.0
62.00	3173.0
63.00	2541.0
64.00	311.0
65.10	379.0
67.10	201.0
68.00	7019.0
69.00	7142.0
70.10	493.0
72.00	384.0
73.00	3041.0
74.00	12250.0
75.00	36880.0
76.10	2952.0
77.00	583.0
78.10	470.0
78.90	2341.0
80.00	637.0
80.90	2256.0
81.90	511.0
85.80	122.0
87.00	3030.0
87.90	3285.0
90.90	292.0
92.00	2109.0
93.00	3253.0
94.00	9177.0
95.00	75904.0
96.00	4975.0
96.90	213.0
103.90	432.0
104.90	135.0
105.90	357.0
111.10	106.0
114.80	129.0
115.90	327.0
116.90	621.0
117.90	295.0
118.90	494.0
128.00	345.0
128.80	123.0
129.90	374.0
135.00	170.0
136.80	107.0
140.90	932.0
142.00	112.0
142.90	1054.0
144.90	204.0
145.90	145.0
147.90	219.0
155.00	157.0
156.80	157.0
159.10	111.0
171.90	745.0
173.00	853.0
174.00	69336.0
175.00	5044.0
175.90	66424.0
177.00	4284.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	461.0
37.00	2515.0
38.00	2155.0
38.90	1035.0
40.10	120.0
44.00	564.0
45.00	488.0
47.00	958.0
48.00	382.0
49.00	2664.0
50.00	11836.0
51.00	3461.0
52.10	213.0
55.00	142.0
55.90	1064.0
57.00	1867.0
60.00	649.0
61.10	3201.0
62.00	3262.0
63.00	2596.0
64.00	302.0
65.00	402.0
67.00	218.0
68.00	6791.0
69.00	7050.0
70.00	642.0
72.00	472.0
73.00	2999.0
74.00	12219.0
75.00	37448.0
76.10	3129.0
77.10	557.0
78.10	418.0
78.90	2461.0
80.00	683.0
81.00	2334.0
81.90	557.0
87.00	3082.0
87.90	3211.0
90.90	275.0
92.00	2128.0
93.00	3476.0
94.00	9320.0
95.00	77320.0
96.00	4778.0
96.90	161.0
103.90	463.0
104.90	159.0
105.90	348.0
114.80	134.0
115.90	312.0
116.90	622.0
117.90	302.0
119.00	506.0
127.80	274.0
128.70	162.0
129.90	408.0
130.90	103.0
135.00	176.0
136.80	114.0
140.90	878.0
142.90	1120.0
144.90	239.0
145.80	123.0
147.80	248.0
154.80	169.0
156.80	163.0
159.10	107.0
161.10	101.0
171.80	865.0
173.00	940.0
174.00	72992.0
174.90	5222.0
176.00	70032.0
177.00	4354.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	451.0
37.00	2333.0
38.00	2087.0
38.90	924.0
40.00	124.0
44.00	574.0
45.00	465.0
47.00	826.0
48.00	322.0
49.00	2555.0
50.00	10723.0
51.00	3381.0
52.00	188.0
55.00	158.0
55.90	945.0
57.00	1699.0
60.00	631.0
61.10	2911.0
62.00	2889.0
63.00	2411.0
64.00	300.0
65.00	465.0
67.00	203.0
68.00	6049.0
69.00	6561.0
70.00	721.0
71.90	501.0
73.00	2798.0
74.00	10943.0
75.00	34488.0
76.10	2969.0
77.00	442.0
78.00	344.0
78.90	2289.0
79.90	677.0
80.90	2219.0
81.80	526.0
87.00	2983.0
87.90	2882.0
91.00	242.0
92.00	1835.0
93.00	3263.0
94.00	8672.0
95.00	72080.0
96.00	4430.0
97.00	101.0
103.90	403.0
105.00	162.0
105.90	291.0
114.80	103.0
115.90	290.0
116.90	581.0
118.00	283.0
118.90	482.0
127.80	286.0
128.70	170.0
129.90	385.0
135.00	147.0
136.90	134.0
140.90	734.0
142.90	972.0
144.90	278.0
145.80	135.0
147.80	225.0
154.80	174.0
156.80	137.0
171.80	897.0
173.00	896.0
174.00	69952.0
174.90	4967.0
175.90	66480.0
177.00	4024.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
40.00	152.0
44.00	340.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34