

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024886.D
 Acq On : 09 Mar 2022 17:30
 Operator : SY/MD
 Sample : VV0309MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 10 05:50:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	298819	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	292496	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	134808	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	110136	36.248	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.500%
7) Chloroethane-d5	1.568	69	98349	41.256	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.520%
11) 1,1-Dichloroethene-d2	2.108	63	155863	30.563	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.120%
21) 2-Butanone-d5	3.892	46	161390	93.334	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.330%
24) Chloroform-d	4.349	84	228294	43.042	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.080%
26) 1,2-Dichloroethane-d4	5.031	65	141730	45.288	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.580%
32) Benzene-d6	5.050	84	471566	43.496	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	6.069	67	152034	45.010	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.020%
41) Toluene-d8	7.314	98	410797	42.770	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.540%
43) trans-1,3-Dichloroprop...	7.619	79	60868	41.471	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.940%
47) 2-Hexanone-d5	8.088	63	116718	91.035	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.040%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	183669	45.844	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.680%
66) 1,2-Dichlorobenzene-d4	11.622	152	148384	47.784	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.560%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.986	75	3947	1.059	ug/L #	68
61) 1,2,3-Trichloropropane	11.246	75	17859	6.621	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024886.D
Acq On : 09 Mar 2022 17:30
Operator : SY/MD
Sample : VV0309MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 10 05:50:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 10 05:49:38 2022
Response via : Initial Calibration

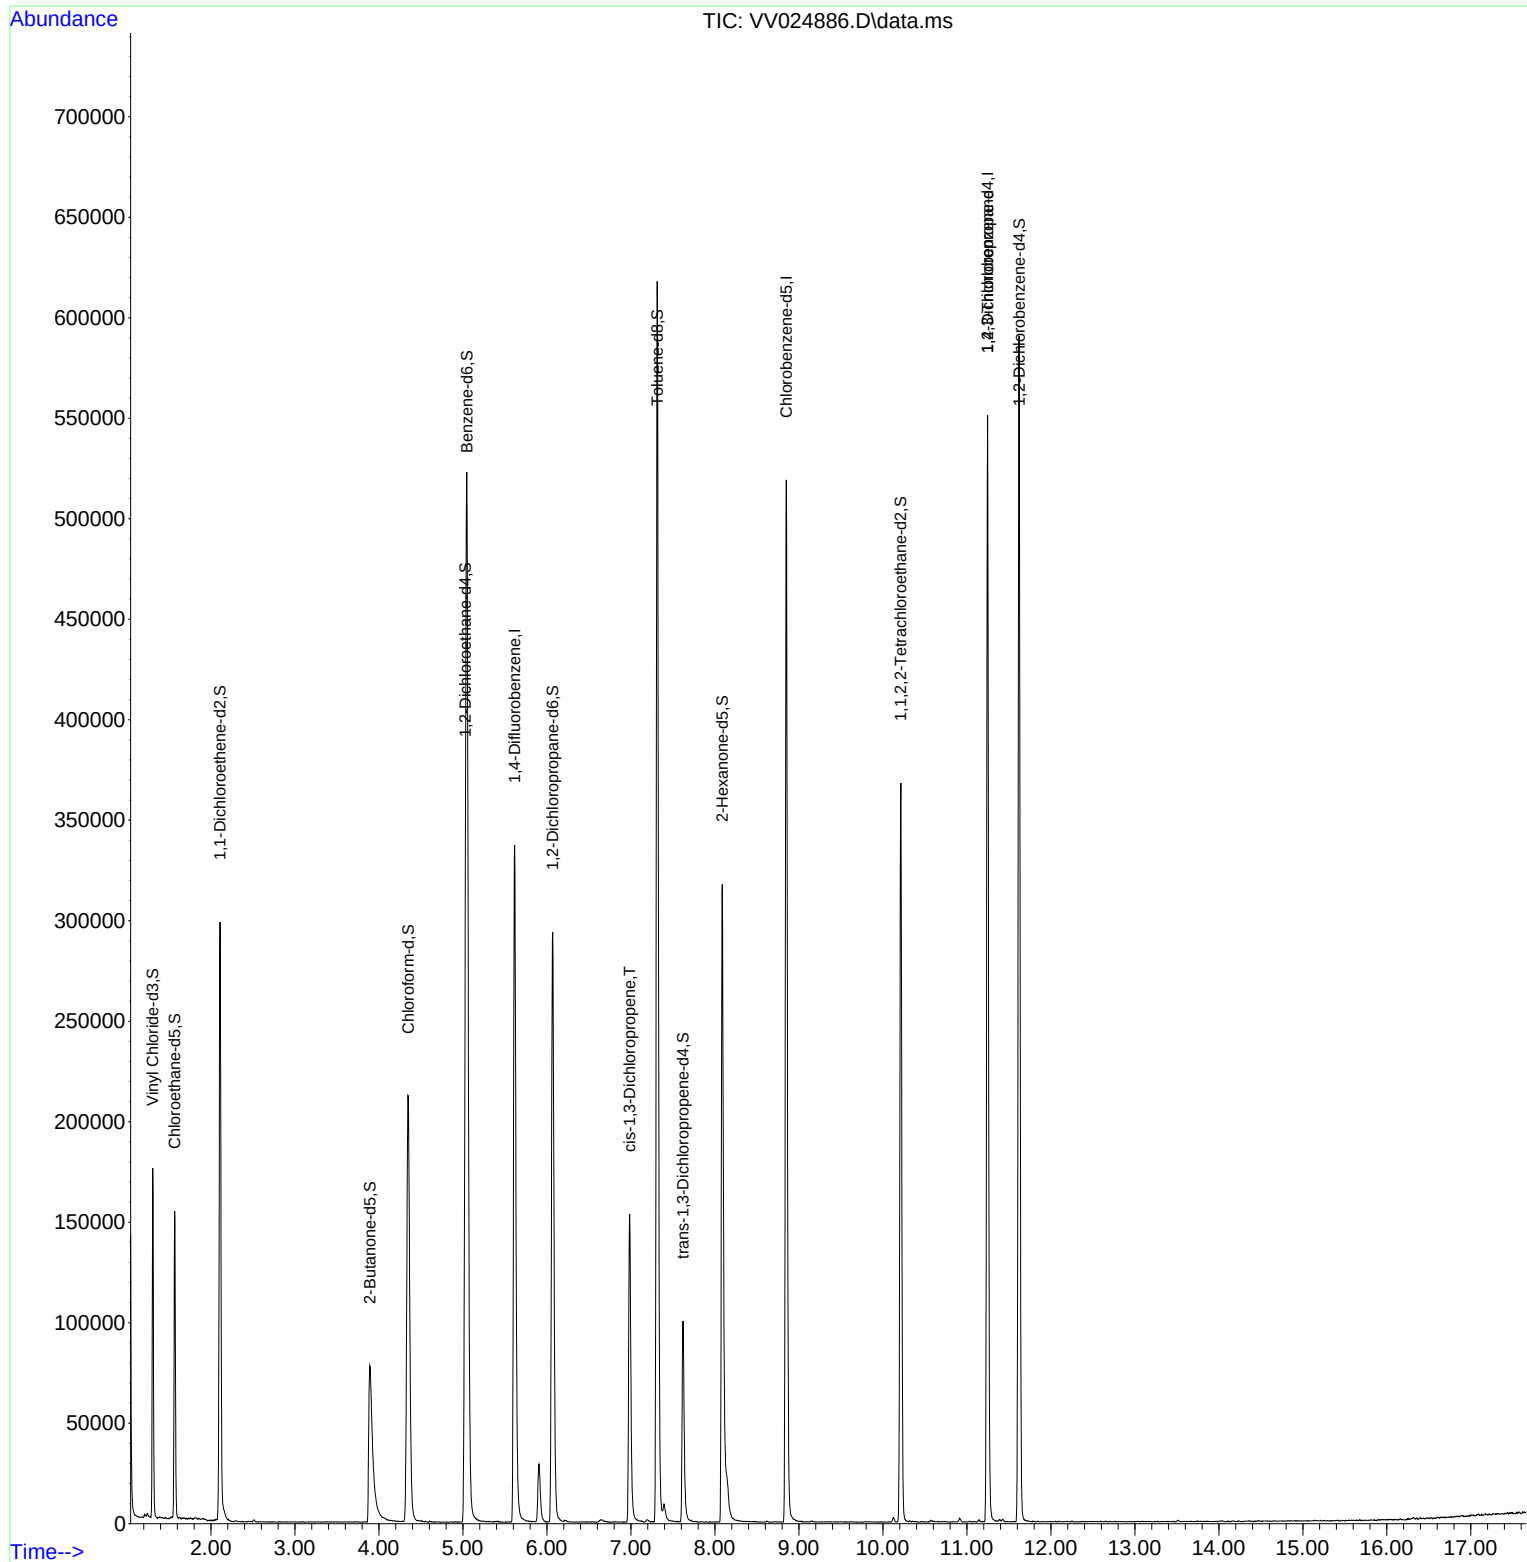

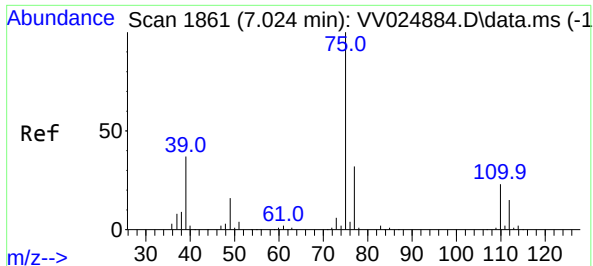

#39

cis-1,3-Dichloropropene

Concen: 1.059 ug/L

RT: 6.986 min Scan# 11

Delta R.T. -0.039 min

Lab File: VV024886.D

Acq: 09 Mar 2022 17:30

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 3947

Ion Ratio Lower Upper

75 100

77 50.8 22.9 42.5#

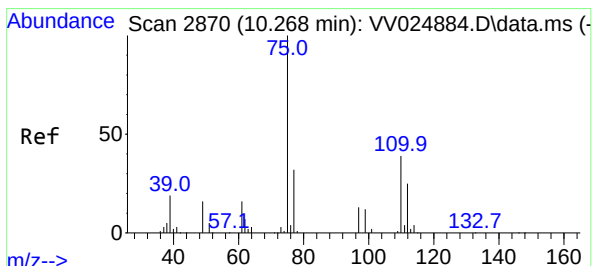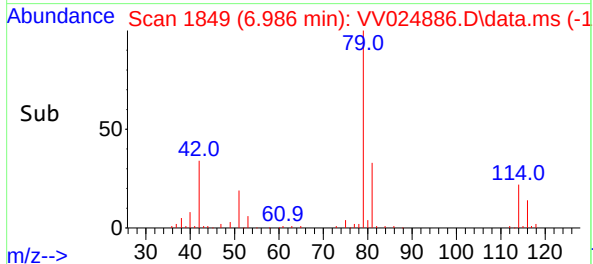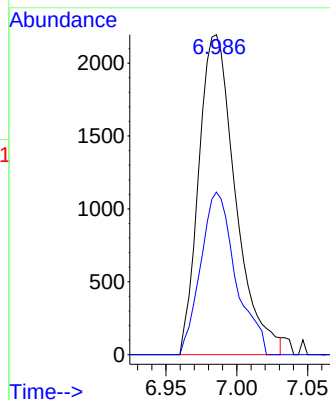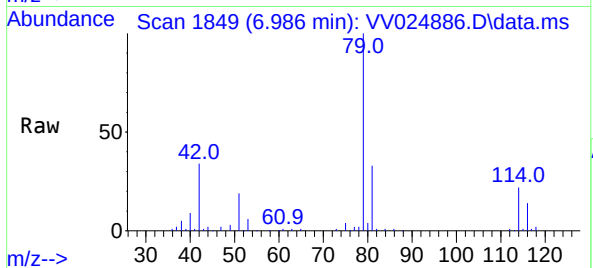

#61

1,2,3-Trichloropropane

Concen: 6.621 ug/L

RT: 11.246 min Scan# 3174

Delta R.T. 0.978 min

Lab File: VV024886.D

Acq: 09 Mar 2022 17:30

Tgt Ion: 75 Resp: 17859

Ion Ratio Lower Upper

75 100

77 31.5 25.4 38.0

110 1.9 31.4 47.2#

