

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024897.D
 Acq On : 10 Mar 2022 01:18
 Operator : SY/MD
 Sample : N1855-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 10 05:52:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	298453	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	293396	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	132450	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	105070	34.623	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.240%
7) Chloroethane-d5	1.568	69	94415	39.655	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.300%
11) 1,1-Dichloroethene-d2	2.108	63	149220	29.296	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.600%#
21) 2-Butanone-d5	3.896	46	160500	92.933	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.930%
24) Chloroform-d	4.349	84	219649	41.463	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.920%
26) 1,2-Dichloroethane-d4	5.031	65	136977	43.823	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.640%
32) Benzene-d6	5.050	84	452940	41.650	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.300%
36) 1,2-Dichloropropane-d6	6.069	67	146900	43.357	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.720%
41) Toluene-d8	7.314	98	395149	41.015	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.020%
43) trans-1,3-Dichloroprop...	7.622	79	58041	39.424	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.840%
47) 2-Hexanone-d5	8.088	63	112966	87.838	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.840%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	179206	44.593	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.180%
66) 1,2-Dichlorobenzene-d4	11.622	152	139223	45.632	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.260%
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	16687	6.296	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024897.D
Acq On : 10 Mar 2022 01:18
Operator : SY/MD
Sample : N1855-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 10 05:52:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 10 05:49:38 2022
Response via : Initial Calibration

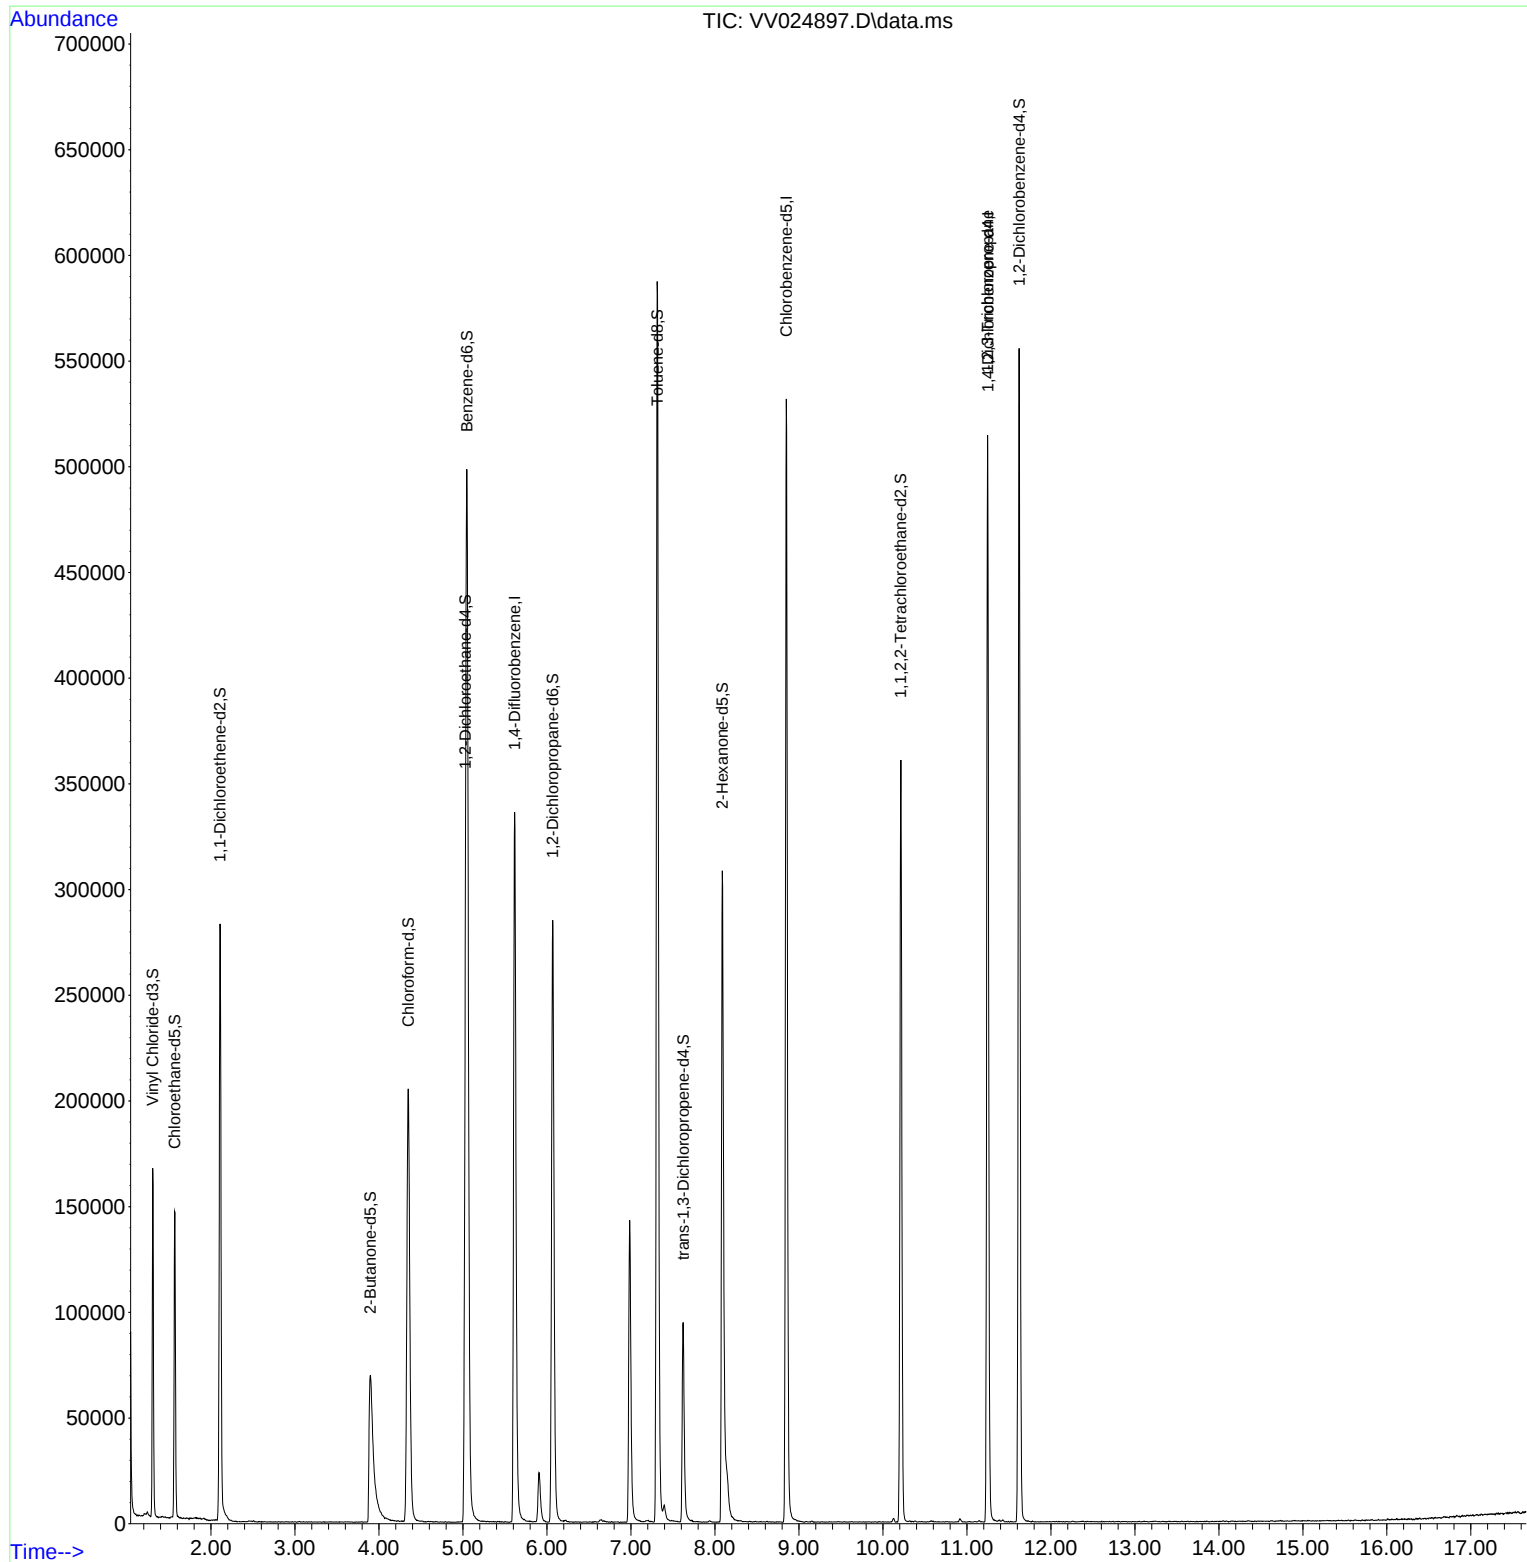

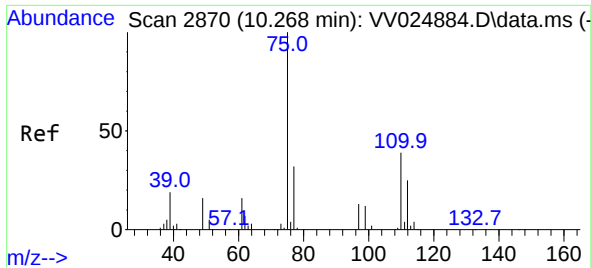

#61
 1,2,3-Trichloropropane
 Concen: 6.296 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV024897.D
 Acq: 10 Mar 2022 01:18

Instrument :
 MSVOA_V
 ClientSampleId :

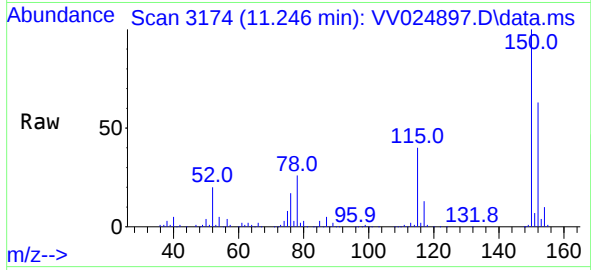

Tgt Ion: 75	Resp: 16687
Ion Ratio	Lower Upper
75	100
77	33.2 25.4 38.0
110	2.5 31.4 47.2#

