




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024891.D
 Acq On : 09 Mar 2022 22:57
 Operator : SY/MD
 Sample : N1856-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D58

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 10 05:51:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

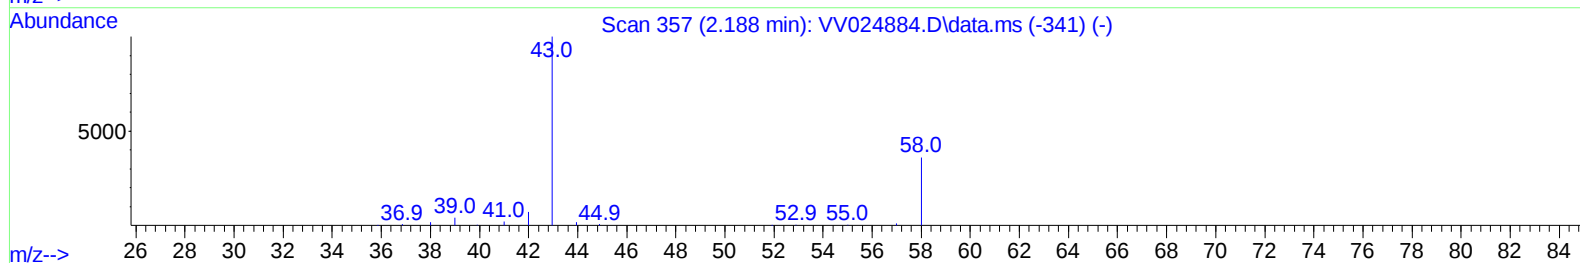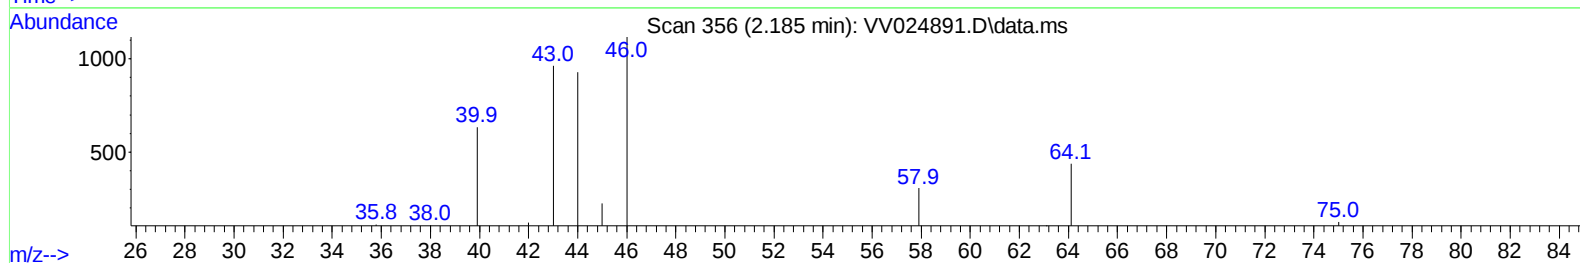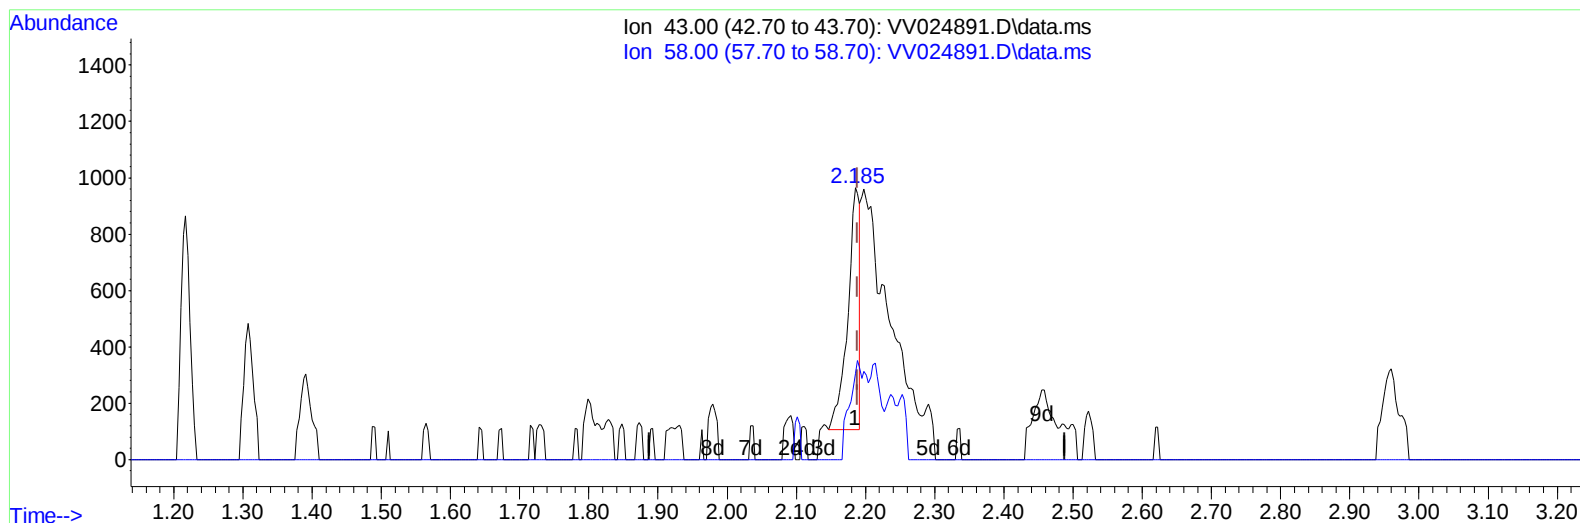

TIC: VV024891.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 0.78 ug/L

response 1042

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	40.98
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024891.D
 Acq On : 09 Mar 2022 22:57
 Operator : SY/MD
 Sample : N1856-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D58

Manual IntegrationsAPPROVED

Quant Time: Mar 10 05:51:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

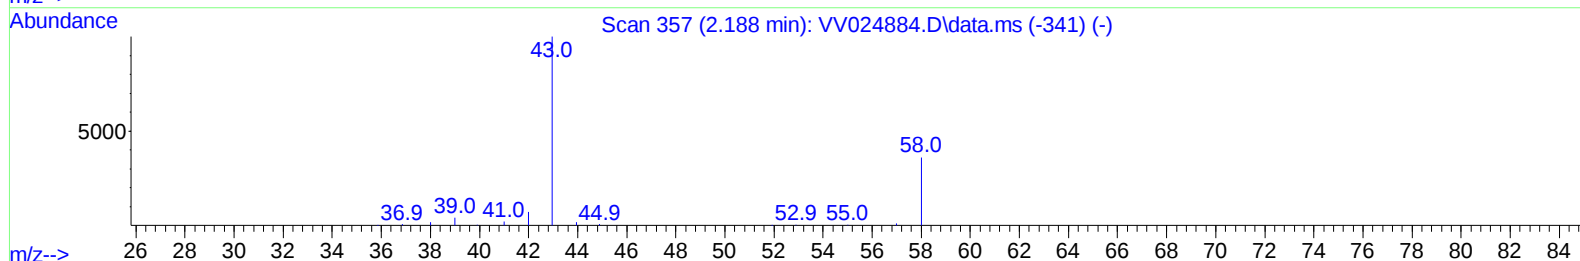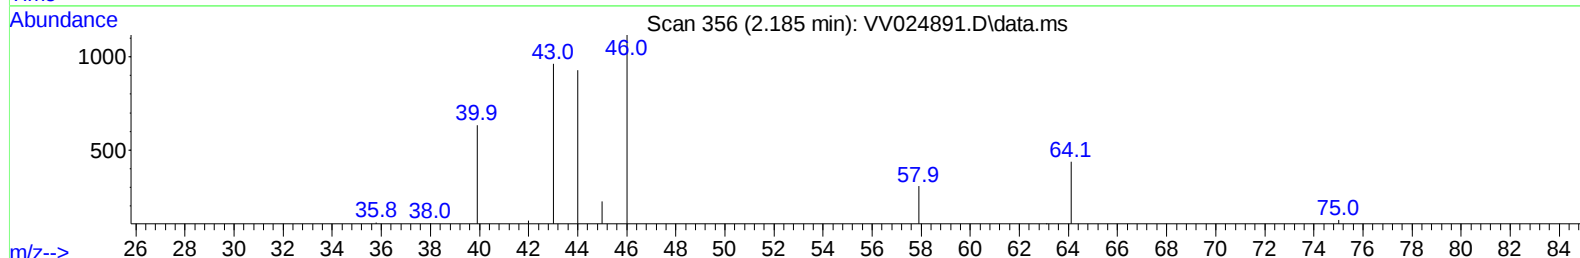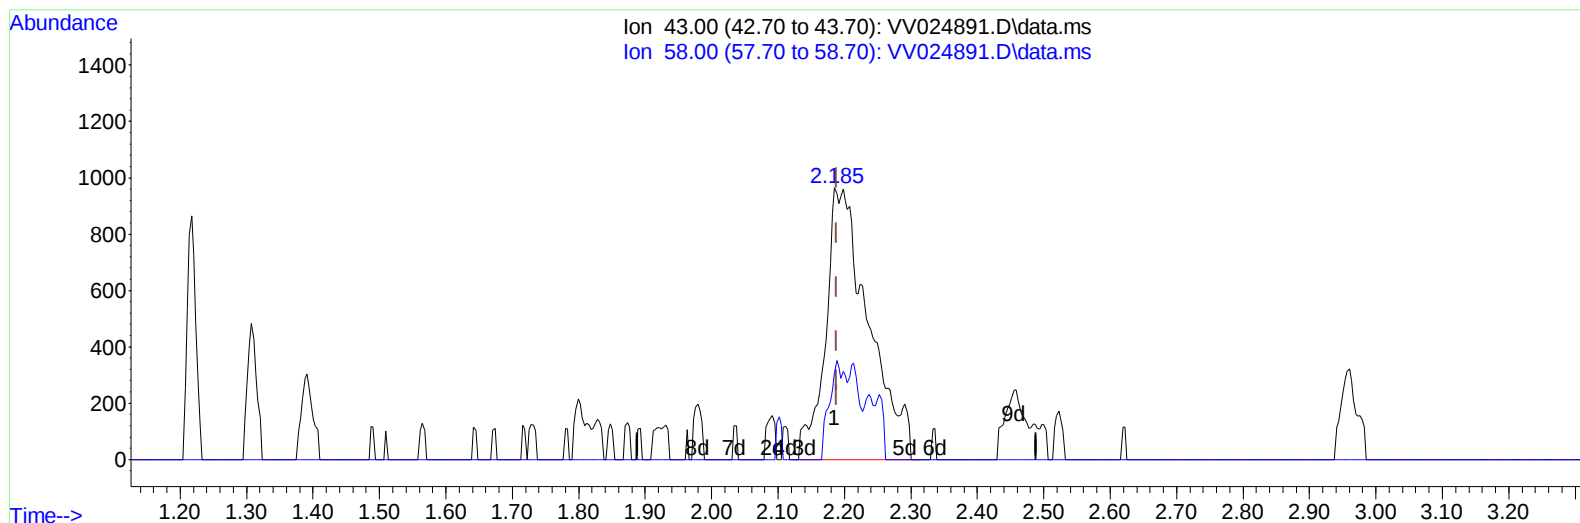

TIC: VV024891.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 3.25 ug/L m

response 4347

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	9.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024891.D
 Acq On : 09 Mar 2022 22:57
 Operator : SY/MD
 Sample : N1856-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D58

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 03/10/2022
 Supervised By : Mahesh Dadoda 03/11/2022

Quant Time: Mar 10 05:51:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	302447	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	294260	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	134097	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	108818	35.384	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	70.760%	
7) Chloroethane-d5	1.568	69	98780	40.940	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	81.880%	
11) 1,1-Dichloroethene-d2	2.108	63	154213	29.876	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	59.760%#	
21) 2-Butanone-d5	3.899	46	162595	92.903	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	92.900%	
24) Chloroform-d	4.349	84	225735	42.049	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.100%	
26) 1,2-Dichloroethane-d4	5.031	65	138695	43.787	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.580%	
32) Benzene-d6	5.050	84	468003	42.909	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.820%	
36) 1,2-Dichloropropane-d6	6.069	67	149258	43.923	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	87.840%	
41) Toluene-d8	7.313	98	405694	41.986	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	83.980%	
43) trans-1,3-Dichloroprop...	7.622	79	59857	40.538	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.080%	
47) 2-Hexanone-d5	8.088	63	115080	89.219	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.220%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	176831	43.873	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.740%	
66) 1,2-Dichlorobenzene-d4	11.622	152	142816	46.234	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.460%	
Target Compounds						
13) Acetone	2.185	43	4347m	3.253	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024891.D
Acq On : 09 Mar 2022 22:57
Operator : SY/MD
Sample : N1856-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0D58

Manual IntegrationsAPPROVED

Quant Time: Mar 10 05:51:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 10 05:49:38 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

