




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 10 05:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

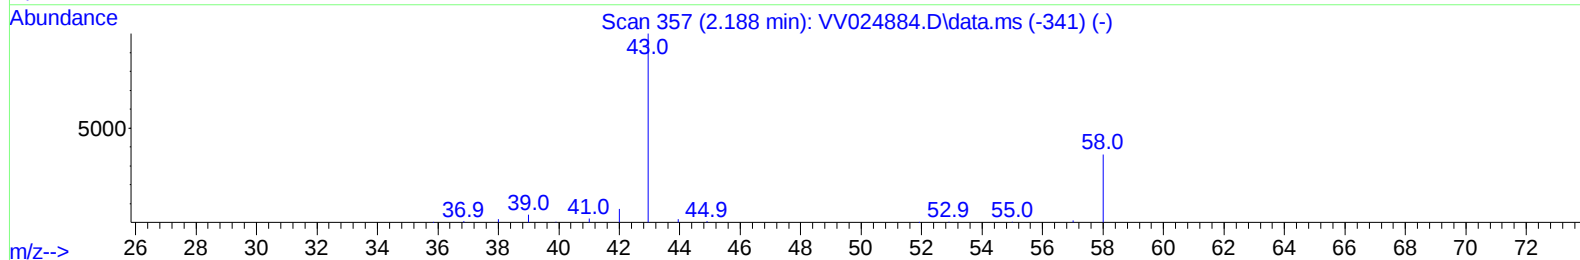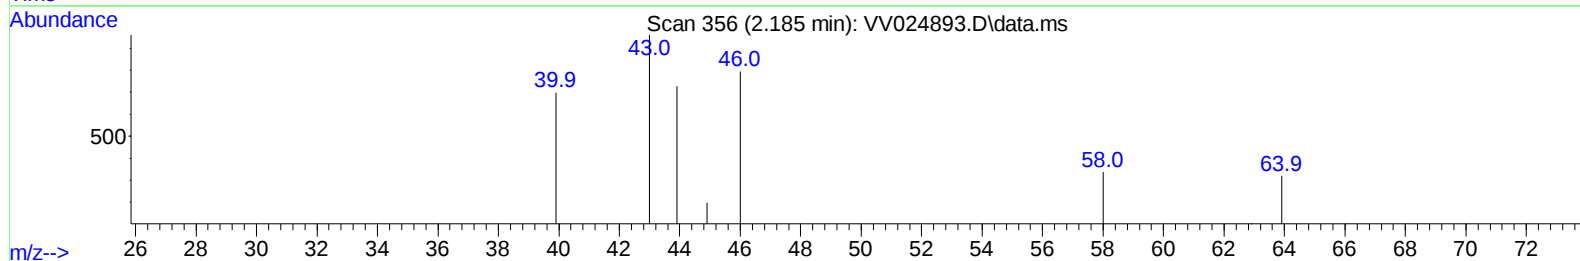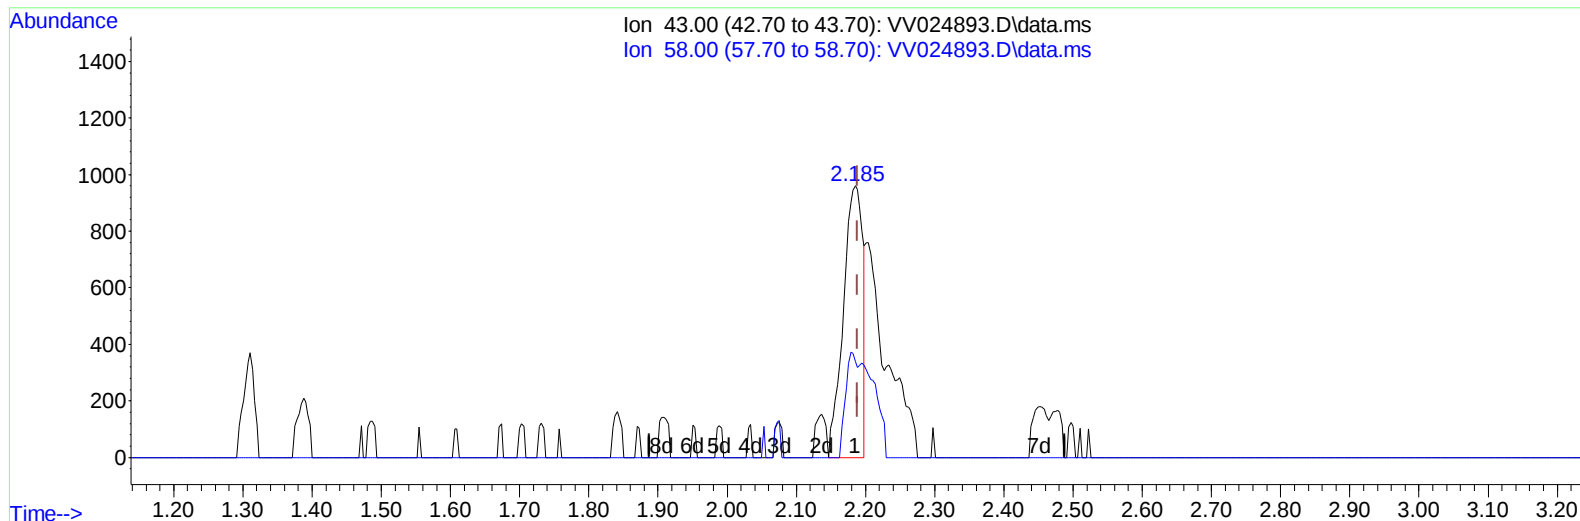

TIC: VV024893.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 1.44 ug/L

response 1877

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	23.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 10 05:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

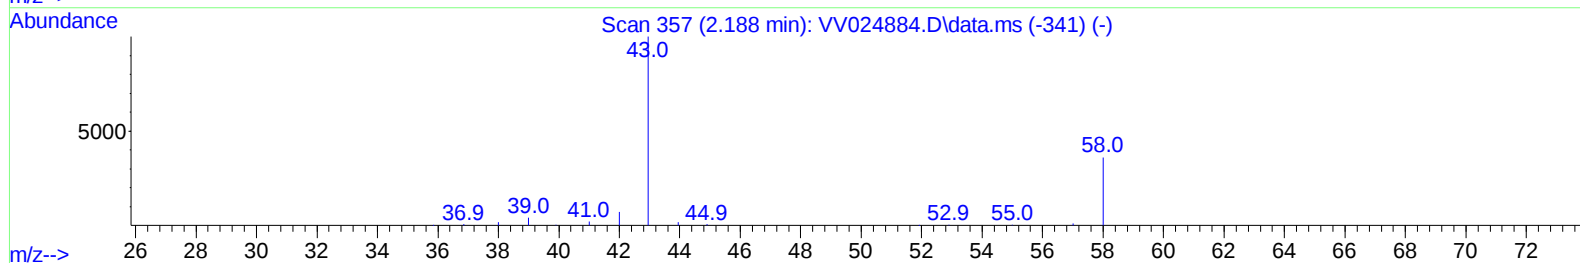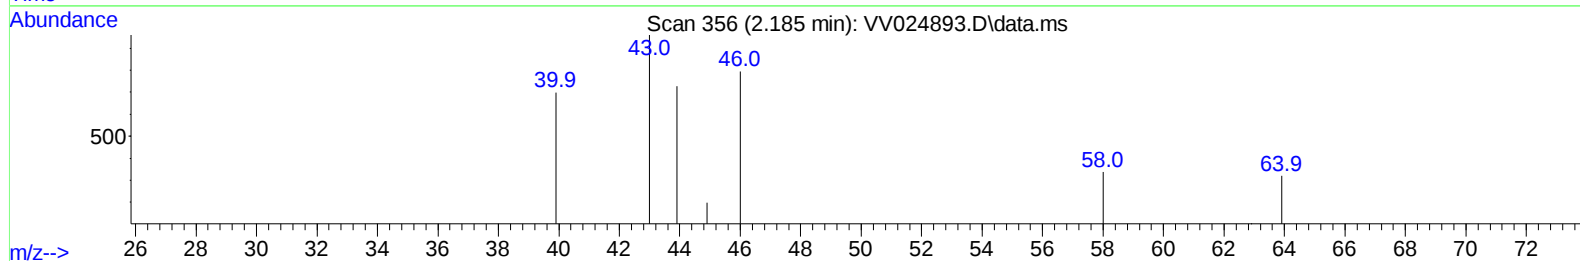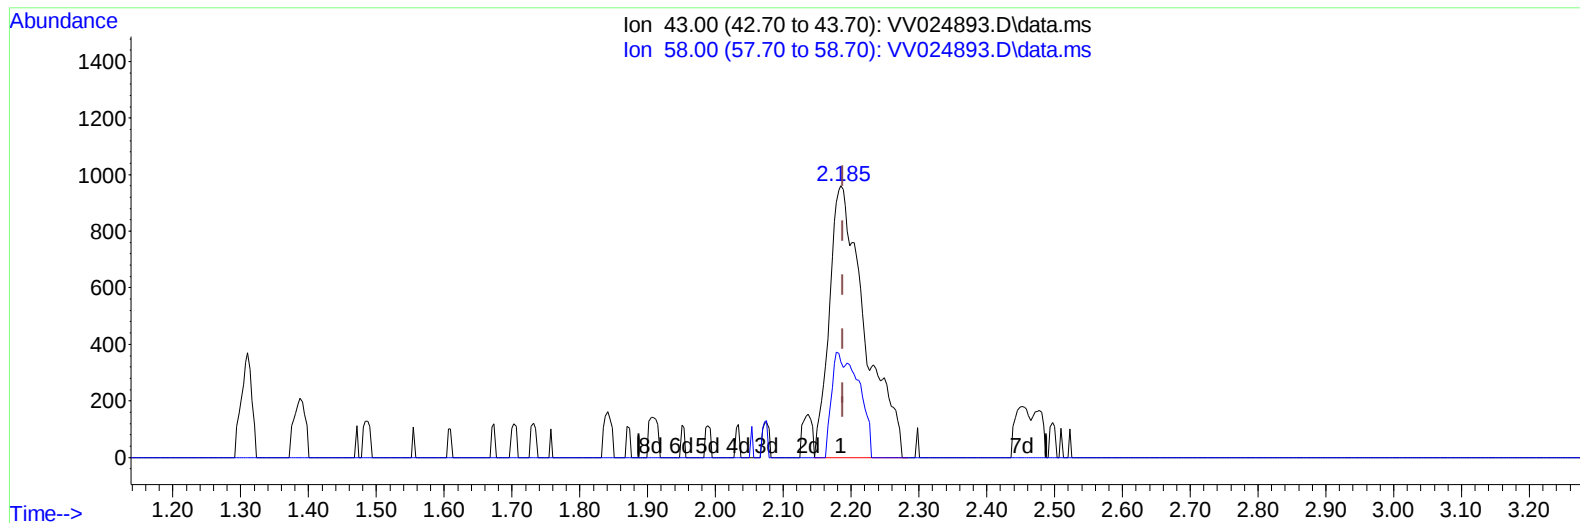

TIC: VV024893.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 2.67 ug/L m

response 3487

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	12.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Manual IntegrationsAPPROVED

Quant Time: Mar 10 05:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	295536	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	285918	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	126413	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	109879	36.565	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	73.120%	
7) Chloroethane-d5	1.568	69	99220	42.084	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	84.160%	
11) 1,1-Dichloroethene-d2	2.108	63	158706	31.466	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	62.940%	
21) 2-Butanone-d5	3.896	46	162337	94.924	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	94.920%	
24) Chloroform-d	4.349	84	230184	43.880	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.760%	
26) 1,2-Dichloroethane-d4	5.031	65	140351	45.346	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.700%	
32) Benzene-d6	5.050	84	476531	44.966	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.940%	
36) 1,2-Dichloropropane-d6	6.069	67	154088	46.668	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	93.340%	
41) Toluene-d8	7.313	98	404334	43.066	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	86.140%	
43) trans-1,3-Dichloroprop...	7.622	79	61014	42.527	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.060%	
47) 2-Hexanone-d5	8.088	63	115232	91.944	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	91.940%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	185129	47.272	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.540%	
66) 1,2-Dichlorobenzene-d4	11.622	152	138520	47.569	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.140%	
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	3487m	2.670	ug/L	
20) cis-1,2-Dichloroethene	3.918	96	2832	1.106	ug/L	97
34) Trichloroethene	5.918	95	9235	3.491	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024893.D
Acq On : 09 Mar 2022 23:44
Operator : SY/MD
Sample : N1856-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0D60

Manual IntegrationsAPPROVED

Quant Time: Mar 10 05:51:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 10 05:49:38 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

