

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030922\
 Data File : VW024896.D
 Acq On : 10 Mar 2022 00:55
 Operator : SY/MD
 Sample : N1855-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D23

Quant Time: Mar 10 05:52:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 10 05:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	305774	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	295583	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	131881	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	104582	33.637	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.280%
7) Chloroethane-d5	1.568	69	96184	39.430	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.860%
11) 1,1-Dichloroethene-d2	2.108	63	150385	28.818	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.640%#
21) 2-Butanone-d5	3.896	46	155264	87.749	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.750%
24) Chloroform-d	4.349	84	222966	41.081	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.160%
26) 1,2-Dichloroethane-d4	5.031	65	135804	42.408	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.820%
32) Benzene-d6	5.050	84	458663	41.864	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.720%
36) 1,2-Dichloropropane-d6	6.069	67	148315	43.450	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.900%
41) Toluene-d8	7.317	98	394409	40.635	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.280%
43) trans-1,3-Dichloroprop...	7.622	79	58470	39.422	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.840%
47) 2-Hexanone-d5	8.088	63	115101	88.836	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.840%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	181042	44.716	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.440%
66) 1,2-Dichlorobenzene-d4	11.622	152	138975	45.747	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.500%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.915	95	18002	6.583	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024896.D
Acq On : 10 Mar 2022 00:55
Operator : SY/MD
Sample : N1855-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D23


Quant Time: Mar 10 05:52:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 10 05:49:38 2022
Response via : Initial Calibration

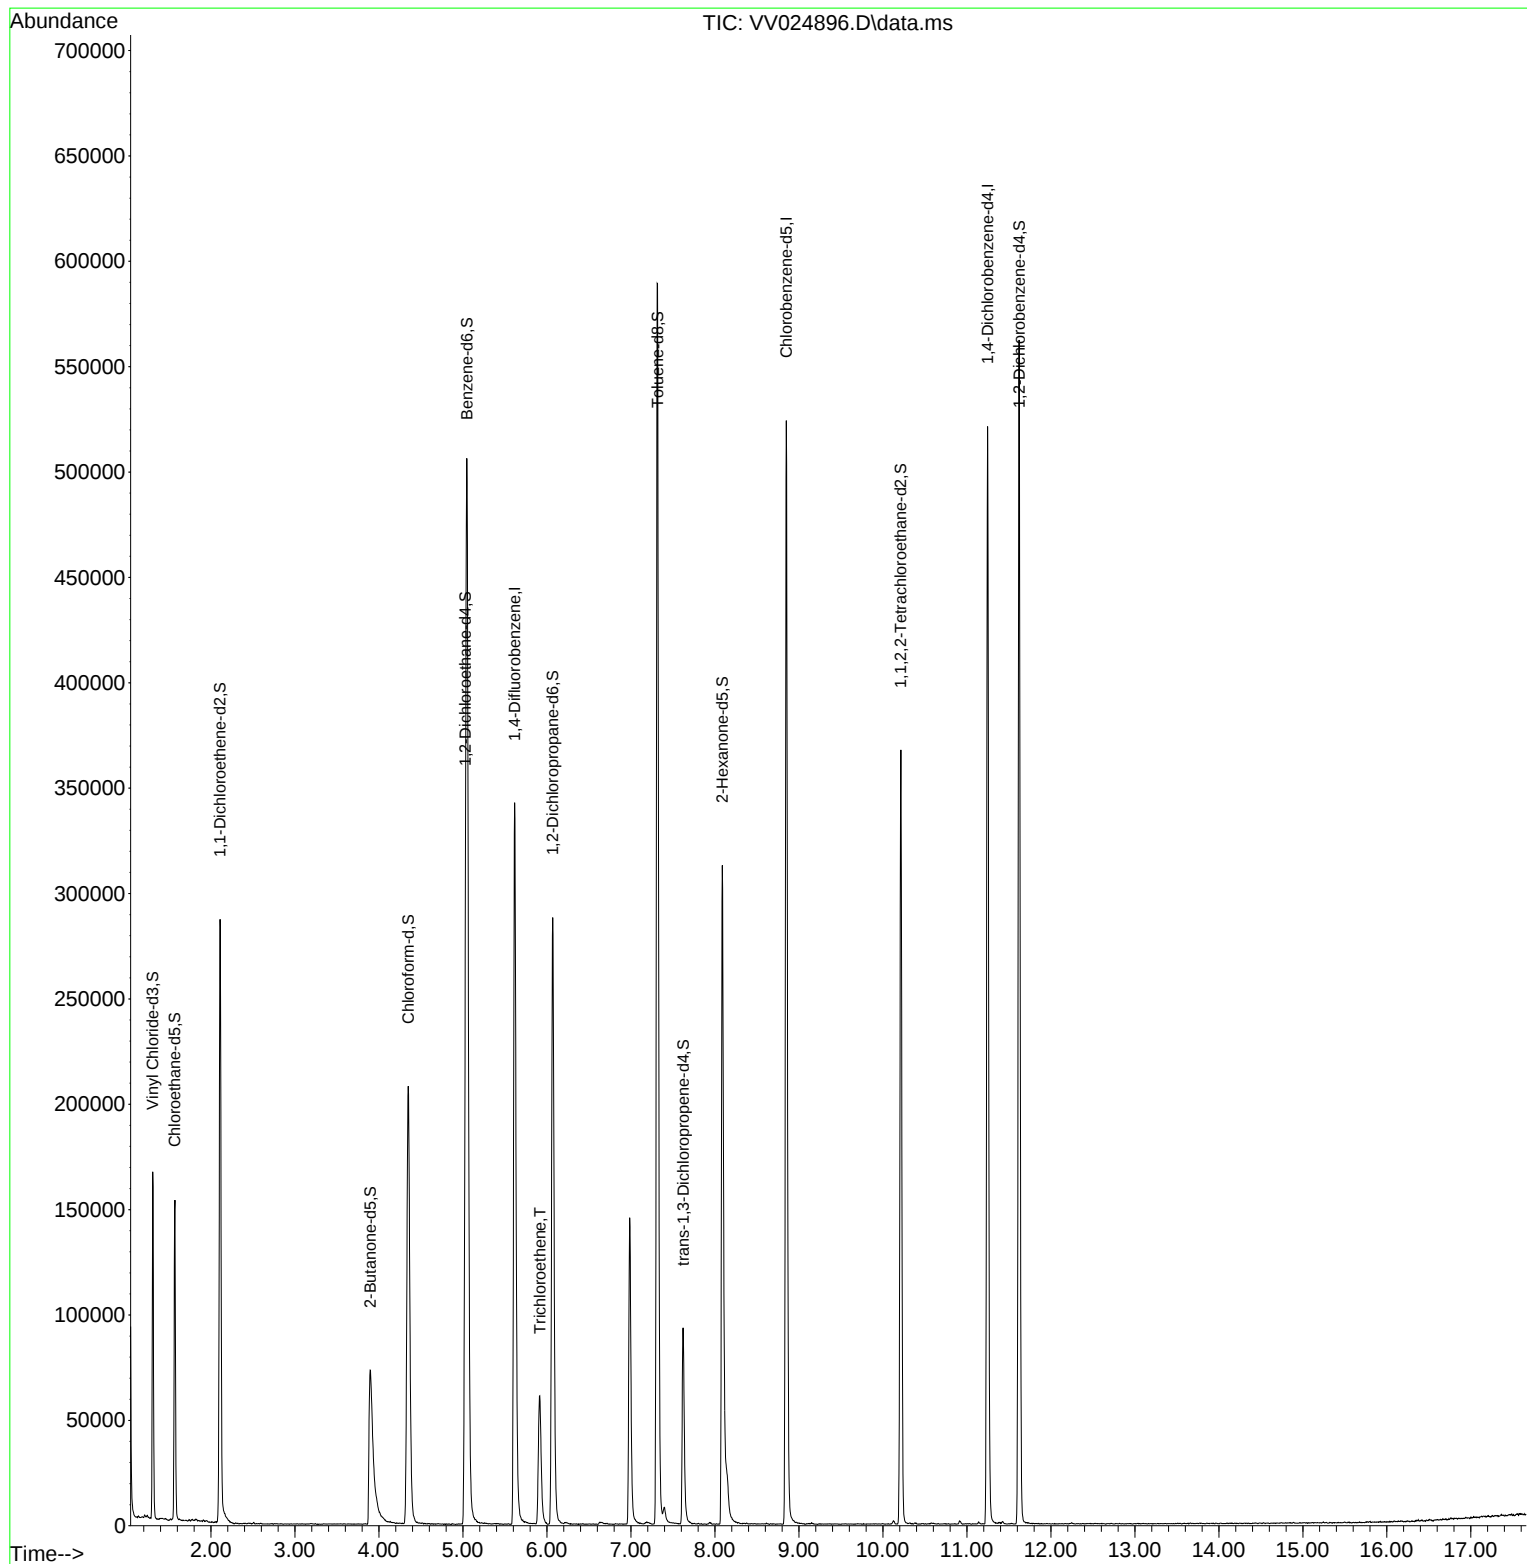

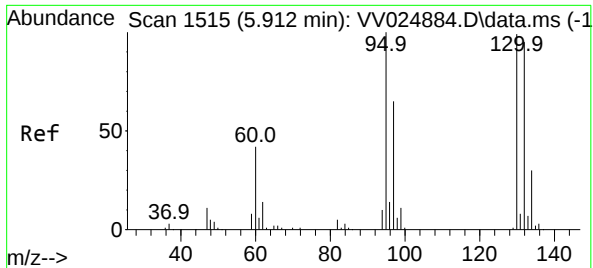

#34
 Trichloroethene
 Concen: 6.583 ug/L
 RT: 5.915 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VV024896.D
 Acq: 10 Mar 2022 00:55

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D23

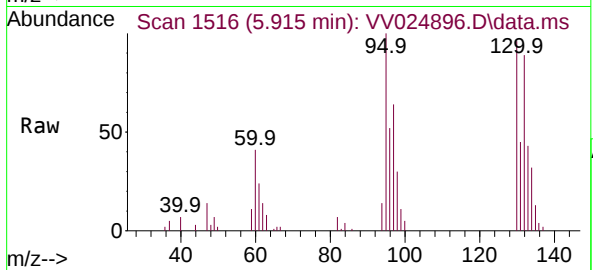

Tgt Ion:	95	Resp:	18002
Ion	Ratio	Lower	Upper
95	100		
97	63.9	45.3	84.1
132	88.6	65.0	120.6
130	96.0	69.3	128.7

