

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024889.D
 Acq On : 09 Mar 2022 22:10
 Operator : SY/MD
 Sample : N1856-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	171423	173964	13.48%	1.869%
2	1.568	156	164	176	rVB	151625	169406	13.13%	1.820%
3	2.105	320	331	360	rBV	290175	430443	33.36%	4.624%
4	2.417	426	428	432	rVB2	300	162	0.01%	0.002%
5	2.500	452	454	458	rBV4	391	376	0.03%	0.004%
6	2.642	495	498	502	rBV2	241	191	0.01%	0.002%
7	2.822	550	554	557	rBV2	221	186	0.01%	0.002%
8	2.928	583	587	589	rBV	182	132	0.01%	0.001%
9	3.044	620	623	625	rBV2	177	115	0.01%	0.001%
10	3.108	640	643	645	rBV2	139	100	0.01%	0.001%
11	3.375	723	726	730	rBV2	142	84	0.01%	0.001%
12	3.581	787	790	793	rBV	224	145	0.01%	0.002%
13	3.597	793	795	798	rBV2	103	83	0.01%	0.001%
14	3.632	803	806	812	rBV2	228	203	0.02%	0.002%
15	3.661	812	815	817	rBV2	164	109	0.01%	0.001%
16	3.690	822	824	827	rVB2	128	63	0.00%	0.001%
17	3.741	836	840	842	rBV	126	105	0.01%	0.001%
18	3.783	850	853	858	rBV	241	205	0.02%	0.002%
19	3.809	858	861	863	rBV2	201	124	0.01%	0.001%
20	3.899	877	889	935	rBV	63455	253103	19.62%	2.719%
21	4.346	1011	1028	1058	rBV	208976	524916	40.68%	5.639%
22	4.564	1094	1096	1099	rBV2	178	81	0.01%	0.001%
23	4.619	1111	1113	1118	rVB2	285	177	0.01%	0.002%
24	4.645	1118	1121	1122	rVB2	150	66	0.01%	0.001%
25	4.664	1122	1127	1133	rBV	270	308	0.02%	0.003%
26	4.728	1144	1147	1151	rVB	241	173	0.01%	0.002%
27	4.770	1156	1160	1162	rBV2	215	147	0.01%	0.002%
28	4.809	1170	1172	1175	rVB3	208	116	0.01%	0.001%
29	4.844	1175	1183	1185	rBV2	281	253	0.02%	0.003%
30	4.931	1202	1210	1211	rBV2	191	248	0.02%	0.003%
31	5.044	1228	1245	1277	rBV2	507175	1290304	100.00%	13.862%
32	5.445	1365	1370	1373	rVB3	222	230	0.02%	0.002%
33	5.490	1380	1384	1385	rBV	201	117	0.01%	0.001%
34	5.513	1389	1391	1394	rVB	134	72	0.01%	0.001%
35	5.548	1399	1402	1406	rBV	150	100	0.01%	0.001%
36	5.571	1406	1409	1411	rBV	98	69	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024889.D
 Acq On : 09 Mar 2022 22:10
 Operator : SY/MD
 Sample : N1856-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	5.616	1411	1423	1450	rBV	333667	667985	51.77%	7.176%
38	5.857	1495	1498	1502	rBV2	269	268	0.02%	0.003%
39	5.908	1502	1514	1538	rVV6	45445	108581	8.42%	1.166%
40	6.066	1550	1563	1584	rBV	282725	578537	44.84%	6.215%
41	6.310	1636	1639	1641	rBV2	115	70	0.01%	0.001%
42	6.352	1649	1652	1653	rBV	174	99	0.01%	0.001%
43	6.442	1676	1680	1682	rBV2	170	116	0.01%	0.001%
44	6.497	1694	1697	1699	rBV	244	146	0.01%	0.002%
45	6.539	1707	1710	1711	rBV	117	64	0.00%	0.001%
46	6.603	1726	1730	1732	rVV	230	145	0.01%	0.002%
47	6.732	1766	1770	1771	rBV	254	165	0.01%	0.002%
48	6.744	1771	1774	1777	rVV3	447	289	0.02%	0.003%
49	6.773	1777	1783	1787	rVV2	255	239	0.02%	0.003%
50	6.834	1799	1802	1805	rBV	195	135	0.01%	0.001%
51	6.857	1806	1809	1812	rVV	131	89	0.01%	0.001%
52	6.886	1815	1818	1820	rBV2	131	85	0.01%	0.001%
53	6.934	1830	1833	1836	rBV	164	102	0.01%	0.001%
54	6.986	1837	1849	1879	rBV	145432	266576	20.66%	2.864%
55	7.314	1939	1951	1970	rBV	593361	1025807	79.50%	11.020%
56	7.619	2037	2046	2075	rBV	95802	166863	12.93%	1.793%
57	7.786	2095	2098	2102	rBV2	298	247	0.02%	0.003%
58	7.854	2116	2119	2123	rVB2	229	163	0.01%	0.002%
59	7.886	2123	2129	2134	rBV2	260	338	0.03%	0.004%
60	7.931	2139	2143	2146	rBV2	319	339	0.03%	0.004%
61	8.088	2182	2192	2234	rBV	299329	592999	45.96%	6.371%
62	8.346	2269	2272	2277	rBV3	447	347	0.03%	0.004%
63	8.477	2310	2313	2317	rVB3	255	174	0.01%	0.002%
64	8.506	2320	2322	2324	rBV	234	109	0.01%	0.001%
65	8.532	2325	2330	2335	rVB3	255	245	0.02%	0.003%
66	8.606	2351	2353	2356	rBV	245	181	0.01%	0.002%
67	8.641	2361	2364	2366	rBV2	185	123	0.01%	0.001%
68	8.770	2402	2404	2409	rVB2	208	137	0.01%	0.001%
69	8.805	2409	2415	2418	rBV	196	193	0.01%	0.002%
70	8.850	2418	2429	2462	rBV	507050	831687	64.46%	8.935%
71	9.066	2494	2496	2499	rBV	213	78	0.01%	0.001%
72	9.153	2517	2523	2525	rBV3	495	562	0.04%	0.006%
73	9.182	2530	2532	2534	rBV	114	70	0.01%	0.001%
74	9.349	2582	2584	2587	rBV	159	90	0.01%	0.001%
75	9.371	2587	2591	2593	rBV2	142	129	0.01%	0.001%
76	9.400	2597	2600	2602	rBV	141	71	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024889.D
 Acq On : 09 Mar 2022 22:10
 Operator : SY/MD
 Sample : N1856-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	9.416	2602	2605	2607	rBV	148	81	0.01%	0.001%
78	9.465	2617	2620	2622	rBV	108	74	0.01%	0.001%
79	9.545	2642	2645	2647	rVB	183	99	0.01%	0.001%
80	9.629	2666	2671	2673	rBV2	135	136	0.01%	0.001%
81	9.722	2696	2700	2703	rBV2	277	212	0.02%	0.002%
82	9.834	2733	2735	2738	rBV2	128	91	0.01%	0.001%
83	10.047	2795	2801	2804	rBV2	209	263	0.02%	0.003%
84	10.124	2818	2825	2831	rBV4	1714	2466	0.19%	0.026%
85	10.214	2840	2853	2873	rBV	357756	561590	43.52%	6.033%
86	10.384	2903	2906	2912	rVB3	346	266	0.02%	0.003%
87	10.423	2914	2918	2922	rBV2	195	200	0.02%	0.002%
88	10.551	2955	2958	2962	rBV2	280	178	0.01%	0.002%
89	10.883	3055	3061	3064	rBV2	322	390	0.03%	0.004%
90	10.921	3066	3073	3078	rVB6	1131	1721	0.13%	0.018%
91	11.030	3102	3107	3111	rVB3	369	363	0.03%	0.004%
92	11.149	3138	3144	3148	rBV2	629	736	0.06%	0.008%
93	11.201	3157	3160	3162	rBV	355	236	0.02%	0.003%
94	11.246	3162	3174	3195	rVV	506068	779358	60.40%	8.373%
95	11.532	3261	3263	3264	rBV	269	99	0.01%	0.001%
96	11.622	3279	3291	3312	rBV	556569	867711	67.25%	9.322%
97	13.117	3753	3756	3758	rBV	222	142	0.01%	0.002%
98	13.458	3858	3862	3866	rBV	357	320	0.02%	0.003%
99	13.796	3965	3967	3969	rBV	269	123	0.01%	0.001%
100	14.432	4162	4165	4167	rBV	344	250	0.02%	0.003%




Sum of corrected areas: 9308424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024889.D
Acq On : 09 Mar 2022 22:10
Operator : SY/MD
Sample : N1856-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

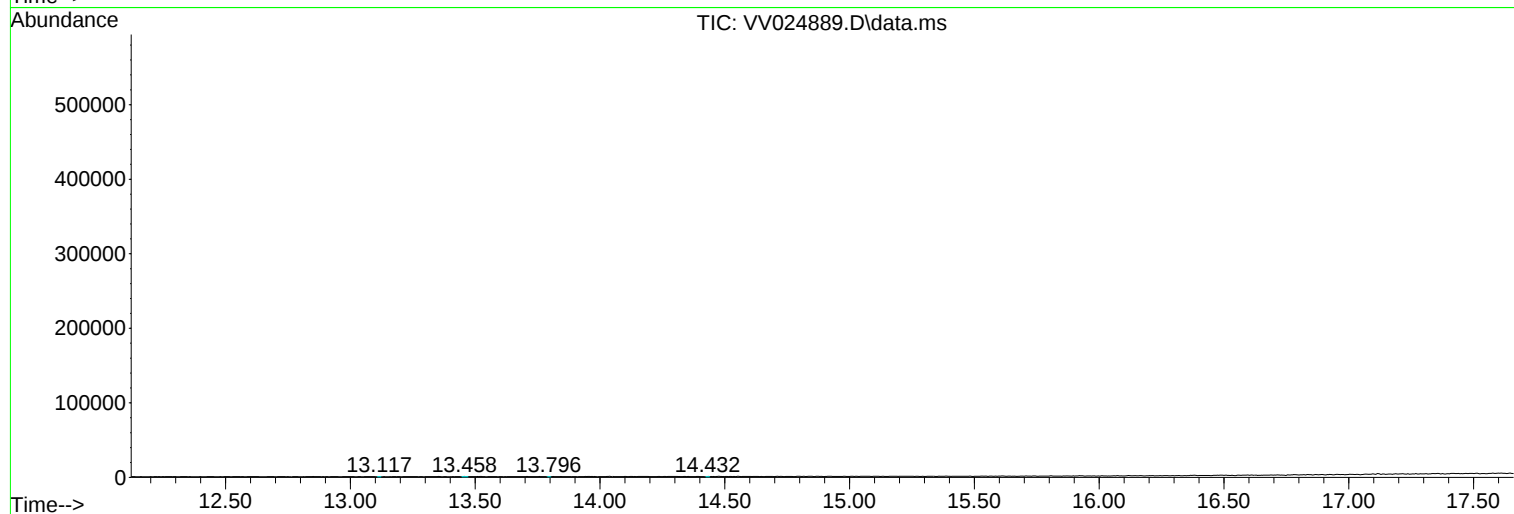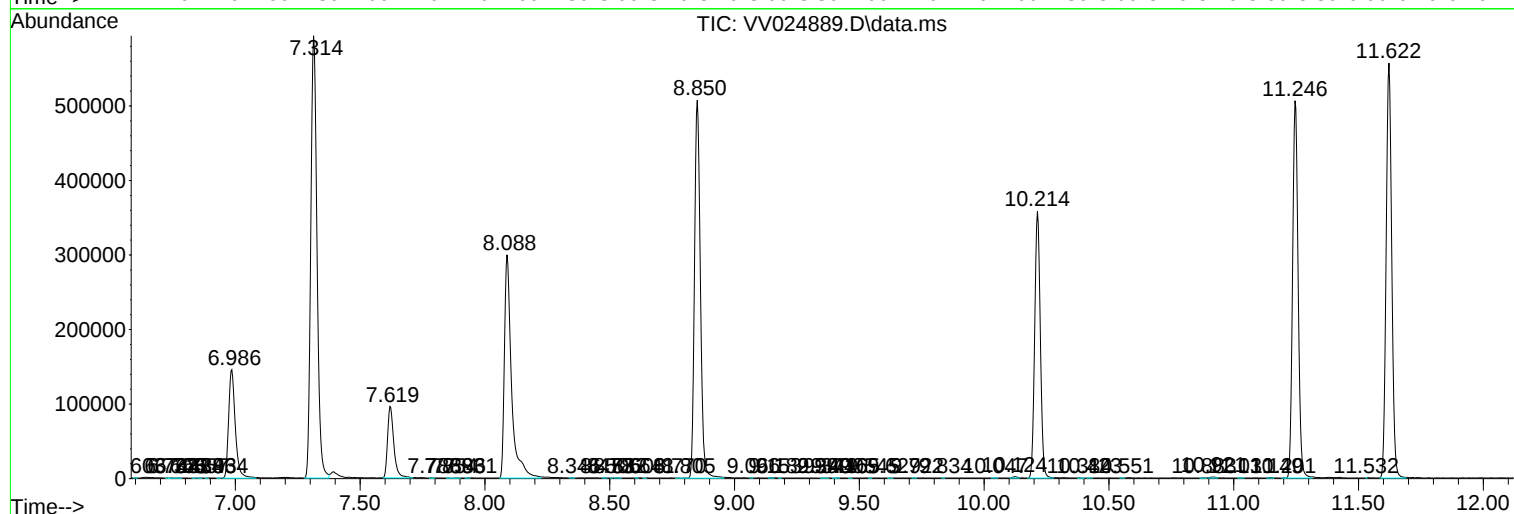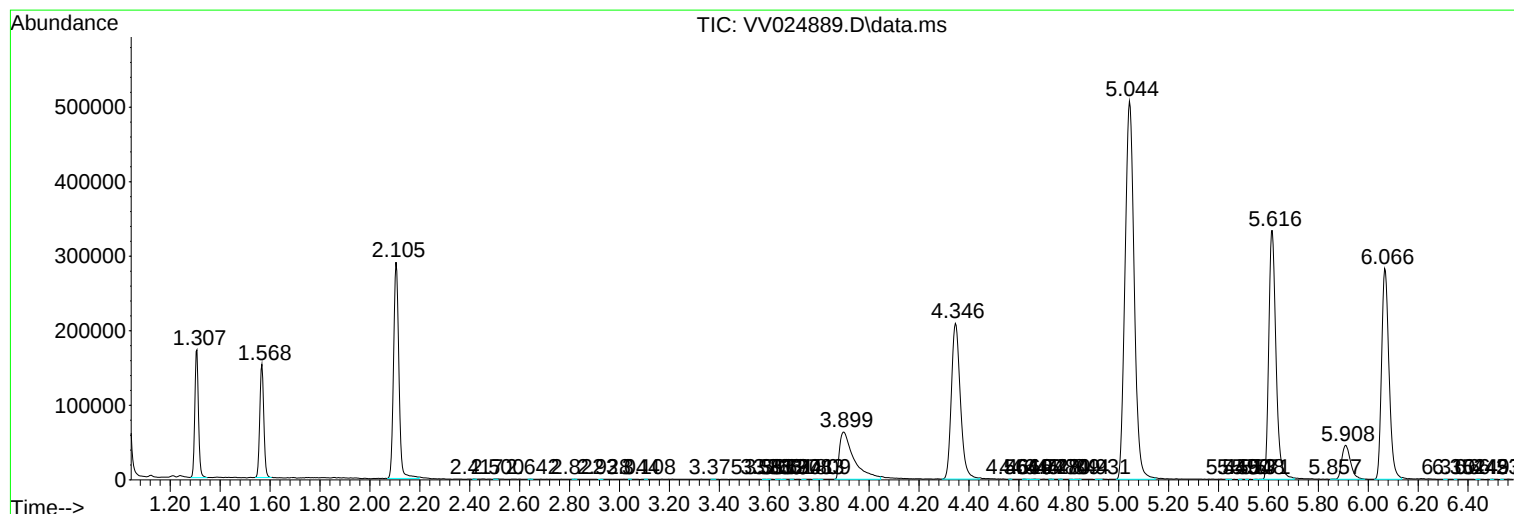

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024889.D
Acq On : 09 Mar 2022 22:10
Operator : SY/MD
Sample : N1856-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024889.D
Acq On : 09 Mar 2022 22:10
Operator : SY/MD
Sample : N1856-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc