

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M

Title : VOC Analysis

Signal : TIC: VV024893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	172889	177028	13.24%	1.854%
2	1.568	157	164	179	rVB	150089	173318	12.96%	1.816%
3	2.056	313	316	320	rBV2	512	551	0.04%	0.006%
4	2.108	321	332	361	rVV	301113	456642	34.15%	4.784%
5	2.445	433	437	441	rBV2	296	298	0.02%	0.003%
6	2.510	450	457	464	rBV5	693	839	0.06%	0.009%
7	2.603	483	486	493	rVB2	176	201	0.02%	0.002%
8	2.635	493	496	503	rBV2	280	321	0.02%	0.003%
9	2.931	584	588	591	rBV2	234	183	0.01%	0.002%
10	3.044	618	623	626	rBV	216	235	0.02%	0.002%
11	3.185	663	667	672	rBV2	240	192	0.01%	0.002%
12	3.744	838	841	846	rVB2	198	203	0.02%	0.002%
13	3.777	846	851	854	rBV2	186	204	0.02%	0.002%
14	3.896	877	888	936	rBV	78379	282190	21.10%	2.956%
15	4.349	1012	1029	1058	rBV	216221	530666	39.68%	5.559%
16	4.474	1066	1068	1073	rVB3	524	399	0.03%	0.004%
17	4.609	1100	1110	1123	rVB7	2538	5973	0.45%	0.063%
18	4.687	1128	1134	1136	rBV	214	235	0.02%	0.002%
19	4.780	1159	1163	1165	rBV	272	209	0.02%	0.002%
20	4.969	1218	1222	1228	rBV2	175	216	0.02%	0.002%
21	5.047	1228	1246	1278	rBV2	527529	1337253	100.00%	14.008%
22	5.452	1369	1372	1376	rVB2	317	265	0.02%	0.003%
23	5.616	1411	1423	1449	rBV	336026	669300	50.05%	7.011%
24	5.912	1502	1515	1542	rVB5	42012	100900	7.55%	1.057%
25	6.069	1550	1564	1589	rBV	299280	606111	45.33%	6.349%
26	6.207	1602	1607	1609	rBV3	625	499	0.04%	0.005%
27	6.249	1618	1620	1627	rVB2	407	374	0.03%	0.004%
28	6.288	1627	1632	1634	rBV	258	199	0.01%	0.002%
29	6.445	1677	1681	1684	rBV2	186	175	0.01%	0.002%
30	6.567	1713	1719	1720	rBV2	208	203	0.02%	0.002%
31	6.645	1733	1743	1746	rBV4	1398	2332	0.17%	0.024%
32	6.985	1838	1849	1872	rBV	152492	273608	20.46%	2.866%
33	7.172	1905	1907	1909	rBV3	578	361	0.03%	0.004%
34	7.313	1935	1951	1970	rBV	600080	1049556	78.49%	10.995%
35	7.619	2037	2046	2072	rVV	100302	173094	12.94%	1.813%
36	7.770	2090	2093	2098	rVB4	343	337	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	7.940	2137	2146	2155	rBV2	1396	2444	0.18%	0.026%
38	8.088	2181	2192	2237	rBV	316126	615053	45.99%	6.443%
39	8.419	2290	2295	2300	rBV2	320	363	0.03%	0.004%
40	8.477	2305	2313	2314	rBV	382	350	0.03%	0.004%
41	8.622	2353	2358	2361	rVV4	533	453	0.03%	0.005%
42	8.706	2380	2384	2387	rVV2	201	183	0.01%	0.002%
43	8.722	2387	2389	2397	rVB2	236	215	0.02%	0.002%
44	8.850	2418	2429	2453	rBV	512602	826786	61.83%	8.661%
45	9.114	2509	2511	2514	rVB2	528	256	0.02%	0.003%
46	9.304	2566	2570	2576	rBV2	214	234	0.02%	0.002%
47	9.419	2603	2606	2610	rVB	317	201	0.02%	0.002%
48	9.471	2619	2622	2628	rVB	264	237	0.02%	0.002%
49	9.558	2643	2649	2651	rBV2	270	208	0.02%	0.002%
50	9.574	2651	2654	2659	rBV	230	205	0.02%	0.002%
51	9.821	2724	2731	2736	rBV2	214	314	0.02%	0.003%
52	10.124	2819	2825	2836	rVB5	2029	2972	0.22%	0.031%
53	10.214	2841	2853	2874	rBV	375498	585265	43.77%	6.131%
54	10.317	2882	2885	2889	rBV2	400	413	0.03%	0.004%
55	10.349	2893	2895	2898	rVV2	740	586	0.04%	0.006%
56	10.378	2901	2904	2912	rVB5	1616	1855	0.14%	0.019%
57	10.423	2912	2918	2922	rBV2	230	276	0.02%	0.003%
58	10.513	2939	2946	2955	rVV4	1388	2334	0.17%	0.024%
59	10.577	2960	2966	2969	rBV4	807	809	0.06%	0.008%
60	10.651	2984	2989	2991	rVV2	190	176	0.01%	0.002%
61	10.696	3000	3003	3009	rVB2	241	197	0.01%	0.002%
62	10.799	3031	3035	3039	rBV2	279	216	0.02%	0.002%
63	10.828	3039	3044	3048	rVV3	265	267	0.02%	0.003%
64	10.870	3053	3057	3062	rBV2	283	306	0.02%	0.003%
65	10.915	3062	3071	3078	rBV5	1700	2785	0.21%	0.029%
66	11.056	3113	3115	3119	rVB	333	231	0.02%	0.002%
67	11.098	3121	3128	3130	rBV2	249	266	0.02%	0.003%
68	11.140	3134	3141	3149	rVB3	987	1340	0.10%	0.014%
69	11.246	3163	3174	3193	rBV	502130	760085	56.84%	7.962%
70	11.371	3211	3213	3215	rBV2	310	203	0.02%	0.002%
71	11.426	3224	3230	3236	rVV5	1374	1710	0.13%	0.018%
72	11.532	3254	3263	3279	rBV2	9402	17870	1.34%	0.187%
73	11.622	3279	3291	3311	rVV	553869	866848	64.82%	9.081%
74	11.731	3323	3325	3328	rBV3	313	192	0.01%	0.002%
75	11.757	3331	3333	3336	rBV2	336	251	0.02%	0.003%
76	11.779	3337	3340	3347	rVB4	795	824	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024893.D
 Acq On : 09 Mar 2022 23:44
 Operator : SY/MD
 Sample : N1856-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.815	3347	3351	3355	rBV2	298	311	0.02%	0.003%
78	11.834	3355	3357	3359	rVV	380	238	0.02%	0.002%
79	11.956	3392	3395	3399	rVB	253	186	0.01%	0.002%
80	12.046	3415	3423	3426	rBV2	244	346	0.03%	0.004%
81	12.088	3432	3436	3438	rBV	399	289	0.02%	0.003%
82	12.410	3532	3536	3541	rBV2	319	278	0.02%	0.003%
83	12.519	3567	3570	3574	rVB	268	175	0.01%	0.002%
84	12.554	3577	3581	3585	rBV	283	248	0.02%	0.003%
85	12.738	3633	3638	3641	rBV	201	213	0.02%	0.002%
86	13.262	3799	3801	3805	rVB	309	203	0.02%	0.002%
87	13.377	3834	3837	3840	rBV2	204	177	0.01%	0.002%
88	13.480	3863	3869	3872	rBV	205	238	0.02%	0.002%
89	13.509	3876	3878	3883	rVV2	315	240	0.02%	0.003%
90	13.654	3919	3923	3924	rBV	262	180	0.01%	0.002%
91	13.860	3984	3987	3990	rBV2	275	177	0.01%	0.002%
92	13.879	3990	3993	3995	rBV	277	180	0.01%	0.002%
93	13.931	4006	4009	4012	rBV2	279	189	0.01%	0.002%
94	14.037	4039	4042	4046	rVB	410	339	0.03%	0.004%
95	14.152	4074	4078	4079	rBV	286	177	0.01%	0.002%
96	14.226	4098	4101	4104	rBV	271	214	0.02%	0.002%
97	14.287	4116	4120	4121	rBV	262	176	0.01%	0.002%
98	14.374	4144	4147	4149	rBV	298	197	0.01%	0.002%
99	15.197	4401	4403	4406	rBV	356	194	0.01%	0.002%
100	15.943	4632	4635	4641	rVB3	663	475	0.04%	0.005%




Sum of corrected areas: 9546089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024893.D
Acq On : 09 Mar 2022 23:44
Operator : SY/MD
Sample : N1856-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COD60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

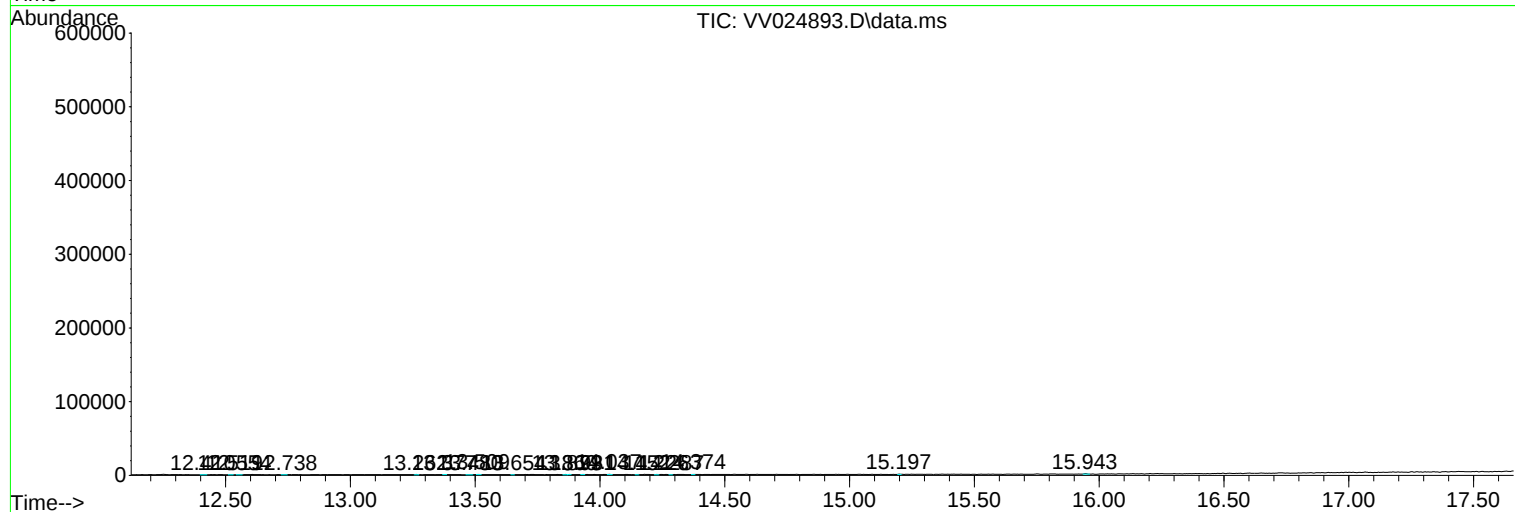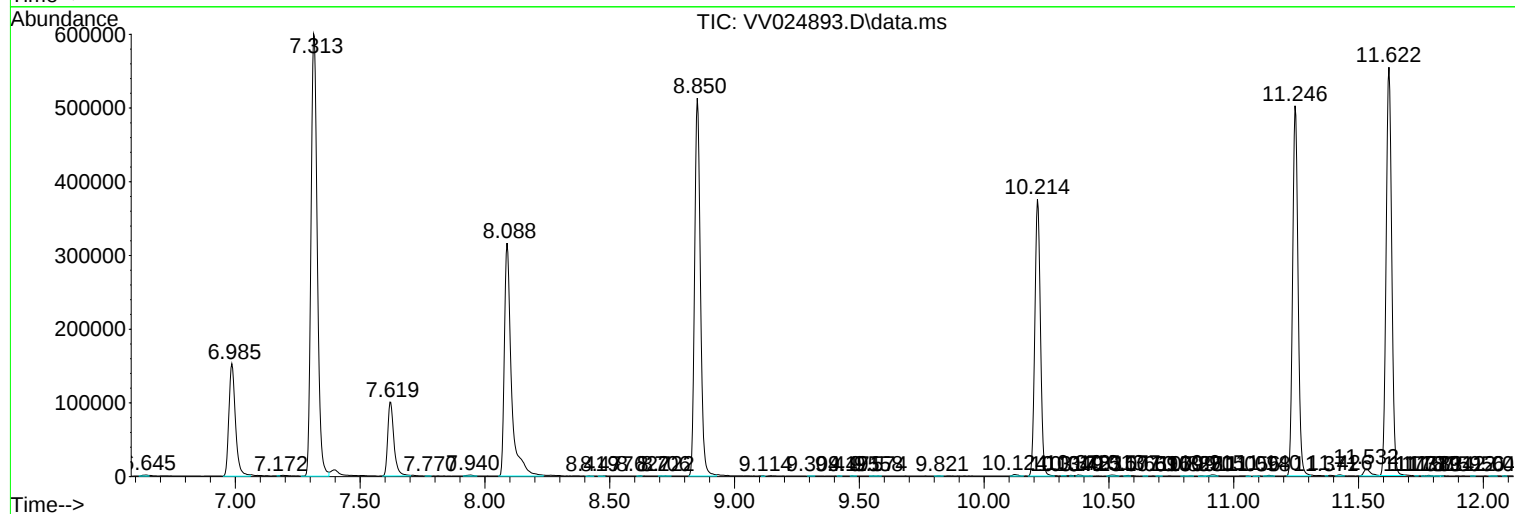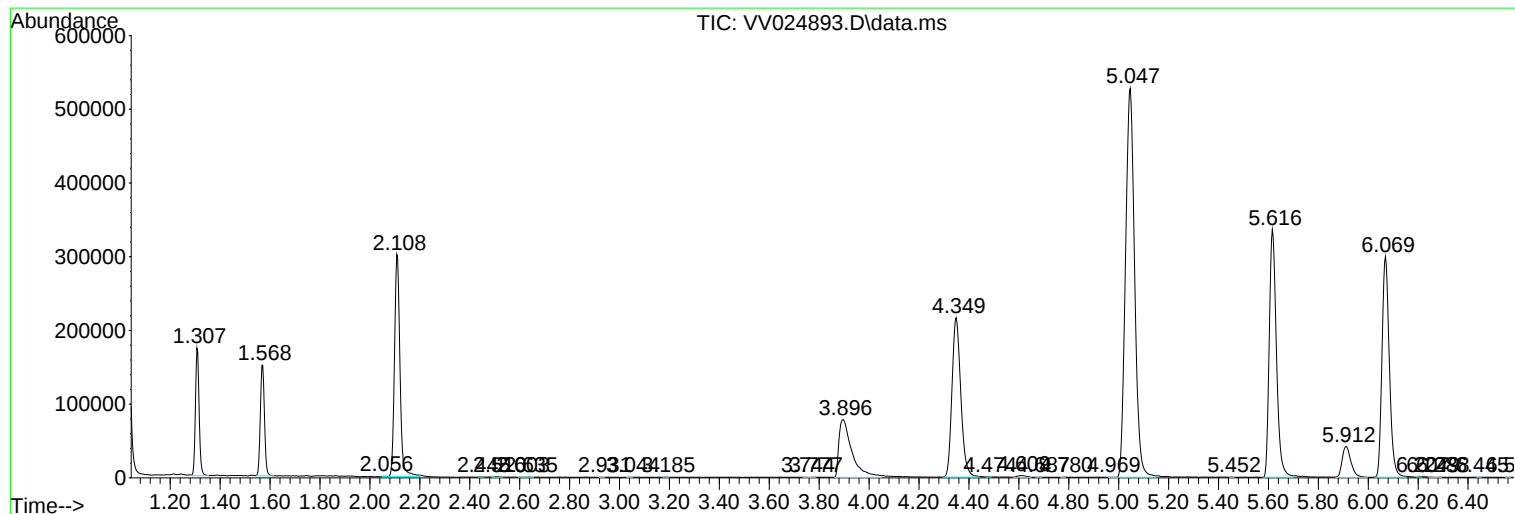

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024893.D
Acq On : 09 Mar 2022 23:44
Operator : SY/MD
Sample : N1856-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024893.D
Acq On : 09 Mar 2022 23:44
Operator : SY/MD
Sample : N1856-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc