

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024896.D
 Acq On : 10 Mar 2022 00:55
 Operator : SY/MD
 Sample : N1855-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	164839	166760	12.98%	1.771%
2	1.571	157	165	178	rVB	151584	169581	13.20%	1.801%
3	2.108	322	332	366	rBV	285747	427069	33.25%	4.536%
4	2.593	477	483	488	rBV3	305	384	0.03%	0.004%
5	2.764	530	536	539	rBV2	357	454	0.04%	0.005%
6	2.873	567	570	571	rBV	153	91	0.01%	0.001%
7	3.072	630	632	635	rBV	164	96	0.01%	0.001%
8	3.092	635	638	640	rVV	142	81	0.01%	0.001%
9	3.134	649	651	654	rBV	157	102	0.01%	0.001%
10	3.272	692	694	697	rVB2	143	73	0.01%	0.001%
11	3.294	697	701	704	rBV2	120	96	0.01%	0.001%
12	3.310	704	706	710	rBV2	95	68	0.01%	0.001%
13	3.709	827	830	833	rBV	188	131	0.01%	0.001%
14	3.754	841	844	846	rVB	153	79	0.01%	0.001%
15	3.809	859	861	862	rBV	93	41	0.00%	0.000%
16	3.822	863	865	868	rVV2	171	121	0.01%	0.001%
17	3.896	878	888	929	rBV	73095	262527	20.44%	2.788%
18	4.349	1013	1029	1059	rBV	207504	514123	40.03%	5.460%
19	4.539	1085	1088	1092	rBV3	302	274	0.02%	0.003%
20	4.584	1100	1102	1105	rBV2	243	156	0.01%	0.002%
21	4.625	1112	1115	1118	rBV2	280	213	0.02%	0.002%
22	4.658	1123	1125	1126	rBV2	186	82	0.01%	0.001%
23	4.686	1131	1134	1135	rBV	154	85	0.01%	0.001%
24	4.777	1160	1162	1165	rBV	166	96	0.01%	0.001%
25	4.789	1165	1166	1169	rVB	169	45	0.00%	0.000%
26	4.809	1169	1172	1174	rBV	230	124	0.01%	0.001%
27	4.825	1174	1177	1179	rBV	131	88	0.01%	0.001%
28	4.854	1184	1186	1188	rBV	80	37	0.00%	0.000%
29	4.870	1189	1191	1199	rBV	361	423	0.03%	0.004%
30	4.924	1204	1208	1211	rBV2	157	146	0.01%	0.002%
31	5.047	1229	1246	1276	rBV2	505644	1284394	100.00%	13.640%
32	5.404	1354	1357	1359	rBV2	240	169	0.01%	0.002%
33	5.442	1366	1369	1371	rBV	217	151	0.01%	0.002%
34	5.494	1380	1385	1388	rBV2	238	219	0.02%	0.002%
35	5.616	1409	1423	1452	rBV	342410	686051	53.41%	7.286%
36	5.915	1502	1516	1539	rBV5	60714	143844	11.20%	1.528%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024896.D
 Acq On : 10 Mar 2022 00:55
 Operator : SY/MD
 Sample : N1855-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.069	1550	1564	1598	rBV	287773	585612	45.59%	6.219%
38	6.211	1605	1608	1610	rBV2	482	359	0.03%	0.004%
39	6.288	1629	1632	1634	rBV2	257	184	0.01%	0.002%
40	6.349	1649	1651	1657	rVB2	235	151	0.01%	0.002%
41	6.375	1657	1659	1660	rBV	119	32	0.00%	0.000%
42	6.397	1664	1666	1668	rBV	122	68	0.01%	0.001%
43	6.474	1687	1690	1692	rBV2	124	73	0.01%	0.001%
44	6.584	1721	1724	1727	rVB	185	107	0.01%	0.001%
45	6.632	1733	1739	1742	rBV4	927	1113	0.09%	0.012%
46	6.796	1787	1790	1793	rBV	105	79	0.01%	0.001%
47	6.815	1793	1796	1799	rBV3	305	227	0.02%	0.002%
48	6.863	1808	1811	1813	rBV	169	92	0.01%	0.001%
49	6.908	1823	1825	1827	rBV	95	37	0.00%	0.000%
50	6.985	1838	1849	1880	rBV	145344	263172	20.49%	2.795%
51	7.114	1886	1889	1895	rVB3	398	354	0.03%	0.004%
52	7.313	1938	1951	1970	rBV	588684	1021731	79.55%	10.851%
53	7.622	2036	2047	2072	rBV	93088	166308	12.95%	1.766%
54	7.911	2133	2137	2138	rBV	195	116	0.01%	0.001%
55	7.940	2140	2146	2148	rBV2	694	714	0.06%	0.008%
56	8.018	2167	2170	2173	rBV	233	148	0.01%	0.002%
57	8.088	2182	2192	2237	rBV	312586	607974	47.34%	6.457%
58	8.612	2353	2355	2358	rVB2	289	110	0.01%	0.001%
59	8.664	2366	2371	2377	rBV	391	443	0.03%	0.005%
60	8.693	2377	2380	2383	rVV2	269	147	0.01%	0.002%
61	8.738	2390	2394	2397	rBV2	167	135	0.01%	0.001%
62	8.850	2417	2429	2455	rBV	523624	855691	66.62%	9.088%
63	9.091	2500	2504	2506	rBV2	293	223	0.02%	0.002%
64	9.153	2520	2523	2526	rVB	480	250	0.02%	0.003%
65	9.233	2544	2548	2549	rBV	190	126	0.01%	0.001%
66	9.397	2596	2599	2602	rBV2	261	191	0.01%	0.002%
67	9.677	2683	2686	2687	rBV	124	70	0.01%	0.001%
68	9.815	2726	2729	2731	rBV2	150	112	0.01%	0.001%
69	10.214	2840	2853	2873	rBV	367358	567028	44.15%	6.022%
70	10.374	2899	2903	2904	rBV	482	342	0.03%	0.004%
71	10.429	2917	2920	2922	rBV	187	124	0.01%	0.001%
72	10.464	2927	2931	2934	rBV	312	337	0.03%	0.004%
73	10.506	2940	2944	2949	rBV	272	186	0.01%	0.002%
74	10.532	2949	2952	2954	rBV	163	123	0.01%	0.001%
75	10.577	2962	2966	2969	rBV2	413	383	0.03%	0.004%
76	10.657	2987	2991	2996	rBV2	296	262	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024896.D
 Acq On : 10 Mar 2022 00:55
 Operator : SY/MD
 Sample : N1855-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M

Title : VOC Analysis

77	10.815	3035	3040	3042	rBV2	180	151	0.01%	0.002%
78	10.911	3066	3070	3072	rBV3	1366	1073	0.08%	0.011%
79	11.140	3137	3141	3148	rVB3	901	909	0.07%	0.010%
80	11.246	3163	3174	3203	rBV	520768	810927	63.14%	8.612%
81	11.622	3278	3291	3310	rBV	561766	868751	67.64%	9.226%
82	11.882	3370	3372	3375	rBV2	292	196	0.02%	0.002%
83	12.043	3420	3422	3426	rBV	277	163	0.01%	0.002%
84	12.673	3612	3618	3620	rBV2	282	349	0.03%	0.004%
85	12.773	3646	3649	3651	rBV2	292	201	0.02%	0.002%

Sum of corrected areas: 9416128




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024896.D
Acq On : 10 Mar 2022 00:55
Operator : SY/MD
Sample : N1855-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

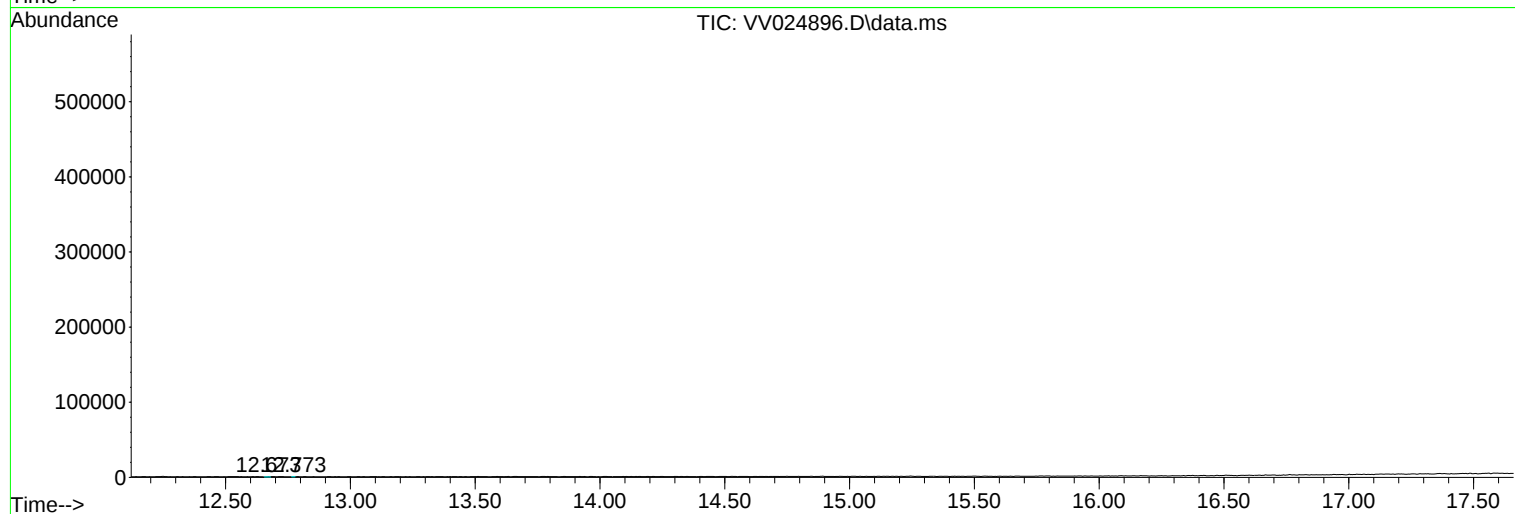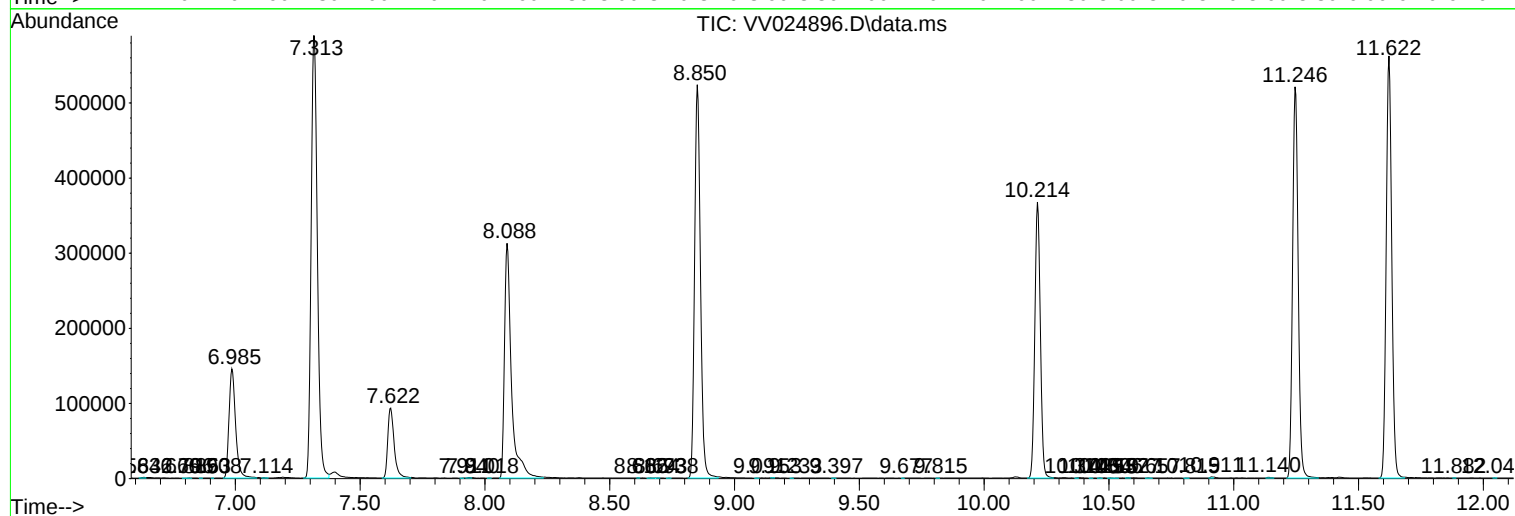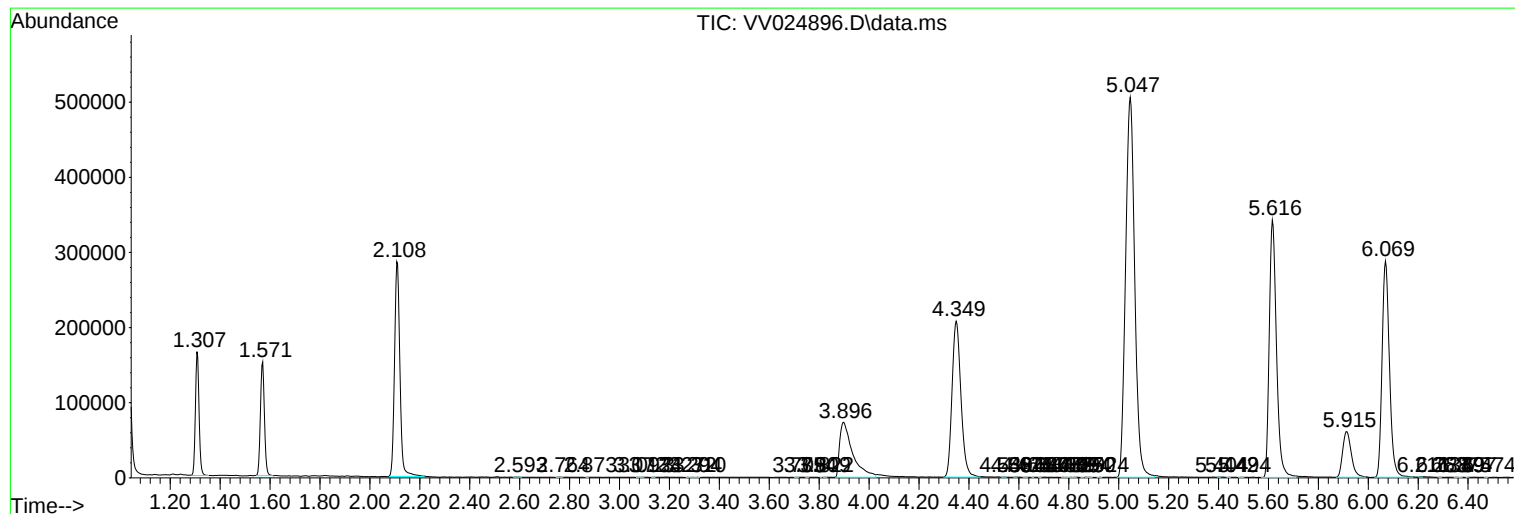

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024896.D
Acq On : 10 Mar 2022 00:55
Operator : SY/MD
Sample : N1855-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
Data File : VV024896.D
Acq On : 10 Mar 2022 00:55
Operator : SY/MD
Sample : N1855-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc