
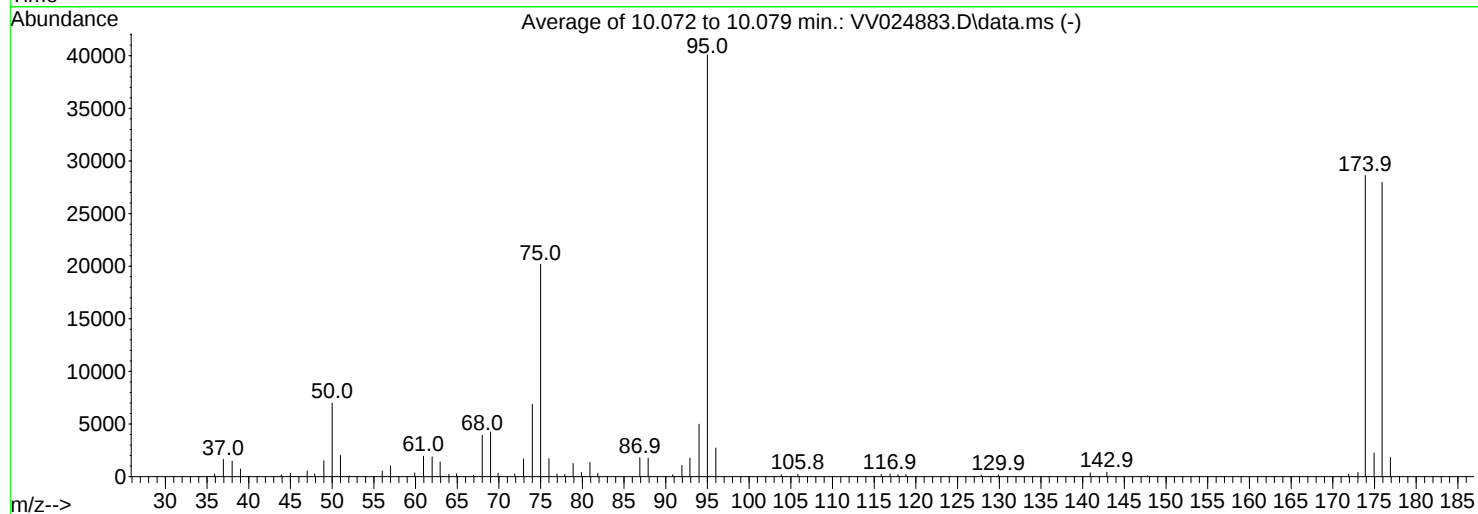


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030922\
 Data File : VV024883.D
 Acq On : 09 Mar 2022 15:32
 Operator : SY/MD
 Sample : BFB202
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB202

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 15 02:18:50 2022

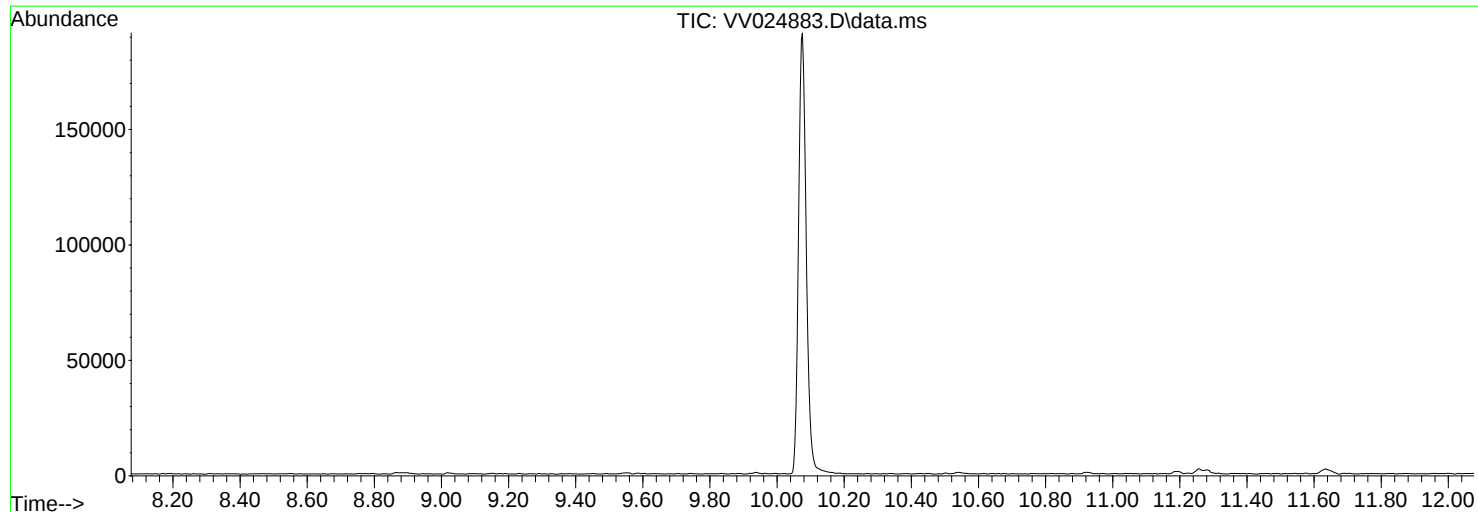

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6992	PASS
75	95	30	80	50.3	20171	PASS
95	95	100	100	100.0	40083	PASS
96	95	5	9	6.8	2720	PASS
173	174	0.00	2	1.4	414	PASS
174	95	50	120	71.4	28613	PASS
175	174	5	9	7.9	2250	PASS
176	174	95	105	97.7	27960	PASS
177	176	5	10	6.5	1825	PASS

m/z	Abundance
39.90	556.0
43.90	349.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.90	235.0
37.00	1557.0
38.00	1518.0
39.00	714.0
39.90	588.0
43.90	498.0
45.00	319.0
47.00	573.0
47.90	334.0
49.00	1654.0
50.00	7268.0
51.00	2220.0
52.10	122.0
56.00	525.0
57.00	987.0
59.90	343.0
61.00	1934.0
62.00	1841.0
63.00	1536.0
64.00	200.0
64.90	232.0
66.90	140.0
68.00	4145.0
69.00	4368.0
69.90	375.0
71.90	275.0
73.00	1673.0
74.00	7065.0
75.00	20720.0
76.00	1920.0
76.90	232.0
77.90	156.0
78.90	1299.0
79.90	404.0
80.90	1435.0
81.80	266.0
86.90	1797.0
87.90	1939.0
90.80	175.0
91.90	1001.0
92.90	1699.0
94.00	5195.0
95.00	41192.0
96.00	2880.0
103.90	192.0
105.90	244.0
115.90	246.0
116.90	296.0
117.90	203.0
118.80	206.0
127.80	154.0
129.90	127.0
140.90	356.0
142.90	449.0
147.80	139.0
171.90	251.0
173.00	410.0
173.90	28424.0
175.00	2293.0
175.90	27904.0
176.90	1817.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.90	267.0
37.00	1741.0
38.00	1539.0
39.00	767.0
39.90	580.0
43.90	525.0
45.00	346.0
47.00	567.0
47.90	274.0
49.00	1560.0
50.00	7169.0
51.00	2047.0
52.00	102.0
56.00	563.0
57.00	1032.0
59.90	371.0
60.90	2004.0
62.00	1956.0
62.90	1448.0
64.00	222.0
64.90	290.0
66.90	128.0
68.00	4053.0
69.00	4375.0
69.90	357.0
71.90	270.0
72.90	1721.0
74.00	7172.0
75.00	20808.0
76.00	1762.0
77.00	248.0
77.90	196.0
78.90	1286.0
79.90	402.0
80.90	1382.0
81.90	331.0
86.90	1867.0
87.90	1814.0
90.90	193.0
92.00	1074.0
92.90	1846.0
94.00	5146.0
95.00	41312.0
96.00	2745.0
103.90	194.0
105.90	264.0
115.90	214.0
116.90	296.0
117.90	189.0
118.80	229.0
127.90	151.0
129.90	183.0
140.90	368.0
142.90	434.0
147.70	130.0
171.90	235.0
173.00	430.0
173.90	29512.0
174.90	2310.0
175.90	28832.0
176.90	1951.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.90	274.0
36.90	1626.0
38.00	1354.0
39.00	695.0
39.90	557.0
43.90	544.0
45.00	331.0
47.00	483.0
47.90	186.0
49.00	1322.0
50.00	6538.0
51.00	1791.0
56.00	525.0
57.00	996.0
59.90	373.0
61.00	1876.0
62.00	1876.0
62.90	1210.0
64.00	225.0
64.90	283.0
67.00	121.0
68.00	3607.0
69.00	3998.0
69.90	289.0
71.90	241.0
72.90	1680.0
74.00	6436.0
75.00	18984.0
76.00	1489.0
77.00	248.0
77.90	223.0
78.90	1155.0
79.90	403.0
80.90	1254.0
81.90	344.0
86.90	1779.0
87.90	1521.0
90.90	184.0
91.90	1139.0
92.90	1766.0
94.00	4607.0
95.00	37744.0
96.00	2535.0
103.80	189.0
105.80	243.0
115.80	177.0
116.90	250.0
117.80	138.0
118.80	237.0
127.90	138.0
129.90	194.0
140.90	375.0
142.90	387.0
171.90	199.0
173.00	402.0
173.90	27904.0
174.90	2146.0
175.90	27144.0
176.90	1708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202