

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014807.D
 Acq On : 10 Mar 2020 17:26
 Operator : SY/MD
 Sample : VV0310WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	190566	203518	14.12%	1.817%
2	1.579	145	152	166	rVB	136972	169146	11.74%	1.510%
3	2.119	310	320	344	rVB	292706	429213	29.78%	3.832%
4	2.460	423	426	427	rBV2	994	525	0.04%	0.005%
5	2.756	513	518	520	rBV3	859	757	0.05%	0.007%
6	3.013	595	598	600	rBV2	528	294	0.02%	0.003%
7	3.045	606	608	614	rVB3	536	376	0.03%	0.003%
8	3.116	626	630	633	rVB3	863	570	0.04%	0.005%
9	3.135	633	636	638	rBV	660	317	0.02%	0.003%
10	3.245	666	670	672	rBV3	647	556	0.04%	0.005%
11	3.296	683	686	689	rBV3	490	333	0.02%	0.003%
12	3.322	689	694	695	rBV2	495	368	0.03%	0.003%
13	3.460	732	737	740	rBV2	825	538	0.04%	0.005%
14	3.798	837	842	845	rBV2	787	573	0.04%	0.005%
15	3.933	871	884	904	rBV	60181	217527	15.09%	1.942%
16	4.376	1007	1022	1044	rBV	226656	552340	38.33%	4.931%
17	4.614	1092	1096	1099	rVB2	680	433	0.03%	0.004%
18	4.672	1112	1114	1117	rVB2	667	304	0.02%	0.003%
19	4.698	1117	1122	1123	rBV2	847	665	0.05%	0.006%
20	4.733	1131	1133	1135	rBV2	512	295	0.02%	0.003%
21	4.785	1144	1149	1151	rBV3	513	430	0.03%	0.004%
22	4.843	1165	1167	1171	rBV2	530	377	0.03%	0.003%
23	4.894	1180	1183	1186	rBV2	534	273	0.02%	0.002%
24	4.926	1189	1193	1195	rBV3	550	405	0.03%	0.004%
25	4.990	1211	1213	1218	rVB2	423	277	0.02%	0.002%
26	5.074	1220	1239	1265	rBV2	573571	1441181	100.00%	12.866%
27	5.588	1395	1399	1402	rVB	498	359	0.02%	0.003%
28	5.640	1402	1415	1441	rBV	462914	927578	64.36%	8.281%
29	5.923	1497	1503	1505	rBV6	2010	2083	0.14%	0.019%
30	6.096	1541	1557	1585	rBV	315116	651683	45.22%	5.818%
31	6.264	1607	1609	1612	rBV3	591	341	0.02%	0.003%
32	6.302	1619	1621	1624	rBV	428	296	0.02%	0.003%
33	6.322	1624	1627	1629	rVB2	509	263	0.02%	0.002%
34	6.495	1678	1681	1684	rVV2	591	374	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014807.D
 Acq On : 10 Mar 2020 17:26
 Operator : SY/MD
 Sample : VV0310WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.547	1693	1697	1698	rBV	450	349	0.02%	0.003%
36	6.585	1703	1709	1712	rBB3	566	511	0.04%	0.005%
37	6.666	1729	1734	1736	rVB3	835	612	0.04%	0.005%
38	6.685	1736	1740	1744	rVB2	630	394	0.03%	0.004%
39	6.720	1747	1751	1753	rBV	435	315	0.02%	0.003%
40	6.826	1780	1784	1787	rBV2	396	341	0.02%	0.003%
41	6.846	1787	1790	1791	rVV2	602	332	0.02%	0.003%
42	7.010	1828	1841	1858	rBV	179839	322283	22.36%	2.877%
43	7.193	1896	1898	1902	rBV	625	443	0.03%	0.004%
44	7.212	1902	1904	1907	rBV2	520	282	0.02%	0.003%
45	7.235	1907	1911	1916	rBV6	628	651	0.05%	0.006%
46	7.338	1930	1943	1968	rBV	716732	1230821	85.40%	10.988%
47	7.569	2013	2015	2017	rVB3	894	405	0.03%	0.004%
48	7.643	2024	2038	2059	rBV	123384	215476	14.95%	1.924%
49	7.852	2101	2103	2107	rBV3	603	525	0.04%	0.005%
50	7.913	2120	2122	2124	rVB	858	295	0.02%	0.003%
51	7.939	2124	2130	2131	rBV3	863	756	0.05%	0.007%
52	8.045	2156	2163	2165	rBV3	672	662	0.05%	0.006%
53	8.119	2172	2186	2220	rBV	357039	754626	52.36%	6.737%
54	8.376	2264	2266	2271	rVB3	851	481	0.03%	0.004%
55	8.399	2271	2273	2276	rBV3	520	288	0.02%	0.003%
56	8.511	2306	2308	2311	rVB3	974	505	0.04%	0.005%
57	8.534	2311	2315	2316	rBV	770	497	0.03%	0.004%
58	8.569	2323	2326	2331	rVB4	575	382	0.03%	0.003%
59	8.875	2407	2421	2442	rBV	701973	1136540	78.86%	10.147%
60	9.116	2492	2496	2498	rBV	578	469	0.03%	0.004%
61	9.151	2504	2507	2511	rBV3	785	579	0.04%	0.005%
62	9.219	2525	2528	2531	rVB2	742	450	0.03%	0.004%
63	9.293	2549	2551	2556	rBV2	427	411	0.03%	0.004%
64	9.431	2591	2594	2600	rBV2	670	645	0.04%	0.006%
65	9.473	2600	2607	2611	rVV4	492	596	0.04%	0.005%
66	9.530	2621	2625	2628	rBV3	556	469	0.03%	0.004%
67	9.566	2630	2636	2637	rBV4	1047	891	0.06%	0.008%
68	9.620	2651	2653	2655	rVB	703	269	0.02%	0.002%
69	9.637	2655	2658	2661	rVB2	642	301	0.02%	0.003%
70	9.849	2721	2724	2726	rBV	542	323	0.02%	0.003%
71	9.878	2729	2733	2736	rVV3	586	433	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014807.D
 Acq On : 10 Mar 2020 17:26
 Operator : SY/MD
 Sample : VV0310WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.022	2772	2778	2780	rVV2	557	408	0.03%	0.004%
73	10.238	2832	2845	2862	rBV	454208	707486	49.09%	6.316%
74	10.309	2865	2867	2871	rVB	725	366	0.03%	0.003%
75	10.370	2883	2886	2888	rBV3	552	298	0.02%	0.003%
76	10.556	2942	2944	2949	rVV2	905	764	0.05%	0.007%
77	10.608	2956	2960	2963	rBV3	475	349	0.02%	0.003%
78	10.727	2993	2997	3002	rBV2	729	672	0.05%	0.006%
79	10.752	3002	3005	3008	rVB2	454	260	0.02%	0.002%
80	11.103	3112	3114	3116	rBV2	592	266	0.02%	0.002%
81	11.177	3135	3137	3140	rBV2	681	493	0.03%	0.004%
82	11.270	3154	3166	3184	rBV	707030	1094166	75.92%	9.768%
83	11.450	3219	3222	3224	rVB	843	400	0.03%	0.004%
84	11.530	3243	3247	3252	rBV4	862	858	0.06%	0.008%
85	11.556	3252	3255	3257	rBV2	663	501	0.03%	0.004%
86	11.646	3269	3283	3302	rBV	691330	1107109	76.82%	9.884%
87	11.852	3345	3347	3349	rBV	615	386	0.03%	0.003%
88	12.071	3409	3415	3416	rBV	391	418	0.03%	0.004%
89	12.386	3511	3513	3516	rBV	551	304	0.02%	0.003%
90	12.476	3538	3541	3544	rBV2	419	348	0.02%	0.003%
91	12.556	3564	3566	3572	rVB3	419	356	0.02%	0.003%
92	12.595	3574	3578	3580	rBV3	420	300	0.02%	0.003%
93	12.620	3583	3586	3589	rVB3	641	384	0.03%	0.003%
94	12.665	3593	3600	3601	rBV3	1526	1379	0.10%	0.012%
95	12.746	3622	3625	3631	rBV4	422	429	0.03%	0.004%
96	12.842	3653	3655	3660	rBV2	526	299	0.02%	0.003%
97	12.913	3674	3677	3681	rBV3	796	604	0.04%	0.005%
98	13.279	3786	3791	3792	rBV3	1897	1687	0.12%	0.015%
99	13.726	3929	3930	3933	rVB2	696	314	0.02%	0.003%
100	14.128	4053	4055	4056	rBV	665	268	0.02%	0.002%


Sum of corrected areas: 11201048

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014807.D
Acq On : 10 Mar 2020 17:26
Operator : SY/MD
Sample : VV0310WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

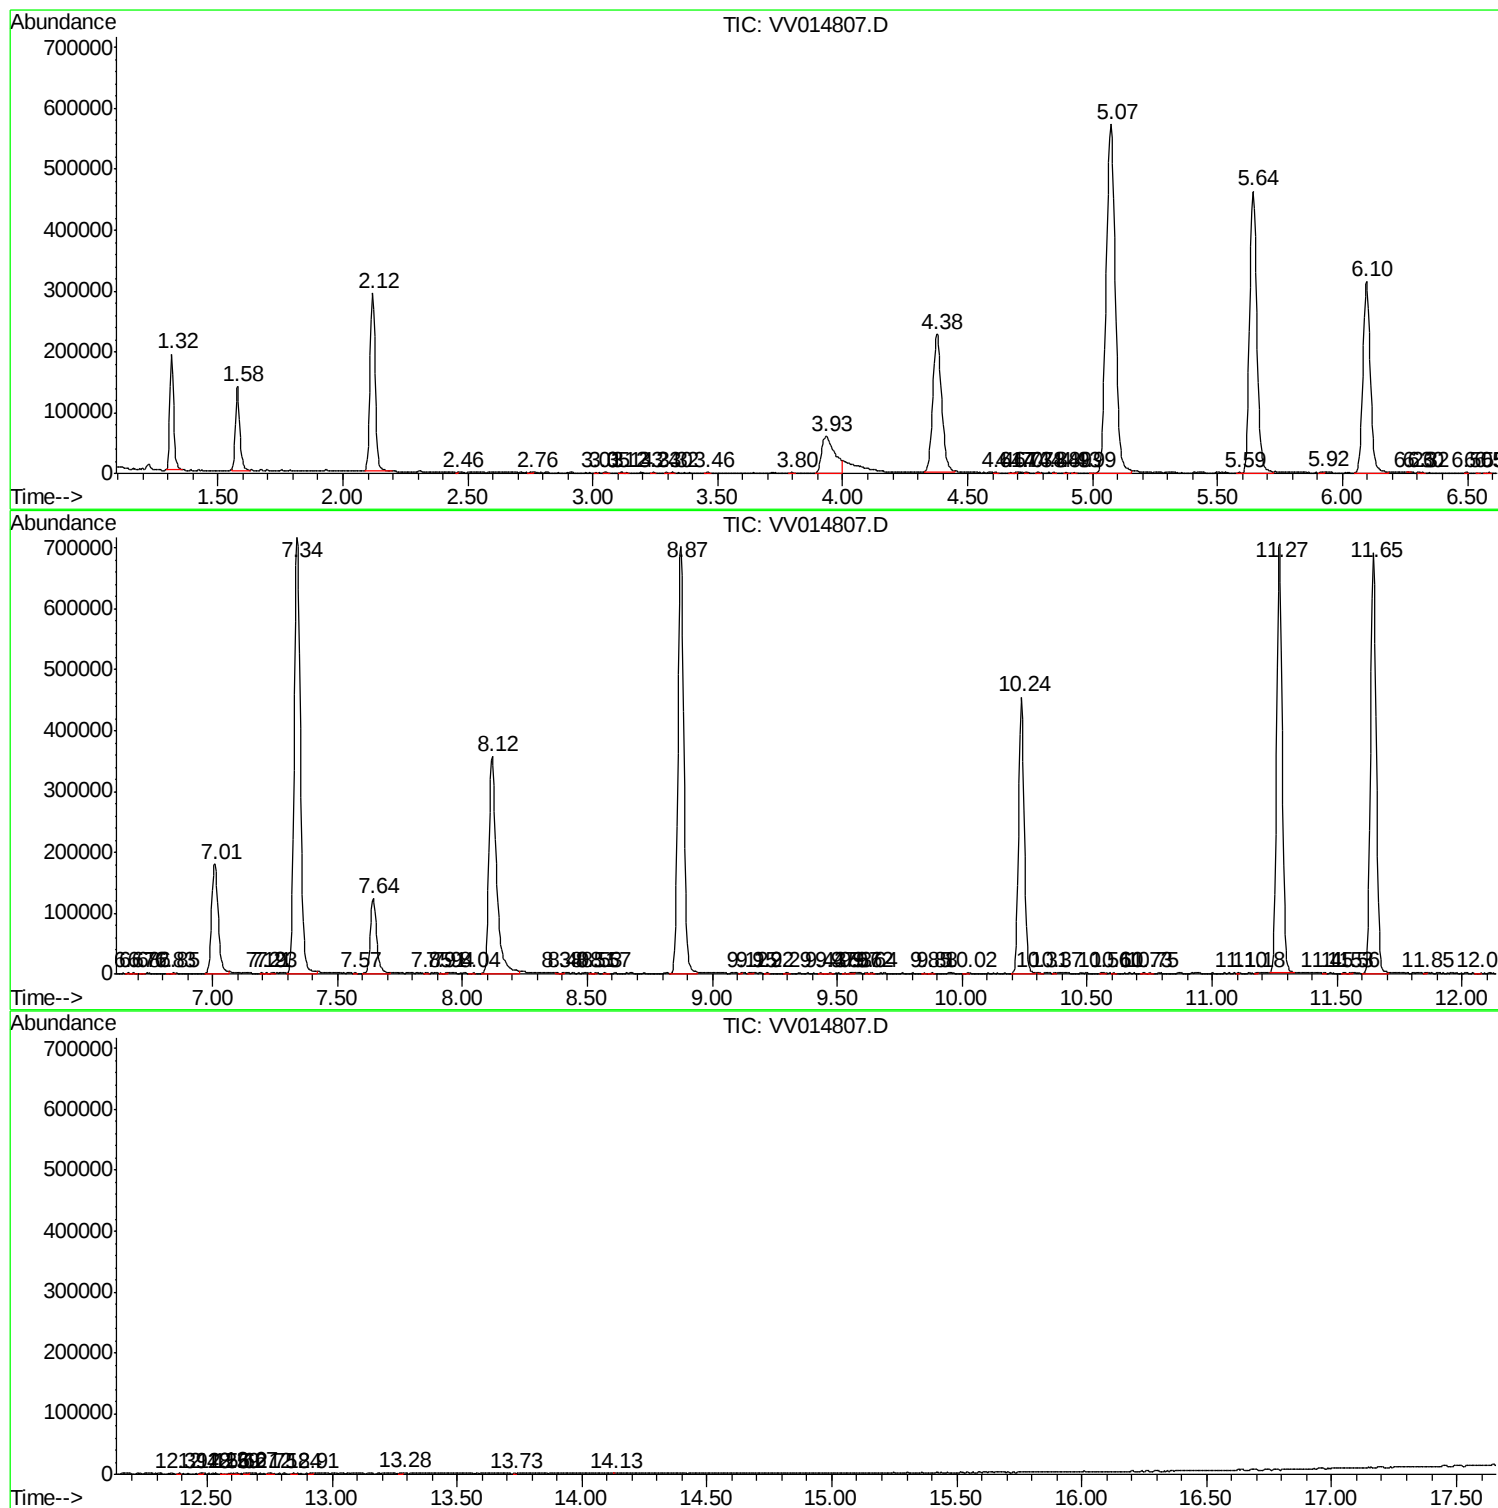

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014807.D
Acq On : 10 Mar 2020 17:26
Operator : SY/MD
Sample : VV0310WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014807.D
Acq On : 10 Mar 2020 17:26
Operator : SY/MD
Sample : VV0310WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc