

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014810.D
 Acq On : 10 Mar 2020 18:38
 Operator : SY/MD
 Sample : L1858-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	87	rVB	155514	166981	12.08%	1.507%
2	1.579	145	152	167	rVB	119148	147403	10.67%	1.330%
3	2.119	311	320	342	rVB	257204	368392	26.65%	3.324%
4	2.872	548	554	557	rBV3	805	773	0.06%	0.007%
5	2.891	557	560	561	rBV2	587	275	0.02%	0.002%
6	2.939	573	575	577	rBV2	718	345	0.02%	0.003%
7	2.971	582	585	587	rBV	487	326	0.02%	0.003%
8	3.184	647	651	655	rBV4	819	701	0.05%	0.006%
9	3.251	670	672	674	rBV4	503	264	0.02%	0.002%
10	3.296	684	686	688	rBV2	440	228	0.02%	0.002%
11	3.328	692	696	698	rVB2	460	256	0.02%	0.002%
12	3.341	698	700	703	rBV2	551	264	0.02%	0.002%
13	3.418	722	724	727	rVB3	393	212	0.02%	0.002%
14	3.486	741	745	749	rBV4	504	547	0.04%	0.005%
15	3.727	817	820	823	rBV4	507	351	0.03%	0.003%
16	3.807	843	845	849	rBV2	442	268	0.02%	0.002%
17	3.852	855	859	860	rBV2	512	351	0.03%	0.003%
18	3.888	866	870	871	rBV2	496	345	0.02%	0.003%
19	3.936	872	885	932	rBV2	73477	333306	24.12%	3.008%
20	4.380	1007	1023	1050	rVB2	219237	548151	39.66%	4.946%
21	4.634	1100	1102	1104	rVB3	692	256	0.02%	0.002%
22	4.862	1169	1173	1175	rVB3	444	247	0.02%	0.002%
23	4.881	1175	1179	1181	rBV3	635	392	0.03%	0.004%
24	4.949	1197	1200	1201	rBV2	529	227	0.02%	0.002%
25	5.074	1220	1239	1264	rBV2	554111	1382102	100.00%	12.472%
26	5.270	1296	1300	1303	rBV4	619	480	0.03%	0.004%
27	5.492	1364	1369	1372	rBV3	676	640	0.05%	0.006%
28	5.556	1387	1389	1395	rVB4	769	603	0.04%	0.005%
29	5.643	1401	1416	1436	rBV	477378	944967	68.37%	8.527%
30	6.097	1540	1557	1580	rBV	309139	630657	45.63%	5.691%
31	6.415	1654	1656	1658	rBV2	442	247	0.02%	0.002%
32	6.457	1667	1669	1672	rVB2	716	303	0.02%	0.003%
33	6.476	1672	1675	1679	rVB2	479	330	0.02%	0.003%
34	6.534	1691	1693	1695	rBV2	518	212	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014810.D
 Acq On : 10 Mar 2020 18:38
 Operator : SY/MD
 Sample : L1858-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.544	1695	1696	1700	rVB2	496	315	0.02%	0.003%
36	6.589	1708	1710	1716	rVB4	657	594	0.04%	0.005%
37	6.695	1738	1743	1744	rBV2	511	404	0.03%	0.004%
38	6.749	1759	1760	1765	rBV3	468	376	0.03%	0.003%
39	6.846	1787	1790	1792	rBV2	350	215	0.02%	0.002%
40	6.952	1821	1823	1826	rBV	510	334	0.02%	0.003%
41	7.010	1829	1841	1859	rVV	168261	301731	21.83%	2.723%
42	7.164	1886	1889	1890	rBV	657	377	0.03%	0.003%
43	7.235	1908	1911	1915	rVB4	520	461	0.03%	0.004%
44	7.257	1915	1918	1919	rBV2	527	256	0.02%	0.002%
45	7.338	1931	1943	1961	rBV	676015	1156573	83.68%	10.436%
46	7.643	2027	2038	2058	rBV	120345	203751	14.74%	1.839%
47	7.843	2097	2100	2101	rBV3	597	313	0.02%	0.003%
48	7.891	2111	2115	2117	rBV2	588	335	0.02%	0.003%
49	7.965	2132	2138	2147	rVB6	2981	4264	0.31%	0.038%
50	8.071	2169	2171	2174	rBV	736	446	0.03%	0.004%
51	8.116	2174	2185	2221	rVV	365648	746176	53.99%	6.733%
52	8.357	2258	2260	2262	rVB2	707	299	0.02%	0.003%
53	8.454	2287	2290	2294	rVB3	932	504	0.04%	0.005%
54	8.524	2308	2312	2313	rBV	571	337	0.02%	0.003%
55	8.566	2322	2325	2329	rBV	472	328	0.02%	0.003%
56	8.653	2350	2352	2355	rVB2	566	211	0.02%	0.002%
57	8.775	2388	2390	2393	rBV2	592	248	0.02%	0.002%
58	8.810	2396	2401	2404	rVB5	1093	852	0.06%	0.008%
59	8.875	2408	2421	2444	rBV	724577	1165755	84.35%	10.519%
60	9.035	2465	2471	2479	rVB6	3256	4786	0.35%	0.043%
61	9.077	2479	2484	2485	rBV5	1344	1113	0.08%	0.010%
62	9.161	2502	2510	2522	rVB3	10295	17192	1.24%	0.155%
63	9.261	2539	2541	2546	rBV3	423	262	0.02%	0.002%
64	9.322	2556	2560	2561	rBV	422	274	0.02%	0.002%
65	9.405	2584	2586	2588	rBV	511	272	0.02%	0.002%
66	9.492	2599	2613	2616	rBV6	2285	3685	0.27%	0.033%
67	9.569	2630	2637	2645	rVB4	4764	7309	0.53%	0.066%
68	9.621	2649	2653	2657	rBV3	722	664	0.05%	0.006%
69	9.662	2662	2666	2669	rBV2	439	285	0.02%	0.003%
70	9.775	2699	2701	2704	rBV3	483	361	0.03%	0.003%
71	9.820	2709	2715	2716	rBV4	1490	1407	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014810.D
 Acq On : 10 Mar 2020 18:38
 Operator : SY/MD
 Sample : L1858-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.016	2773	2776	2778	rBV2	630	361	0.03%	0.003%
73	10.042	2781	2784	2786	rVV3	549	345	0.02%	0.003%
74	10.238	2832	2845	2860	rBV	452478	710564	51.41%	6.412%
75	10.341	2874	2877	2882	rBV3	701	586	0.04%	0.005%
76	10.363	2882	2884	2887	rBV2	527	300	0.02%	0.003%
77	10.515	2929	2931	2932	rBV2	466	226	0.02%	0.002%
78	10.633	2965	2968	2970	rBV2	466	218	0.02%	0.002%
79	10.823	3025	3027	3033	rVB2	564	397	0.03%	0.004%
80	10.852	3033	3036	3039	rVV4	593	448	0.03%	0.004%
81	10.875	3040	3043	3044	rVV2	874	527	0.04%	0.005%
82	11.270	3153	3166	3184	rBV	724499	1124437	81.36%	10.146%
83	11.434	3214	3217	3220	rBV3	933	639	0.05%	0.006%
84	11.514	3240	3242	3245	rVB3	700	335	0.02%	0.003%
85	11.553	3245	3254	3255	rBV7	1802	1966	0.14%	0.018%
86	11.646	3270	3283	3296	rBV	692656	1077053	77.93%	9.719%
87	12.013	3394	3397	3404	rBV4	709	895	0.06%	0.008%
88	12.080	3416	3418	3420	rBV2	422	228	0.02%	0.002%
89	12.277	3474	3479	3480	rBV3	679	560	0.04%	0.005%
90	12.325	3493	3494	3499	rVB	447	245	0.02%	0.002%
91	12.363	3503	3506	3508	rBV2	956	551	0.04%	0.005%
92	12.428	3524	3526	3528	rBV	496	229	0.02%	0.002%
93	12.492	3538	3546	3552	rBV2	875	1350	0.10%	0.012%
94	12.688	3605	3607	3609	rBV	577	298	0.02%	0.003%
95	12.878	3662	3666	3668	rBV3	457	358	0.03%	0.003%
96	13.170	3755	3757	3759	rBV2	591	236	0.02%	0.002%
97	13.206	3766	3768	3770	rBV2	563	272	0.02%	0.002%
98	13.286	3786	3793	3802	rVB9	1572	2400	0.17%	0.022%
99	13.907	3984	3986	3995	rVB4	835	785	0.06%	0.007%
100	14.328	4114	4117	4122	rVB5	1108	748	0.05%	0.007%


Sum of corrected areas: 11082024

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014810.D
Acq On : 10 Mar 2020 18:38
Operator : SY/MD
Sample : L1858-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

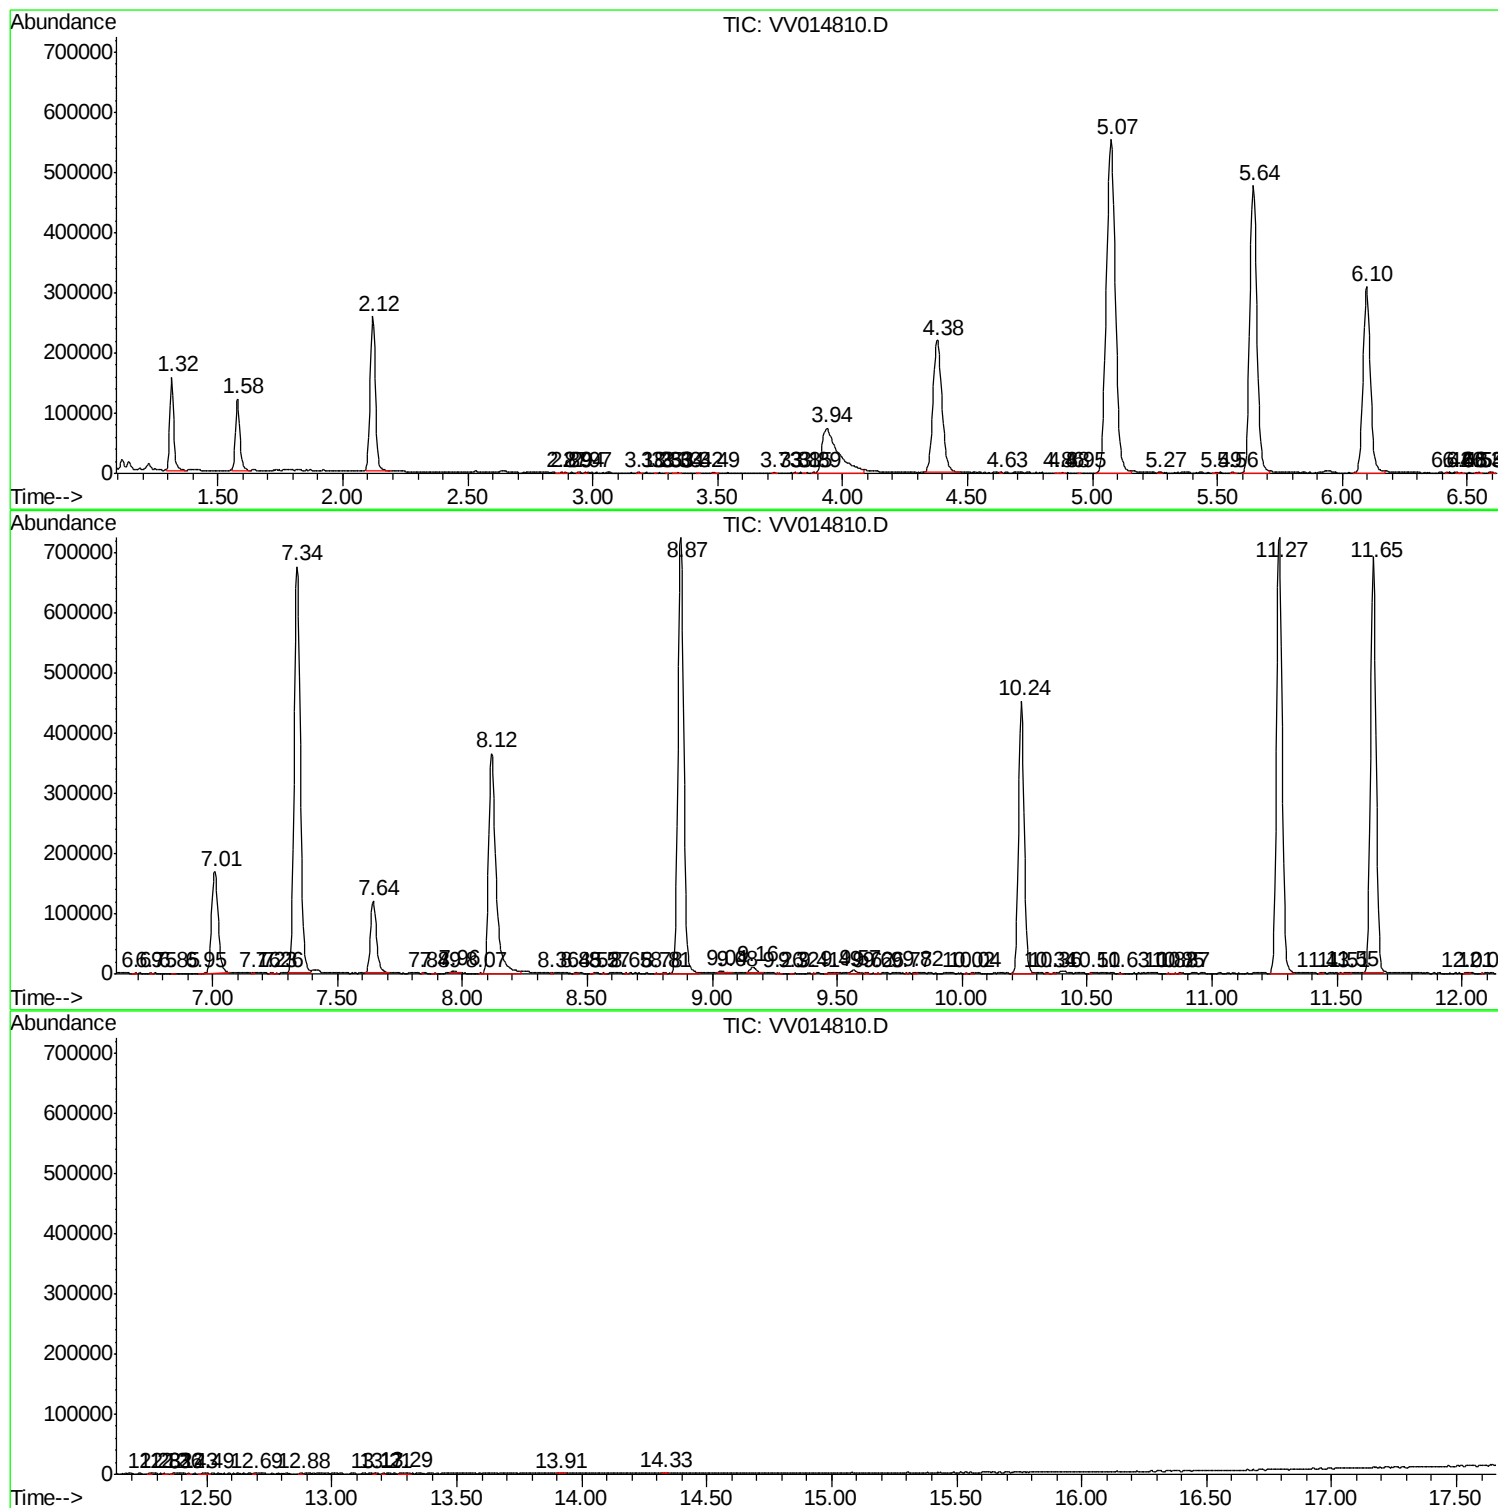

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014810.D
Acq On : 10 Mar 2020 18:38
Operator : SY/MD
Sample : L1858-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014810.D
Acq On : 10 Mar 2020 18:38
Operator : SY/MD
Sample : L1858-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc