

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014811.D
 Acq On : 10 Mar 2020 19:02
 Operator : SY/MD
 Sample : L1858-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	147192	157825	12.01%	1.462%
2	1.579	145	152	166	rVB	119449	144820	11.02%	1.341%
3	2.119	311	320	334	rVB	244373	343614	26.14%	3.183%
4	2.762	517	520	522	rBV3	1000	621	0.05%	0.006%
5	2.958	577	581	582	rBV	485	304	0.02%	0.003%
6	3.068	613	615	617	rBV3	773	363	0.03%	0.003%
7	3.122	629	632	636	rBV4	645	480	0.04%	0.004%
8	3.158	640	643	646	rVB3	618	421	0.03%	0.004%
9	3.273	672	679	681	rVB4	588	629	0.05%	0.006%
10	3.569	768	771	774	rVB2	985	620	0.05%	0.006%
11	3.595	774	779	781	rBV2	599	360	0.03%	0.003%
12	3.618	784	786	791	rBV2	597	418	0.03%	0.004%
13	3.698	808	811	814	rBV2	399	334	0.03%	0.003%
14	3.765	829	832	834	rVB3	536	307	0.02%	0.003%
15	3.778	834	836	837	rBV2	643	315	0.02%	0.003%
16	3.865	861	863	866	rVB	596	334	0.03%	0.003%
17	3.881	866	868	870	rBV	414	271	0.02%	0.003%
18	3.936	871	885	929	rBV2	74861	305143	23.21%	2.826%
19	4.376	1008	1022	1049	rVB2	211075	528042	40.17%	4.891%
20	4.617	1095	1097	1101	rBV2	532	359	0.03%	0.003%
21	4.740	1132	1135	1139	rVB2	543	345	0.03%	0.003%
22	4.791	1148	1151	1155	rVB2	512	313	0.02%	0.003%
23	4.817	1155	1159	1161	rBV3	399	278	0.02%	0.003%
24	4.846	1164	1168	1169	rBV3	800	570	0.04%	0.005%
25	4.929	1191	1194	1197	rBV2	684	367	0.03%	0.003%
26	5.010	1214	1219	1220	rBV2	620	565	0.04%	0.005%
27	5.074	1221	1239	1263	rBV2	531258	1314550	100.00%	12.176%
28	5.453	1355	1357	1361	rBV3	364	232	0.02%	0.002%
29	5.643	1403	1416	1437	rBV	458725	902733	68.67%	8.362%
30	5.801	1463	1465	1467	rBV2	1099	552	0.04%	0.005%
31	5.836	1474	1476	1479	rBV	551	234	0.02%	0.002%
32	5.939	1495	1508	1530	rBV	83980	166475	12.66%	1.542%
33	6.096	1540	1557	1583	rBV	294720	603063	45.88%	5.586%
34	6.289	1614	1617	1619	rBV2	865	489	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014811.D
 Acq On : 10 Mar 2020 19:02
 Operator : SY/MD
 Sample : L1858-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.514	1685	1687	1690	rBV3	492	272	0.02%	0.003%
36	6.531	1690	1692	1694	rBV2	581	355	0.03%	0.003%
37	6.605	1713	1715	1718	rVB2	722	355	0.03%	0.003%
38	6.627	1718	1722	1724	rBV	1077	826	0.06%	0.008%
39	6.752	1760	1761	1765	rVB	664	350	0.03%	0.003%
40	6.781	1768	1770	1774	rVB2	614	356	0.03%	0.003%
41	6.810	1774	1779	1780	rBV2	472	375	0.03%	0.003%
42	6.846	1786	1790	1793	rBV3	571	366	0.03%	0.003%
43	6.862	1793	1795	1798	rVV2	501	302	0.02%	0.003%
44	6.958	1823	1825	1827	rBV	424	259	0.02%	0.002%
45	7.010	1828	1841	1862	rVV	158787	290563	22.10%	2.691%
46	7.209	1901	1903	1906	rBV2	485	280	0.02%	0.003%
47	7.338	1930	1943	1962	rBV	647935	1110640	84.49%	10.287%
48	7.502	1992	1994	1998	rBV	932	634	0.05%	0.006%
49	7.643	2027	2038	2054	rBV	114339	192567	14.65%	1.784%
50	7.858	2103	2105	2107	rBV2	706	335	0.03%	0.003%
51	7.929	2125	2127	2129	rBV2	501	252	0.02%	0.002%
52	7.961	2129	2137	2144	rVV	2919	5056	0.38%	0.047%
53	8.035	2157	2160	2162	rBV2	699	421	0.03%	0.004%
54	8.116	2174	2185	2221	rBV	352857	720389	54.80%	6.673%
55	8.395	2269	2272	2279	rVB5	1067	1096	0.08%	0.010%
56	8.424	2279	2281	2284	rBV2	614	300	0.02%	0.003%
57	8.559	2320	2323	2330	rBV3	532	731	0.06%	0.007%
58	8.675	2356	2359	2364	rBV3	867	759	0.06%	0.007%
59	8.875	2408	2421	2439	rBV	695407	1125268	85.60%	10.423%
60	9.093	2488	2489	2494	rBV2	562	283	0.02%	0.003%
61	9.161	2502	2510	2520	rVB3	8100	12408	0.94%	0.115%
62	9.280	2544	2547	2549	rVB2	577	268	0.02%	0.002%
63	9.299	2549	2553	2556	rVB3	852	559	0.04%	0.005%
64	9.321	2556	2560	2561	rBV2	462	260	0.02%	0.002%
65	9.399	2581	2584	2585	rBV2	519	246	0.02%	0.002%
66	9.453	2598	2601	2605	rVB2	559	374	0.03%	0.003%
67	9.566	2627	2636	2648	rBV5	3787	6629	0.50%	0.061%
68	9.813	2711	2713	2715	rBV3	889	428	0.03%	0.004%
69	9.919	2744	2746	2751	rVB2	434	235	0.02%	0.002%
70	9.948	2751	2755	2761	rBV3	1117	985	0.07%	0.009%
71	10.064	2789	2791	2794	rVB3	551	302	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014811.D
 Acq On : 10 Mar 2020 19:02
 Operator : SY/MD
 Sample : L1858-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.116	2804	2807	2810	rBV	506	267	0.02%	0.002%
73	10.161	2819	2821	2825	rBV	440	248	0.02%	0.002%
74	10.238	2833	2845	2865	rBV	441272	687805	52.32%	6.371%
75	10.354	2878	2881	2884	rBV3	583	454	0.03%	0.004%
76	10.379	2884	2889	2890	rVV3	807	748	0.06%	0.007%
77	10.405	2891	2897	2905	rVB	4618	6797	0.52%	0.063%
78	10.534	2930	2937	2940	rBV5	1120	1524	0.12%	0.014%
79	10.672	2975	2980	2985	rBV4	890	803	0.06%	0.007%
80	10.855	3034	3037	3039	rBV3	366	248	0.02%	0.002%
81	11.080	3104	3107	3110	rBV3	482	309	0.02%	0.003%
82	11.177	3130	3137	3150	rBV8	2488	5072	0.39%	0.047%
83	11.270	3153	3166	3186	rBV	695944	1085434	82.57%	10.054%
84	11.482	3228	3232	3233	rBV	868	490	0.04%	0.005%
85	11.559	3249	3256	3270	rBV9	3422	7230	0.55%	0.067%
86	11.646	3270	3283	3304	rVV	650950	1037001	78.89%	9.605%
87	11.755	3315	3317	3321	rVB3	973	531	0.04%	0.005%
88	11.997	3387	3392	3393	rBV2	552	437	0.03%	0.004%
89	12.370	3501	3508	3513	rBV6	2571	3650	0.28%	0.034%
90	12.566	3566	3569	3570	rBV2	431	258	0.02%	0.002%
91	12.665	3597	3600	3601	rBV	929	593	0.05%	0.005%
92	12.781	3631	3636	3638	rBV2	650	509	0.04%	0.005%
93	12.845	3654	3656	3659	rBV2	424	311	0.02%	0.003%
94	12.903	3671	3674	3677	rBV2	714	434	0.03%	0.004%
95	13.061	3721	3723	3724	rBV	441	248	0.02%	0.002%
96	13.331	3805	3807	3809	rBV3	627	269	0.02%	0.002%
97	13.350	3809	3813	3815	rBV3	628	353	0.03%	0.003%
98	13.636	3900	3902	3906	rBV3	547	395	0.03%	0.004%
99	13.720	3925	3928	3933	rBV3	686	645	0.05%	0.006%
100	14.540	4179	4183	4186	rBV3	1016	797	0.06%	0.007%


Sum of corrected areas: 10796290

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014811.D
Acq On : 10 Mar 2020 19:02
Operator : SY/MD
Sample : L1858-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

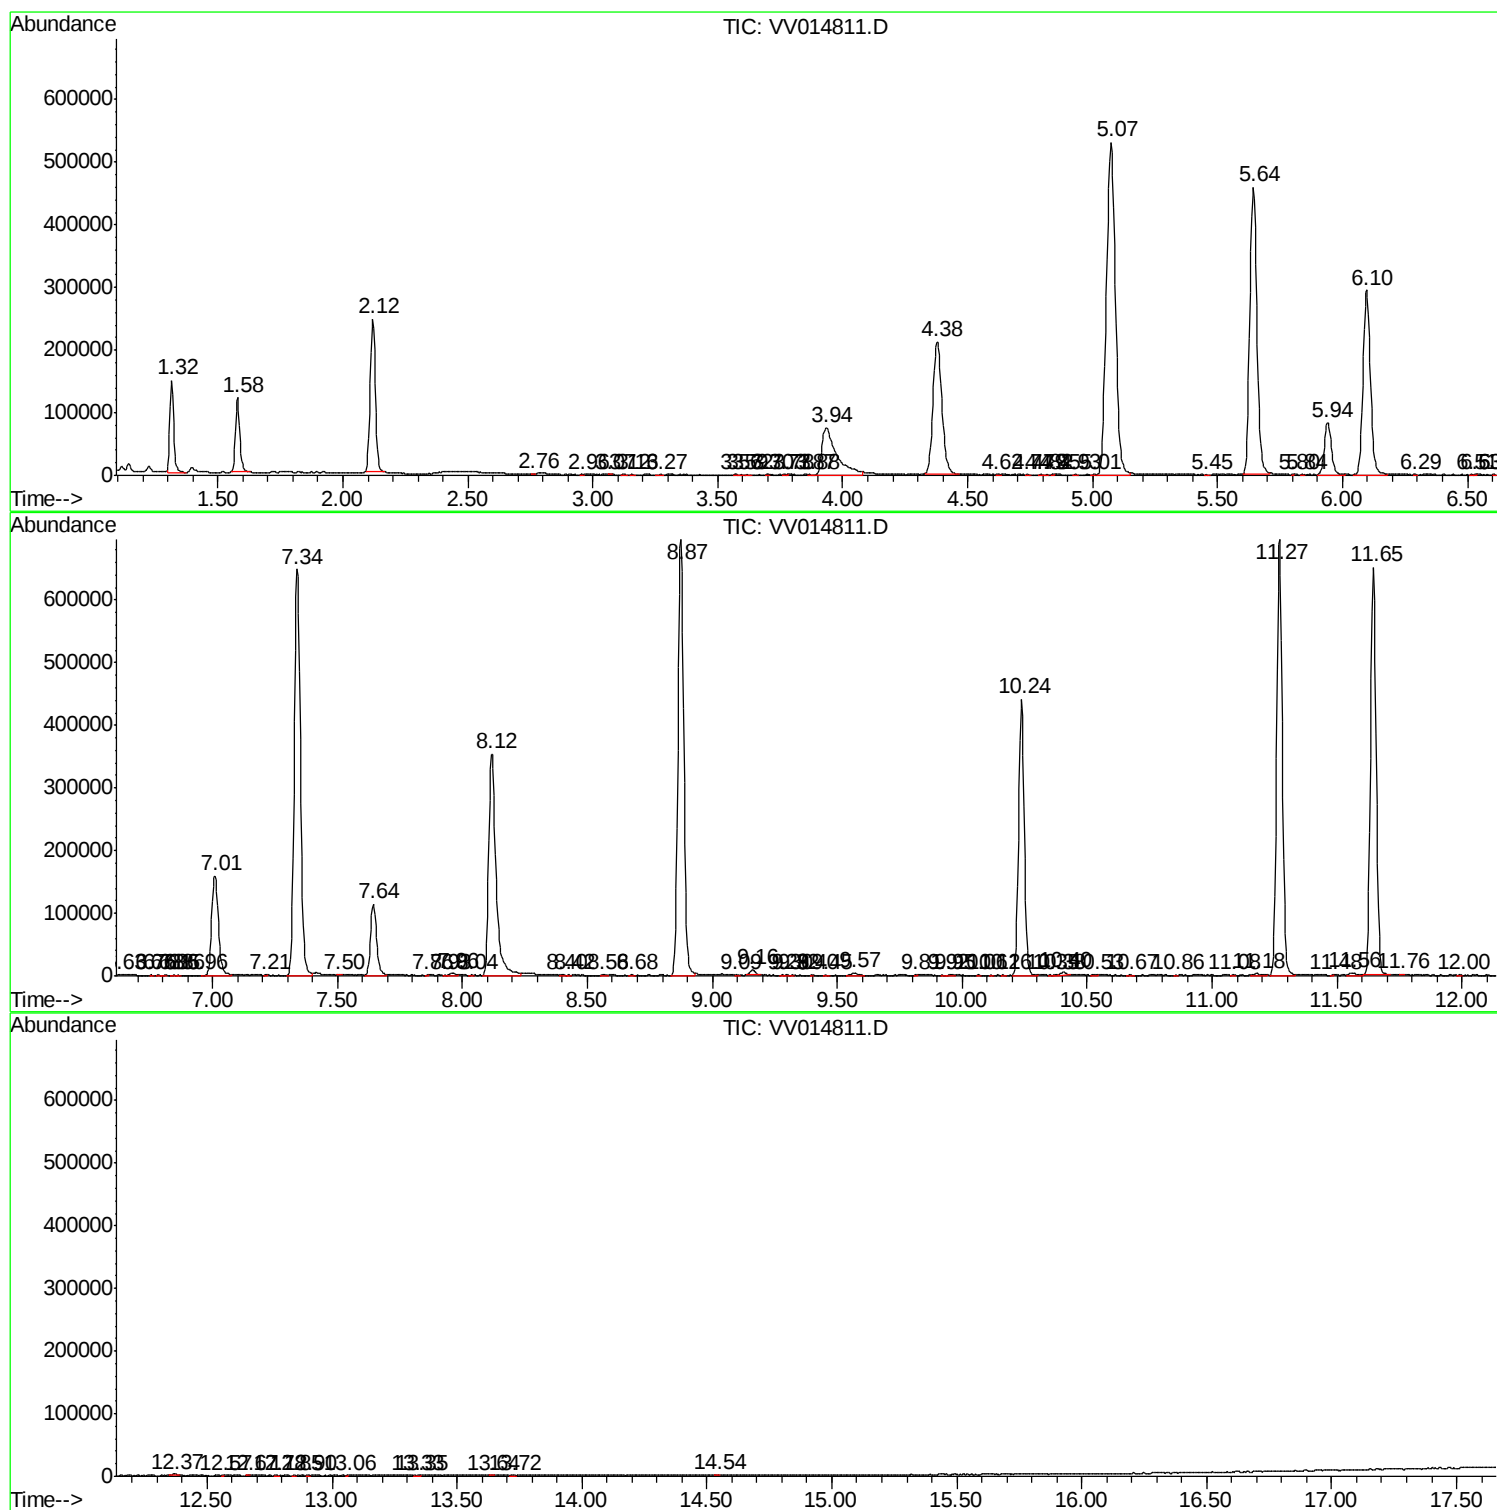

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014811.D
Acq On : 10 Mar 2020 19:02
Operator : SY/MD
Sample : L1858-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014811.D
Acq On : 10 Mar 2020 19:02
Operator : SY/MD
Sample : L1858-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRF6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc