

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014815.D
 Acq On : 10 Mar 2020 20:39
 Operator : SY/MD
 Sample : L1840-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	137972	149505	11.34%	1.416%
2	1.579	144	152	170	rVB	118798	148529	11.27%	1.406%
3	2.119	311	320	338	rVB	240822	339043	25.73%	3.211%
4	2.666	488	490	493	rVB2	664	319	0.02%	0.003%
5	2.727	507	509	512	rBV2	489	244	0.02%	0.002%
6	2.836	538	543	546	rBV4	627	477	0.04%	0.005%
7	2.862	548	551	556	rBV3	377	337	0.03%	0.003%
8	3.080	616	619	622	rBV2	432	403	0.03%	0.004%
9	3.154	641	642	647	rVB2	389	212	0.02%	0.002%
10	3.244	665	670	672	rBV3	585	467	0.04%	0.004%
11	3.280	678	681	683	rBV3	748	441	0.03%	0.004%
12	3.386	710	714	716	rBV4	596	490	0.04%	0.005%
13	3.447	731	733	735	rBV2	423	215	0.02%	0.002%
14	3.486	741	745	752	rVB4	426	478	0.04%	0.005%
15	3.547	760	764	766	rBV3	584	318	0.02%	0.003%
16	3.576	770	773	774	rBV2	443	274	0.02%	0.003%
17	3.640	791	793	796	rBV	335	217	0.02%	0.002%
18	3.659	796	799	803	rBV2	343	275	0.02%	0.003%
19	3.711	813	815	818	rVB	568	303	0.02%	0.003%
20	3.733	820	822	823	rBV	523	234	0.02%	0.002%
21	3.855	858	860	865	rVB3	440	294	0.02%	0.003%
22	3.936	870	885	922	rBV	67314	283551	21.52%	2.685%
23	4.376	1007	1022	1047	rVB	209400	514494	39.04%	4.872%
24	4.643	1104	1105	1107	rBV	492	239	0.02%	0.002%
25	4.685	1115	1118	1120	rBV2	430	298	0.02%	0.003%
26	4.746	1133	1137	1140	rBV3	927	708	0.05%	0.007%
27	4.794	1150	1152	1154	rBV3	526	274	0.02%	0.003%
28	4.852	1168	1170	1173	rBV3	410	245	0.02%	0.002%
29	4.871	1173	1176	1178	rVV3	498	300	0.02%	0.003%
30	4.923	1188	1192	1194	rBV2	430	257	0.02%	0.002%
31	4.994	1211	1214	1215	rBV	617	274	0.02%	0.003%
32	5.074	1221	1239	1262	rBV2	529729	1317806	100.00%	12.479%
33	5.392	1336	1338	1340	rVB	625	251	0.02%	0.002%
34	5.402	1340	1341	1344	rBV	525	315	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014815.D
 Acq On : 10 Mar 2020 20:39
 Operator : SY/MD
 Sample : L1840-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	5.486	1364	1367	1369	rBV	622	309	0.02%	0.003%
36	5.524	1374	1379	1381	rBV3	516	434	0.03%	0.004%
37	5.559	1387	1390	1395	rVB3	846	720	0.05%	0.007%
38	5.582	1395	1397	1401	rBV	741	441	0.03%	0.004%
39	5.643	1401	1416	1439	rBV	450847	892125	67.70%	8.448%
40	5.791	1460	1462	1464	rBV2	500	261	0.02%	0.002%
41	5.916	1497	1501	1503	rBV4	1405	1201	0.09%	0.011%
42	6.045	1538	1541	1542	rBV2	401	211	0.02%	0.002%
43	6.096	1542	1557	1582	rVV	294393	596269	45.25%	5.646%
44	6.225	1595	1597	1599	rBV4	899	558	0.04%	0.005%
45	6.350	1634	1636	1638	rBV	485	233	0.02%	0.002%
46	6.363	1638	1640	1644	rBV	681	500	0.04%	0.005%
47	6.534	1690	1693	1696	rBV2	614	418	0.03%	0.004%
48	6.576	1703	1706	1711	rBV4	348	382	0.03%	0.004%
49	6.643	1716	1727	1734	rBV9	1501	3176	0.24%	0.030%
50	7.006	1829	1840	1858	rBV	161203	286639	21.75%	2.714%
51	7.338	1930	1943	1963	rBV	639067	1093981	83.02%	10.359%
52	7.588	2017	2021	2025	rBV4	803	437	0.03%	0.004%
53	7.643	2027	2038	2061	rBV	115038	192781	14.63%	1.826%
54	7.752	2068	2072	2074	rBV3	887	673	0.05%	0.006%
55	7.884	2109	2113	2115	rVV4	583	385	0.03%	0.004%
56	7.965	2129	2138	2149	rVB5	2991	5753	0.44%	0.054%
57	8.039	2159	2161	2164	rVB3	753	386	0.03%	0.004%
58	8.064	2164	2169	2171	rBV2	417	339	0.03%	0.003%
59	8.116	2173	2185	2218	rBV	361377	714111	54.19%	6.762%
60	8.537	2315	2316	2320	rVB2	402	228	0.02%	0.002%
61	8.563	2320	2324	2325	rBV	532	339	0.03%	0.003%
62	8.601	2331	2336	2337	rBV2	743	466	0.04%	0.004%
63	8.874	2408	2421	2443	rBV	688846	1105616	83.90%	10.470%
64	9.373	2574	2576	2578	rBV2	441	211	0.02%	0.002%
65	9.559	2632	2634	2635	rBV	443	224	0.02%	0.002%
66	9.691	2672	2675	2677	rVB2	466	215	0.02%	0.002%
67	9.762	2695	2697	2704	rVB3	539	395	0.03%	0.004%
68	9.810	2710	2712	2714	rBV	395	245	0.02%	0.002%
69	9.855	2723	2726	2728	rVB	665	314	0.02%	0.003%
70	9.923	2743	2747	2750	rBV4	498	451	0.03%	0.004%
71	10.029	2778	2780	2783	rVB2	513	237	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014815.D
 Acq On : 10 Mar 2020 20:39
 Operator : SY/MD
 Sample : L1840-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.051	2783	2787	2789	rBV2	606	431	0.03%	0.004%
73	10.064	2789	2791	2793	rBV2	440	248	0.02%	0.002%
74	10.093	2798	2800	2803	rVB	540	273	0.02%	0.003%
75	10.145	2814	2816	2821	rVB2	370	246	0.02%	0.002%
76	10.173	2823	2825	2831	rVB3	762	338	0.03%	0.003%
77	10.238	2832	2845	2861	rBV	440312	680689	51.65%	6.446%
78	10.408	2886	2898	2908	rVB5	4089	7415	0.56%	0.070%
79	10.498	2924	2926	2927	rBV3	601	240	0.02%	0.002%
80	10.675	2979	2981	2984	rBV2	643	340	0.03%	0.003%
81	10.701	2988	2989	2992	rBV2	378	226	0.02%	0.002%
82	10.852	3033	3036	3039	rBV	353	211	0.02%	0.002%
83	10.871	3039	3042	3043	rBV	1001	484	0.04%	0.005%
84	10.939	3057	3063	3070	rVB4	1727	1938	0.15%	0.018%
85	11.096	3109	3112	3114	rVB3	576	352	0.03%	0.003%
86	11.135	3122	3124	3126	rBV	451	267	0.02%	0.003%
87	11.154	3128	3130	3133	rVB2	418	208	0.02%	0.002%
88	11.183	3133	3139	3142	rBV4	821	1012	0.08%	0.010%
89	11.270	3154	3166	3185	rBV	682143	1056672	80.18%	10.006%
90	11.517	3235	3243	3254	rBV2	18915	36646	2.78%	0.347%
91	11.643	3271	3282	3303	rBV	670076	1079016	81.88%	10.218%
92	11.945	3367	3376	3385	rBV3	13374	24313	1.84%	0.230%
93	12.080	3415	3418	3420	rVB2	739	351	0.03%	0.003%
94	12.257	3467	3473	3474	rBV3	1023	887	0.07%	0.008%
95	12.366	3505	3507	3510	rBV2	543	374	0.03%	0.004%
96	12.537	3558	3560	3563	rBV3	697	353	0.03%	0.003%
97	12.794	3638	3640	3643	rBV3	691	444	0.03%	0.004%
98	13.318	3801	3803	3804	rBV	480	249	0.02%	0.002%
99	13.923	3989	3991	3993	rBV2	687	318	0.02%	0.003%
100	14.286	4098	4104	4107	rBV7	1574	1932	0.15%	0.018%


Sum of corrected areas: 10560224

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014815.D
Acq On : 10 Mar 2020 20:39
Operator : SY/MD
Sample : L1840-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

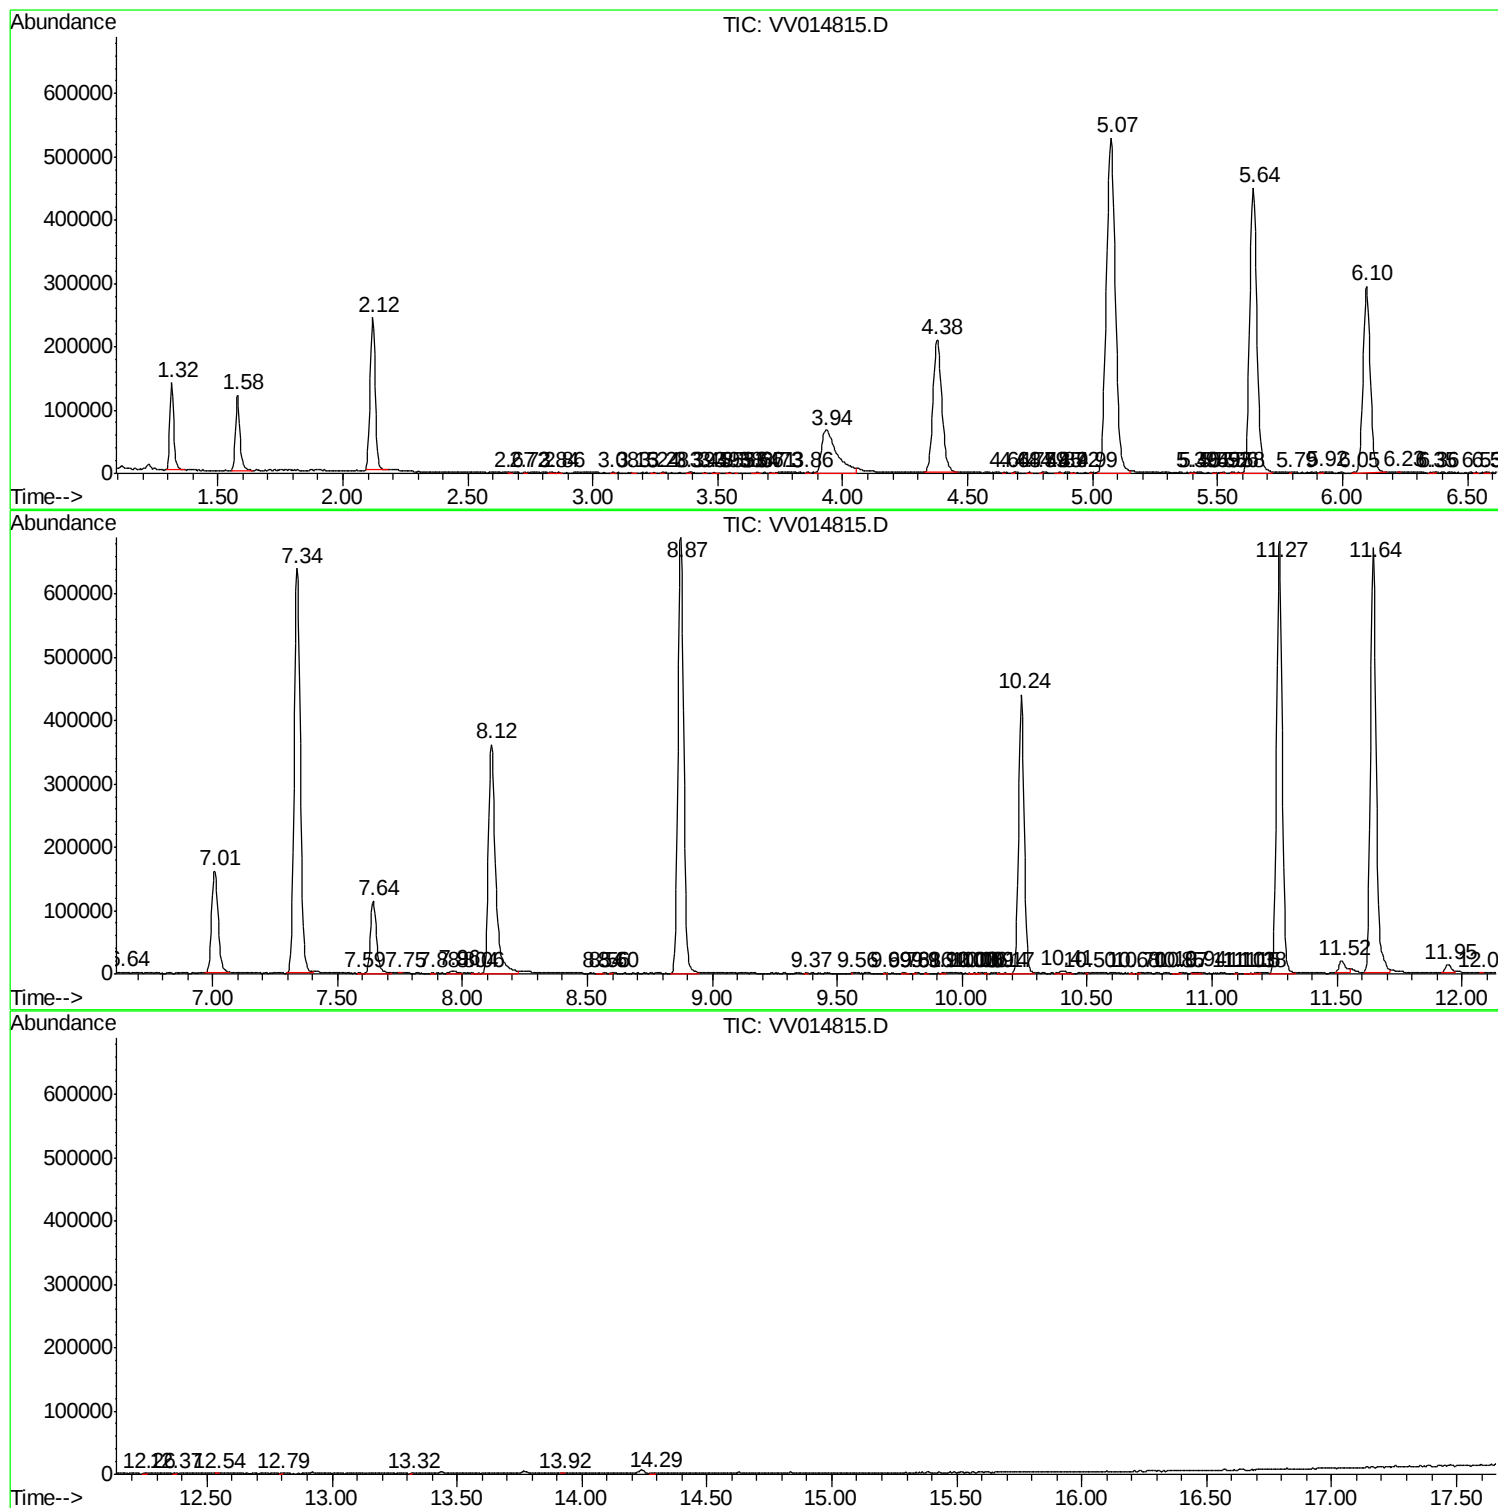

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014815.D
Acq On : 10 Mar 2020 20:39
Operator : SY/MD
Sample : L1840-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014815.D
Acq On : 10 Mar 2020 20:39
Operator : SY/MD
Sample : L1840-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc