

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014816.D
 Acq On : 10 Mar 2020 21:04
 Operator : SY/MD
 Sample : L1840-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	138701	148102	11.40%	1.429%
2	1.579	145	152	164	rVB	115902	136624	10.51%	1.318%
3	2.119	310	320	339	rBV	239080	342777	26.38%	3.307%
4	2.765	519	521	523	rBV2	694	295	0.02%	0.003%
5	2.852	547	548	551	rBV	519	245	0.02%	0.002%
6	2.939	573	575	578	rVB2	534	275	0.02%	0.003%
7	2.962	578	582	585	rBV2	413	407	0.03%	0.004%
8	3.103	624	626	631	rBV3	394	317	0.02%	0.003%
9	3.132	631	635	639	rVV3	587	462	0.04%	0.004%
10	3.190	648	653	656	rBV	651	588	0.05%	0.006%
11	3.251	670	672	675	rBV	625	404	0.03%	0.004%
12	3.376	707	711	714	rBV2	323	286	0.02%	0.003%
13	3.392	714	716	718	rBV2	641	317	0.02%	0.003%
14	3.521	753	756	763	rVV2	473	592	0.05%	0.006%
15	3.640	788	793	796	rBV	317	372	0.03%	0.004%
16	3.695	807	810	813	rBV	514	263	0.02%	0.003%
17	3.717	815	817	820	rBV2	423	274	0.02%	0.003%
18	3.859	860	861	866	rBV4	501	369	0.03%	0.004%
19	3.929	871	883	930	rBV	68330	288634	22.21%	2.785%
20	4.376	1004	1022	1047	rBV	209096	521707	40.15%	5.034%
21	4.585	1084	1087	1090	rBV2	521	342	0.03%	0.003%
22	4.621	1096	1098	1101	rBV2	351	254	0.02%	0.002%
23	4.701	1121	1123	1127	rVB3	546	264	0.02%	0.003%
24	4.904	1182	1186	1189	rBV4	500	430	0.03%	0.004%
25	4.971	1201	1207	1209	rBV3	475	405	0.03%	0.004%
26	5.074	1221	1239	1264	rBV2	521051	1299456	100.00%	12.538%
27	5.270	1297	1300	1302	rBV2	689	450	0.03%	0.004%
28	5.341	1321	1322	1326	rVB3	675	422	0.03%	0.004%
29	5.560	1386	1390	1391	rBV2	330	245	0.02%	0.002%
30	5.643	1401	1416	1436	rBV	445599	881346	67.82%	8.504%
31	5.897	1492	1495	1498	rBV2	612	378	0.03%	0.004%
32	5.920	1498	1502	1503	rBV2	1572	1106	0.09%	0.011%
33	6.096	1542	1557	1577	rBV	291120	586470	45.13%	5.659%
34	6.328	1627	1629	1632	rBV	469	354	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014816.D
 Acq On : 10 Mar 2020 21:04
 Operator : SY/MD
 Sample : L1840-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.479	1672	1676	1677	rBV2	420	328	0.03%	0.003%
36	6.505	1682	1684	1688	rVB2	481	259	0.02%	0.002%
37	6.531	1688	1692	1696	rBV2	620	523	0.04%	0.005%
38	6.588	1709	1710	1713	rBV	502	240	0.02%	0.002%
39	6.621	1717	1720	1721	rBV3	1146	645	0.05%	0.006%
40	6.707	1744	1747	1750	rBV3	711	544	0.04%	0.005%
41	7.010	1826	1841	1864	rBV	157013	283942	21.85%	2.740%
42	7.203	1897	1901	1903	rVB3	590	400	0.03%	0.004%
43	7.215	1903	1905	1908	rBV3	771	614	0.05%	0.006%
44	7.248	1913	1915	1917	rBV2	451	276	0.02%	0.003%
45	7.293	1927	1929	1930	rBV	626	286	0.02%	0.003%
46	7.338	1931	1943	1967	rVV	629537	1087059	83.65%	10.489%
47	7.643	2024	2038	2057	rBV	109449	189710	14.60%	1.830%
48	7.797	2081	2086	2087	rBV3	394	277	0.02%	0.003%
49	7.897	2115	2117	2122	rBV3	693	484	0.04%	0.005%
50	7.929	2122	2127	2128	rVV	501	382	0.03%	0.004%
51	7.965	2130	2138	2145	rVV6	2598	4083	0.31%	0.039%
52	8.003	2148	2150	2156	rVB4	1163	851	0.07%	0.008%
53	8.116	2173	2185	2216	rBV	355026	716160	55.11%	6.910%
54	8.614	2338	2340	2343	rBV3	532	297	0.02%	0.003%
55	8.691	2362	2364	2366	rVB	501	256	0.02%	0.002%
56	8.711	2366	2370	2373	rBV3	685	742	0.06%	0.007%
57	8.875	2406	2421	2442	rBV	665478	1084044	83.42%	10.460%
58	9.035	2469	2471	2476	rBV5	655	342	0.03%	0.003%
59	9.129	2496	2500	2502	rVB2	665	424	0.03%	0.004%
60	9.141	2502	2504	2506	rBV	401	263	0.02%	0.003%
61	9.225	2526	2530	2531	rBV3	435	248	0.02%	0.002%
62	9.257	2535	2540	2544	rBV3	727	760	0.06%	0.007%
63	9.299	2551	2553	2555	rVB	612	267	0.02%	0.003%
64	9.341	2564	2566	2571	rBV2	616	567	0.04%	0.005%
65	9.392	2580	2582	2583	rBV	587	245	0.02%	0.002%
66	9.492	2610	2613	2616	rBV2	490	305	0.02%	0.003%
67	9.563	2631	2635	2641	rBV4	888	919	0.07%	0.009%
68	9.659	2663	2665	2667	rVV2	549	335	0.03%	0.003%
69	9.688	2671	2674	2678	rBV	387	312	0.02%	0.003%
70	9.871	2728	2731	2735	rVB4	525	327	0.03%	0.003%
71	9.894	2735	2738	2739	rBV	528	273	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014816.D
 Acq On : 10 Mar 2020 21:04
 Operator : SY/MD
 Sample : L1840-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBES7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.932	2744	2750	2752	rBV	595	463	0.04%	0.004%
73	10.112	2802	2806	2808	rBV	437	250	0.02%	0.002%
74	10.238	2832	2845	2860	rBV	430362	671276	51.66%	6.477%
75	10.350	2874	2880	2884	rBV4	926	1215	0.09%	0.012%
76	10.447	2908	2910	2916	rVB3	717	475	0.04%	0.005%
77	10.476	2916	2919	2921	rBV3	763	490	0.04%	0.005%
78	10.582	2948	2952	2956	rVB4	719	581	0.04%	0.006%
79	10.672	2978	2980	2984	rVB2	554	347	0.03%	0.003%
80	10.707	2988	2991	2992	rBV	364	253	0.02%	0.002%
81	10.752	3002	3005	3006	rBV2	809	399	0.03%	0.004%
82	10.926	3056	3059	3063	rBV2	1235	1139	0.09%	0.011%
83	11.009	3083	3085	3091	rVB4	730	482	0.04%	0.005%
84	11.093	3109	3111	3116	rVB	630	392	0.03%	0.004%
85	11.122	3116	3120	3124	rBV2	710	647	0.05%	0.006%
86	11.270	3154	3166	3184	rBV	672305	1031078	79.35%	9.949%
87	11.382	3198	3201	3203	rBV2	1054	705	0.05%	0.007%
88	11.521	3236	3244	3249	rBV5	8820	14150	1.09%	0.137%
89	11.646	3271	3283	3306	rBV	639070	1028396	79.14%	9.923%
90	11.952	3368	3378	3386	rBV4	6855	12554	0.97%	0.121%
91	12.122	3429	3431	3434	rBV3	728	331	0.03%	0.003%
92	12.382	3508	3512	3515	rBV3	466	444	0.03%	0.004%
93	12.611	3581	3583	3586	rBB3	613	323	0.02%	0.003%
94	12.839	3650	3654	3656	rBV3	463	357	0.03%	0.003%
95	13.006	3703	3706	3708	rBV3	519	321	0.02%	0.003%
96	13.087	3728	3731	3733	rBV3	864	704	0.05%	0.007%
97	13.138	3743	3747	3750	rVB3	684	464	0.04%	0.004%
98	13.244	3777	3780	3782	rBV2	715	491	0.04%	0.005%
99	13.765	3939	3942	3949	rVB6	1542	1521	0.12%	0.015%
100	13.849	3965	3968	3970	rBV	696	486	0.04%	0.005%


Sum of corrected areas: 10363955

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014816.D
Acq On : 10 Mar 2020 21:04
Operator : SY/MD
Sample : L1840-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

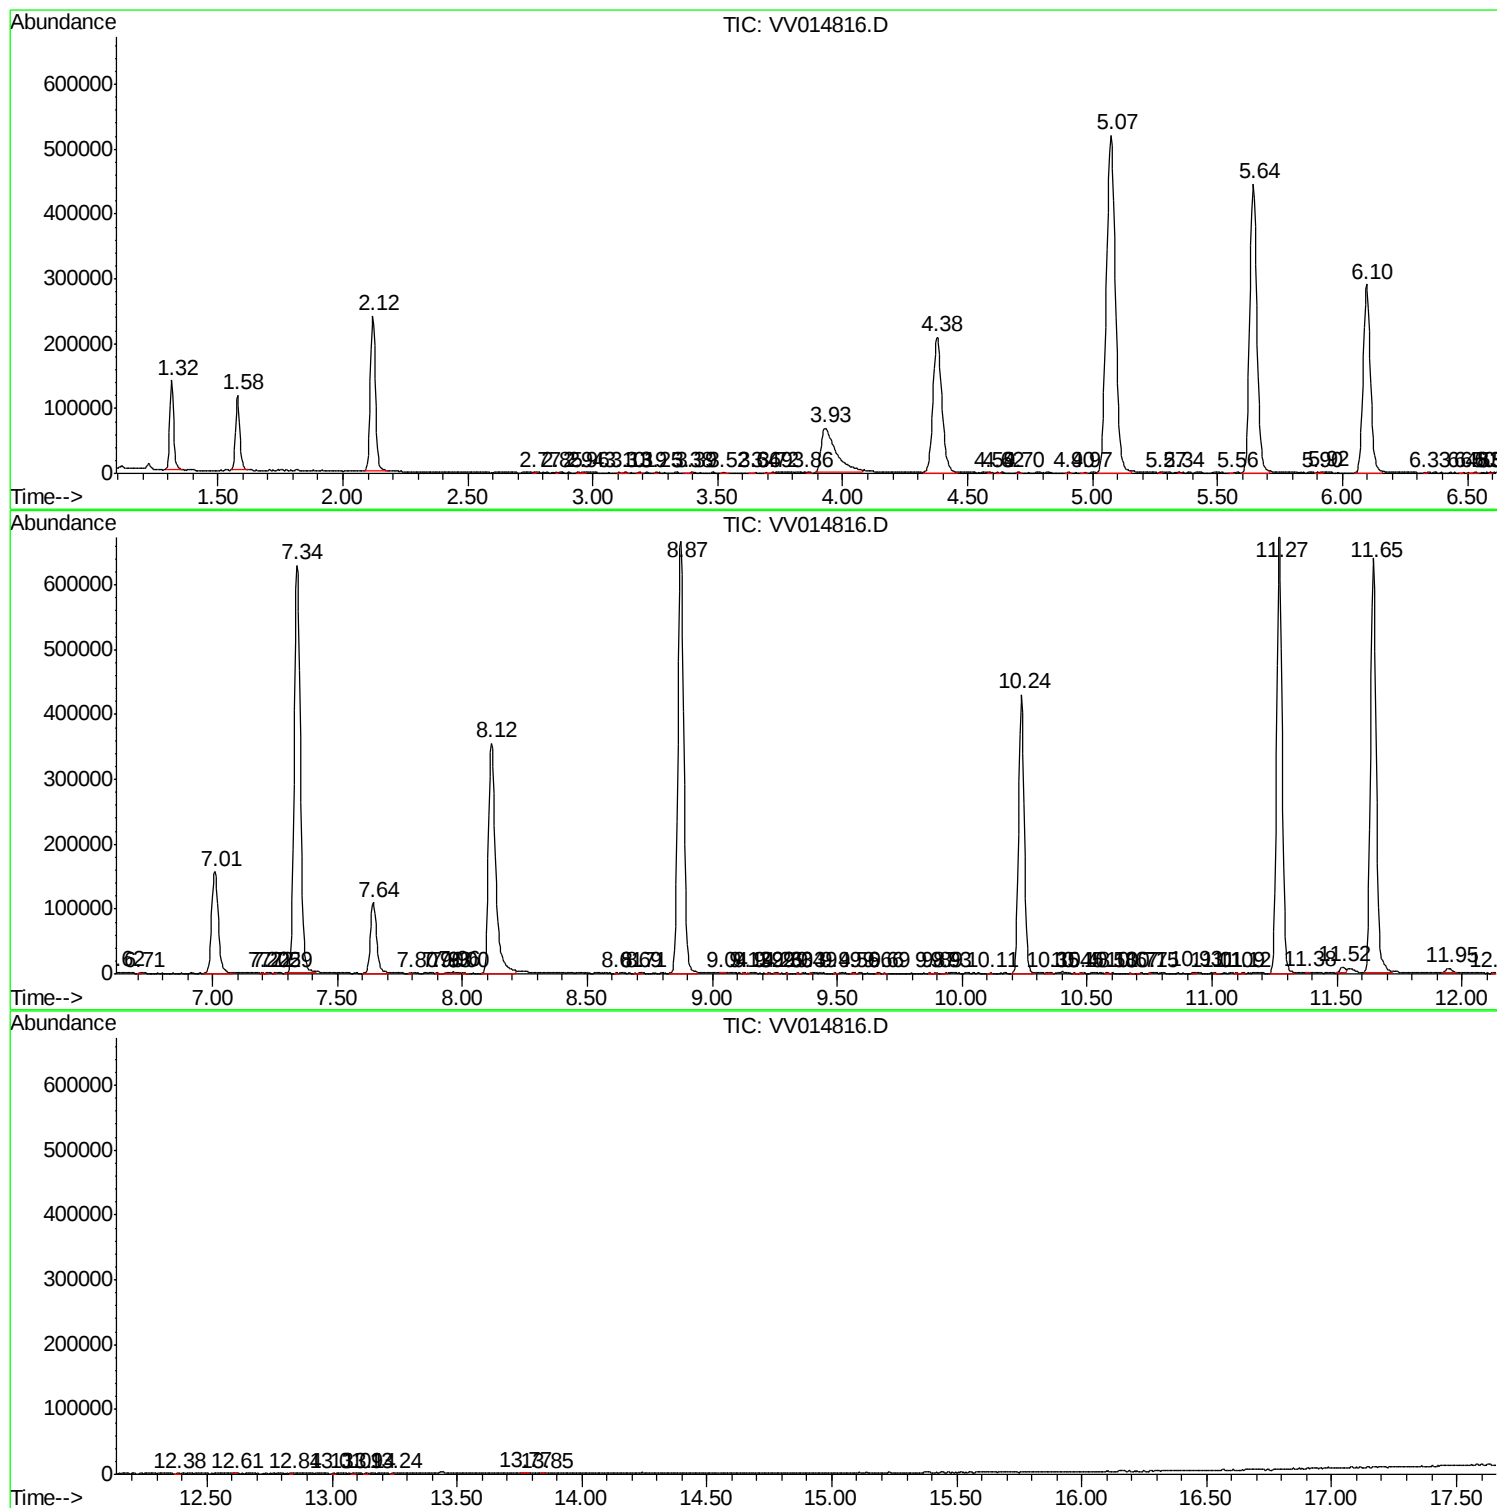

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014816.D
Acq On : 10 Mar 2020 21:04
Operator : SY/MD
Sample : L1840-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014816.D
Acq On : 10 Mar 2020 21:04
Operator : SY/MD
Sample : L1840-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBES7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc