

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014824.D
 Acq On : 11 Mar 2020 00:17
 Operator : SY/MD
 Sample : L1840-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.113	4	7	21	rVB	24562	23970	1.50%	0.187%
2	1.315	63	70	83	rVB	182841	197571	12.36%	1.542%
3	1.576	145	151	167	rVB	150002	181036	11.32%	1.413%
4	2.119	311	320	337	rVB	300645	427670	26.75%	3.338%
5	2.347	389	391	393	rBV	989	479	0.03%	0.004%
6	2.666	487	490	493	rBV3	847	569	0.04%	0.004%
7	2.949	574	578	579	rBV3	658	383	0.02%	0.003%
8	3.145	636	639	641	rVB2	598	312	0.02%	0.002%
9	3.199	654	656	658	rBV2	461	277	0.02%	0.002%
10	3.225	662	664	669	rBV2	482	378	0.02%	0.003%
11	3.341	699	700	702	rVB	370	127	0.01%	0.001%
12	3.376	708	711	712	rBV2	622	301	0.02%	0.002%
13	3.447	732	733	734	rBV2	163	42	0.00%	0.000%
14	3.470	738	740	743	rVB2	504	247	0.02%	0.002%
15	3.482	743	744	747	rBV	313	136	0.01%	0.001%
16	3.531	756	759	762	rBV	464	327	0.02%	0.003%
17	3.598	777	780	781	rBV	359	157	0.01%	0.001%
18	3.637	788	792	795	rBV3	403	307	0.02%	0.002%
19	3.669	800	802	804	rVB2	286	117	0.01%	0.001%
20	3.685	804	807	809	rBV	290	165	0.01%	0.001%
21	3.711	812	815	816	rBV	321	175	0.01%	0.001%
22	3.749	818	827	832	rBV5	2605	4817	0.30%	0.038%
23	3.929	870	883	930	rBV2	85558	357059	22.33%	2.787%
24	4.376	1007	1022	1044	rBV	254299	623643	39.00%	4.867%
25	4.678	1113	1116	1118	rBV4	590	348	0.02%	0.003%
26	4.756	1138	1140	1144	rBV	331	205	0.01%	0.002%
27	4.852	1167	1170	1173	rBV2	495	284	0.02%	0.002%
28	4.868	1173	1175	1177	rBV2	433	221	0.01%	0.002%
29	4.904	1182	1186	1188	rBV2	335	293	0.02%	0.002%
30	4.939	1195	1197	1198	rBV2	333	114	0.01%	0.001%
31	4.984	1207	1211	1212	rBV4	435	246	0.02%	0.002%
32	5.071	1219	1238	1271	rBV2	637887	1599065	100.00%	12.479%
33	5.305	1309	1311	1312	rBV	302	115	0.01%	0.001%
34	5.508	1369	1374	1379	rVB4	834	722	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014824.D
 Acq On : 11 Mar 2020 00:17
 Operator : SY/MD
 Sample : L1840-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	5.531	1379	1381	1382	rBV	304	140	0.01%	0.001%
36	5.540	1382	1384	1386	rVB	375	147	0.01%	0.001%
37	5.566	1390	1392	1393	rBV	563	247	0.02%	0.002%
38	5.643	1401	1416	1442	rBV	555155	1105762	69.15%	8.629%
39	5.929	1497	1505	1517	rVB9	2971	5337	0.33%	0.042%
40	6.096	1541	1557	1579	rBV	355845	722851	45.20%	5.641%
41	6.209	1590	1592	1594	rBV2	958	489	0.03%	0.004%
42	6.273	1610	1612	1616	rVB2	958	542	0.03%	0.004%
43	6.312	1622	1624	1626	rBV3	584	228	0.01%	0.002%
44	6.344	1632	1634	1636	rVB	682	284	0.02%	0.002%
45	6.357	1636	1638	1640	rVB	290	101	0.01%	0.001%
46	6.376	1640	1644	1646	rVB2	546	356	0.02%	0.003%
47	6.395	1646	1650	1652	rBV	516	340	0.02%	0.003%
48	6.486	1675	1678	1679	rBV2	453	300	0.02%	0.002%
49	6.527	1689	1691	1692	rBV	390	158	0.01%	0.001%
50	6.714	1745	1749	1752	rBV4	711	586	0.04%	0.005%
51	6.826	1782	1784	1785	rBV	357	180	0.01%	0.001%
52	6.936	1813	1818	1823	rBV2	497	548	0.03%	0.004%
53	7.010	1828	1841	1862	rBV	193659	344033	21.51%	2.685%
54	7.129	1877	1878	1880	rBV	439	220	0.01%	0.002%
55	7.280	1923	1925	1927	rBV2	410	218	0.01%	0.002%
56	7.338	1930	1943	1964	rBV	787422	1344579	84.09%	10.493%
57	7.575	2015	2017	2021	rVB3	756	433	0.03%	0.003%
58	7.643	2028	2038	2053	rBV2	129469	224505	14.04%	1.752%
59	7.823	2092	2094	2095	rBV2	460	161	0.01%	0.001%
60	7.836	2096	2098	2103	rVB	612	330	0.02%	0.003%
61	7.968	2129	2139	2144	rBV2	3060	5072	0.32%	0.040%
62	8.116	2173	2185	2223	rBV	438129	871595	54.51%	6.802%
63	8.463	2291	2293	2296	rBV3	584	322	0.02%	0.003%
64	8.559	2321	2323	2327	rVB3	657	453	0.03%	0.004%
65	8.588	2327	2332	2333	rBV	773	518	0.03%	0.004%
66	8.678	2357	2360	2362	rBV2	452	260	0.02%	0.002%
67	8.707	2367	2369	2370	rBV2	393	173	0.01%	0.001%
68	8.730	2374	2376	2378	rBV	437	237	0.01%	0.002%
69	8.820	2401	2404	2408	rVB2	839	512	0.03%	0.004%
70	8.874	2408	2421	2445	rBV	840383	1350580	84.46%	10.540%
71	9.071	2480	2482	2484	rBV2	558	159	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014824.D
 Acq On : 11 Mar 2020 00:17
 Operator : SY/MD
 Sample : L1840-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.087	2485	2487	2491	rVB4	933	544	0.03%	0.004%
73	9.344	2563	2567	2568	rBV	442	284	0.02%	0.002%
74	9.354	2568	2570	2571	rBV	267	92	0.01%	0.001%
75	9.395	2580	2583	2586	rVB2	326	229	0.01%	0.002%
76	9.473	2604	2607	2614	rVB5	754	705	0.04%	0.006%
77	9.521	2618	2622	2624	rBV	473	322	0.02%	0.003%
78	9.604	2644	2648	2649	rBV2	603	339	0.02%	0.003%
79	9.794	2706	2707	2708	rBV	163	50	0.00%	0.000%
80	9.868	2728	2730	2731	rBV	320	127	0.01%	0.001%
81	10.022	2775	2778	2780	rBV3	413	245	0.02%	0.002%
82	10.238	2833	2845	2863	rBV	527760	816263	51.05%	6.370%
83	10.392	2881	2893	2895	rBV8	8452	14943	0.93%	0.117%
84	10.669	2974	2979	2980	rBV2	769	656	0.04%	0.005%
85	10.874	3038	3043	3049	rVB4	1514	1128	0.07%	0.009%
86	11.048	3091	3097	3100	rBV3	1175	1128	0.07%	0.009%
87	11.270	3154	3166	3186	rBV	845067	1309521	81.89%	10.220%
88	11.646	3271	3283	3301	rBV	793115	1236935	77.35%	9.653%
89	11.945	3364	3376	3388	rBV4	9649	18730	1.17%	0.146%
90	12.218	3459	3461	3463	rBV	708	382	0.02%	0.003%
91	12.485	3532	3544	3548	rBV6	4046	6398	0.40%	0.050%


Sum of corrected areas: 12813855

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014824.D
Acq On : 11 Mar 2020 00:17
Operator : SY/MD
Sample : L1840-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

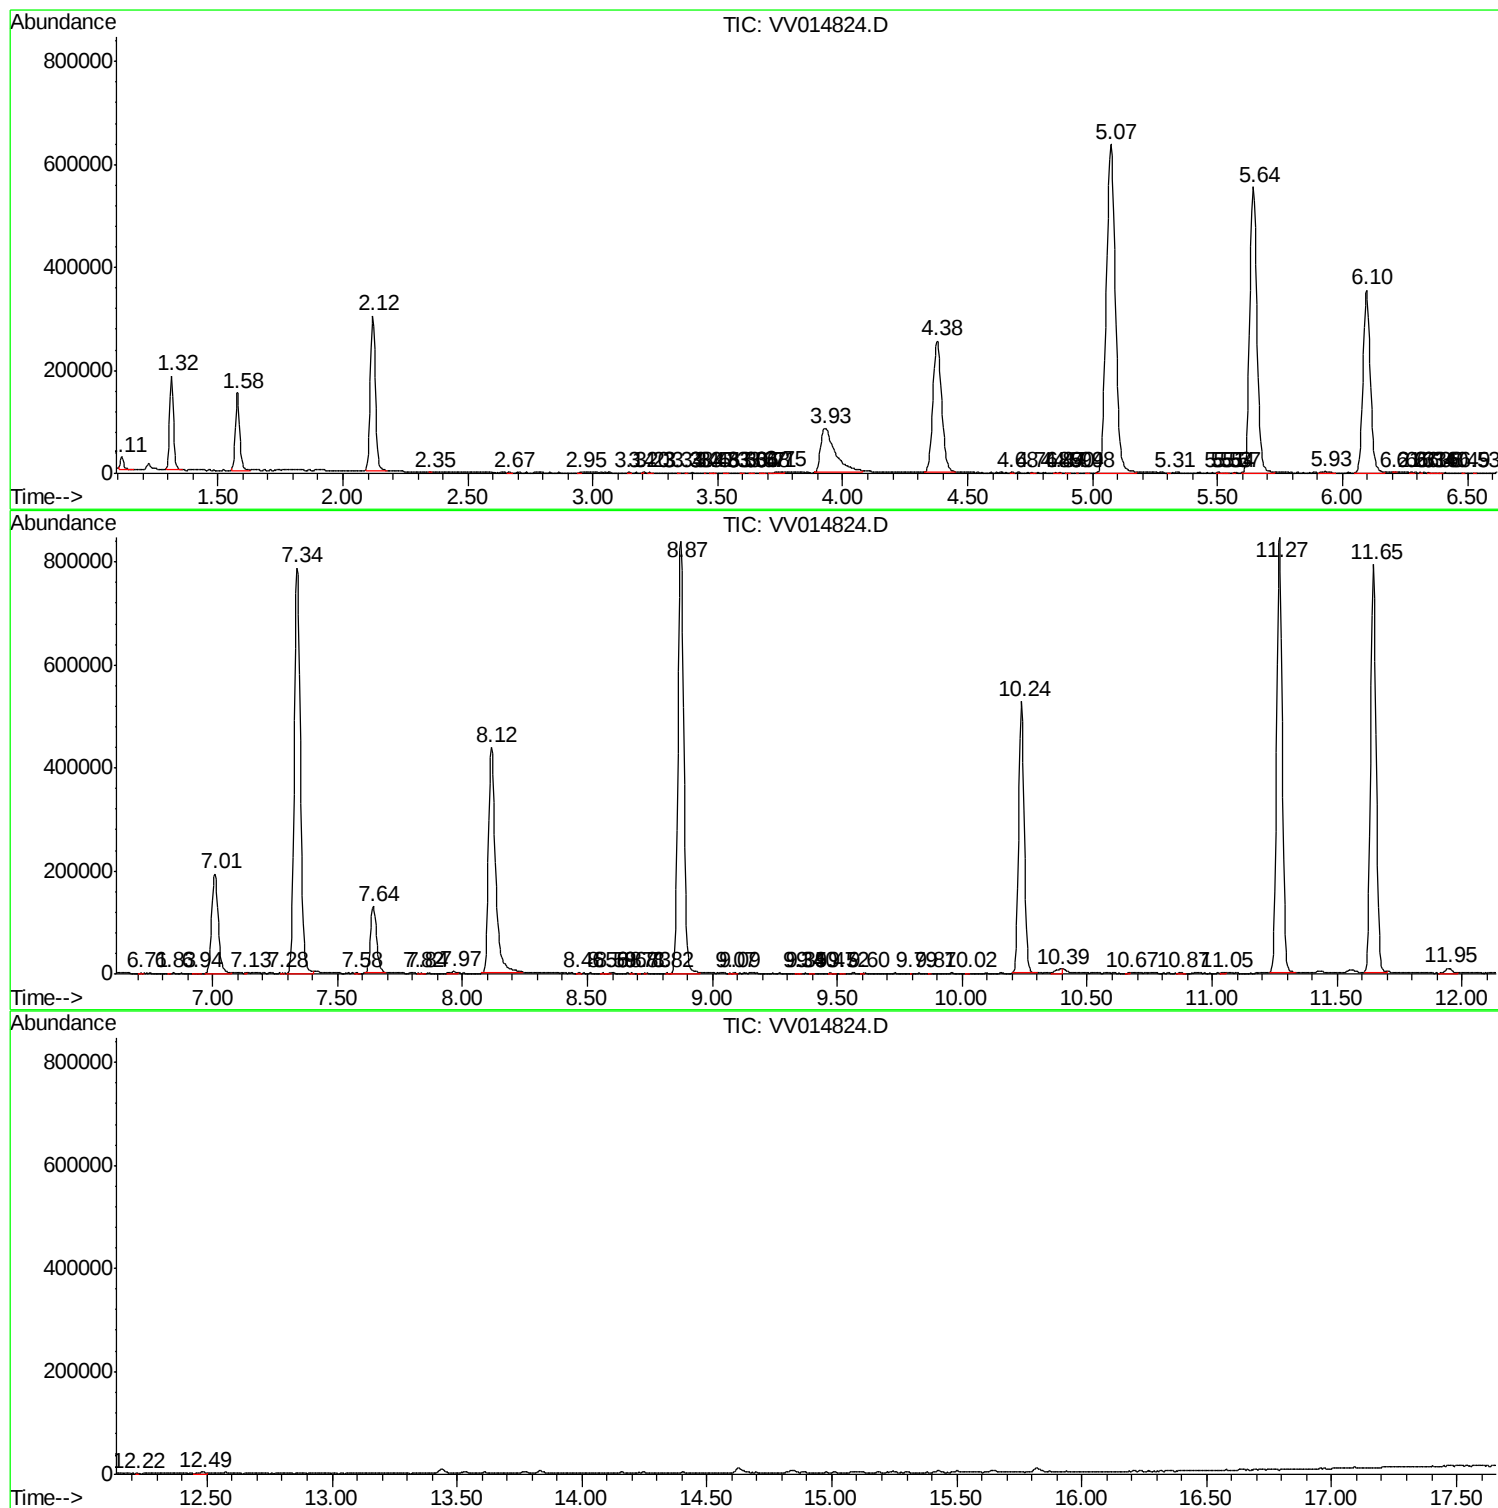

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014824.D
Acq On : 11 Mar 2020 00:17
Operator : SY/MD
Sample : L1840-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014824.D
Acq On : 11 Mar 2020 00:17
Operator : SY/MD
Sample : L1840-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc