

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014825.D
 Acq On : 11 Mar 2020 00:41
 Operator : SY/MD
 Sample : L1840-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	177040	185359	11.62%	1.473%
2	1.579	145	152	167	rVB	146625	179686	11.27%	1.428%
3	2.119	311	320	340	rVB	294743	419574	26.31%	3.335%
4	2.611	471	473	475	rBV	501	282	0.02%	0.002%
5	2.679	491	494	497	rBV3	717	360	0.02%	0.003%
6	2.917	564	568	570	rBV2	429	366	0.02%	0.003%
7	3.142	634	638	641	rVV2	475	340	0.02%	0.003%
8	3.154	641	642	646	rVB	401	273	0.02%	0.002%
9	3.376	709	711	714	rBV	401	214	0.01%	0.002%
10	3.444	729	732	735	rBV2	421	272	0.02%	0.002%
11	3.460	735	737	739	rBV	291	190	0.01%	0.002%
12	3.489	744	746	749	rVB	657	325	0.02%	0.003%
13	3.598	778	780	783	rVB2	518	298	0.02%	0.002%
14	3.627	787	789	792	rBV	389	194	0.01%	0.002%
15	3.650	792	796	797	rBV	345	206	0.01%	0.002%
16	3.753	814	828	839	rBV7	2525	7133	0.45%	0.057%
17	3.936	871	885	926	rBV2	80563	351852	22.06%	2.797%
18	4.380	1007	1023	1047	rBV	249833	614397	38.53%	4.883%
19	4.669	1111	1113	1115	rBV	692	332	0.02%	0.003%
20	4.682	1115	1117	1119	rBV2	558	308	0.02%	0.002%
21	4.730	1130	1132	1133	rBV	504	171	0.01%	0.001%
22	4.785	1144	1149	1152	rBV4	504	532	0.03%	0.004%
23	4.833	1161	1164	1166	rBV2	453	277	0.02%	0.002%
24	4.881	1177	1179	1183	rBV2	637	348	0.02%	0.003%
25	4.945	1192	1199	1201	rBV2	639	666	0.04%	0.005%
26	5.074	1218	1239	1270	rBV2	634513	1594691	100.00%	12.675%
27	5.283	1302	1304	1306	rBV2	577	275	0.02%	0.002%
28	5.325	1315	1317	1320	rBV	1062	424	0.03%	0.003%
29	5.367	1326	1330	1331	rBV	452	264	0.02%	0.002%
30	5.428	1345	1349	1352	rBV3	863	712	0.04%	0.006%
31	5.473	1358	1363	1364	rBV2	576	356	0.02%	0.003%
32	5.643	1403	1416	1443	rVB	545157	1076712	67.52%	8.558%
33	5.855	1478	1482	1483	rBV	518	319	0.02%	0.003%
34	5.929	1497	1505	1516	rVB6	2773	5016	0.31%	0.040%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014825.D
 Acq On : 11 Mar 2020 00:41
 Operator : SY/MD
 Sample : L1840-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	5.971	1516	1518	1520	rVB	521	234	0.01%	0.002%
36	5.987	1520	1523	1525	rBV3	585	363	0.02%	0.003%
37	6.035	1532	1538	1540	rBV3	697	734	0.05%	0.006%
38	6.096	1542	1557	1575	rBV	355347	718992	45.09%	5.715%
39	6.379	1643	1645	1647	rBV	453	216	0.01%	0.002%
40	6.402	1650	1652	1655	rBV2	746	408	0.03%	0.003%
41	6.450	1664	1667	1668	rBV	648	355	0.02%	0.003%
42	6.482	1674	1677	1679	rBV2	343	240	0.02%	0.002%
43	6.547	1694	1697	1700	rVB2	342	200	0.01%	0.002%
44	6.569	1700	1704	1705	rBV	789	412	0.03%	0.003%
45	6.781	1767	1770	1773	rVB3	406	202	0.01%	0.002%
46	6.794	1773	1774	1777	rVB2	487	181	0.01%	0.001%
47	6.814	1777	1780	1786	rBV4	551	583	0.04%	0.005%
48	6.859	1790	1794	1799	rVB3	527	573	0.04%	0.005%
49	6.891	1799	1804	1806	rBV3	454	428	0.03%	0.003%
50	6.932	1813	1817	1820	rVB	439	272	0.02%	0.002%
51	6.949	1820	1822	1824	rBV	767	422	0.03%	0.003%
52	7.010	1827	1841	1863	rBV	191627	344912	21.63%	2.741%
53	7.260	1916	1919	1921	rBV3	463	345	0.02%	0.003%
54	7.338	1931	1943	1959	rBV	779423	1327433	83.24%	10.551%
55	7.643	2025	2038	2059	rBV	134339	230410	14.45%	1.831%
56	7.817	2090	2092	2095	rVB2	432	195	0.01%	0.002%
57	7.862	2102	2106	2109	rBV4	621	497	0.03%	0.004%
58	7.878	2109	2111	2114	rVB	512	262	0.02%	0.002%
59	7.894	2114	2116	2117	rBV	556	289	0.02%	0.002%
60	7.932	2125	2128	2130	rBV3	571	373	0.02%	0.003%
61	8.116	2172	2185	2223	rBV2	438516	877038	55.00%	6.971%
62	8.527	2311	2313	2317	rVB	528	271	0.02%	0.002%
63	8.746	2376	2381	2383	rBV2	445	409	0.03%	0.003%
64	8.772	2386	2389	2392	rVB3	549	386	0.02%	0.003%
65	8.804	2397	2399	2401	rBV2	423	210	0.01%	0.002%
66	8.875	2408	2421	2444	rBV	809808	1302889	81.70%	10.355%
67	9.135	2500	2502	2505	rBV2	497	228	0.01%	0.002%
68	9.151	2505	2507	2510	rBV2	995	705	0.04%	0.006%
69	9.202	2519	2523	2524	rBV	439	270	0.02%	0.002%
70	9.328	2560	2562	2568	rVB2	587	433	0.03%	0.003%
71	9.386	2578	2580	2583	rVB	422	192	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031020\
 Data File : VV014825.D
 Acq On : 11 Mar 2020 00:41
 Operator : SY/MD
 Sample : L1840-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBET6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	9.479	2604	2609	2611	rBV2	607	498	0.03%	0.004%
73	9.627	2652	2655	2657	rBV2	439	243	0.02%	0.002%
74	9.662	2665	2666	2670	rVB2	485	209	0.01%	0.002%
75	9.829	2712	2718	2722	rBV4	986	1205	0.08%	0.010%
76	9.900	2737	2740	2743	rBV3	637	405	0.03%	0.003%
77	9.942	2750	2753	2756	rBV2	1001	756	0.05%	0.006%
78	10.013	2773	2775	2777	rVV2	484	284	0.02%	0.002%
79	10.058	2787	2789	2791	rBV	440	200	0.01%	0.002%
80	10.100	2799	2802	2805	rBV2	472	314	0.02%	0.002%
81	10.238	2831	2845	2869	rBV	526702	825802	51.78%	6.564%
82	10.354	2877	2881	2882	rBV3	900	585	0.04%	0.005%
83	10.383	2882	2890	2891	rBV2	4613	4927	0.31%	0.039%
84	10.466	2914	2916	2919	rVB3	839	364	0.02%	0.003%
85	10.524	2928	2934	2936	rBV3	1439	1382	0.09%	0.011%
86	11.061	3099	3101	3105	rVB3	750	460	0.03%	0.004%
87	11.125	3116	3121	3123	rBV2	502	444	0.03%	0.004%
88	11.270	3154	3166	3187	rBV	816663	1250112	78.39%	9.936%
89	11.646	3271	3283	3304	rBV	769045	1205130	75.57%	9.578%
90	11.945	3369	3376	3388	rVB5	6299	11045	0.69%	0.088%
91	12.456	3533	3535	3536	rBV5	687	323	0.02%	0.003%
92	12.479	3536	3542	3553	rVB8	3984	6883	0.43%	0.055%
93	12.537	3558	3560	3563	rBV2	652	363	0.02%	0.003%
94	12.662	3596	3599	3600	rBV	582	325	0.02%	0.003%
95	12.710	3612	3614	3616	rBV2	500	277	0.02%	0.002%
96	12.804	3638	3643	3647	rBV5	1656	1976	0.12%	0.016%
97	13.289	3788	3794	3800	rBV6	1582	1939	0.12%	0.015%
98	13.344	3809	3811	3814	rBV	574	379	0.02%	0.003%
99	13.524	3864	3867	3872	rBV4	2457	2422	0.15%	0.019%
100	14.630	4204	4211	4217	rBV6	4759	7125	0.45%	0.057%


Sum of corrected areas: 12581663

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031020\
Data File : VV014825.D
Acq On : 11 Mar 2020 00:41
Operator : SY/MD
Sample : L1840-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

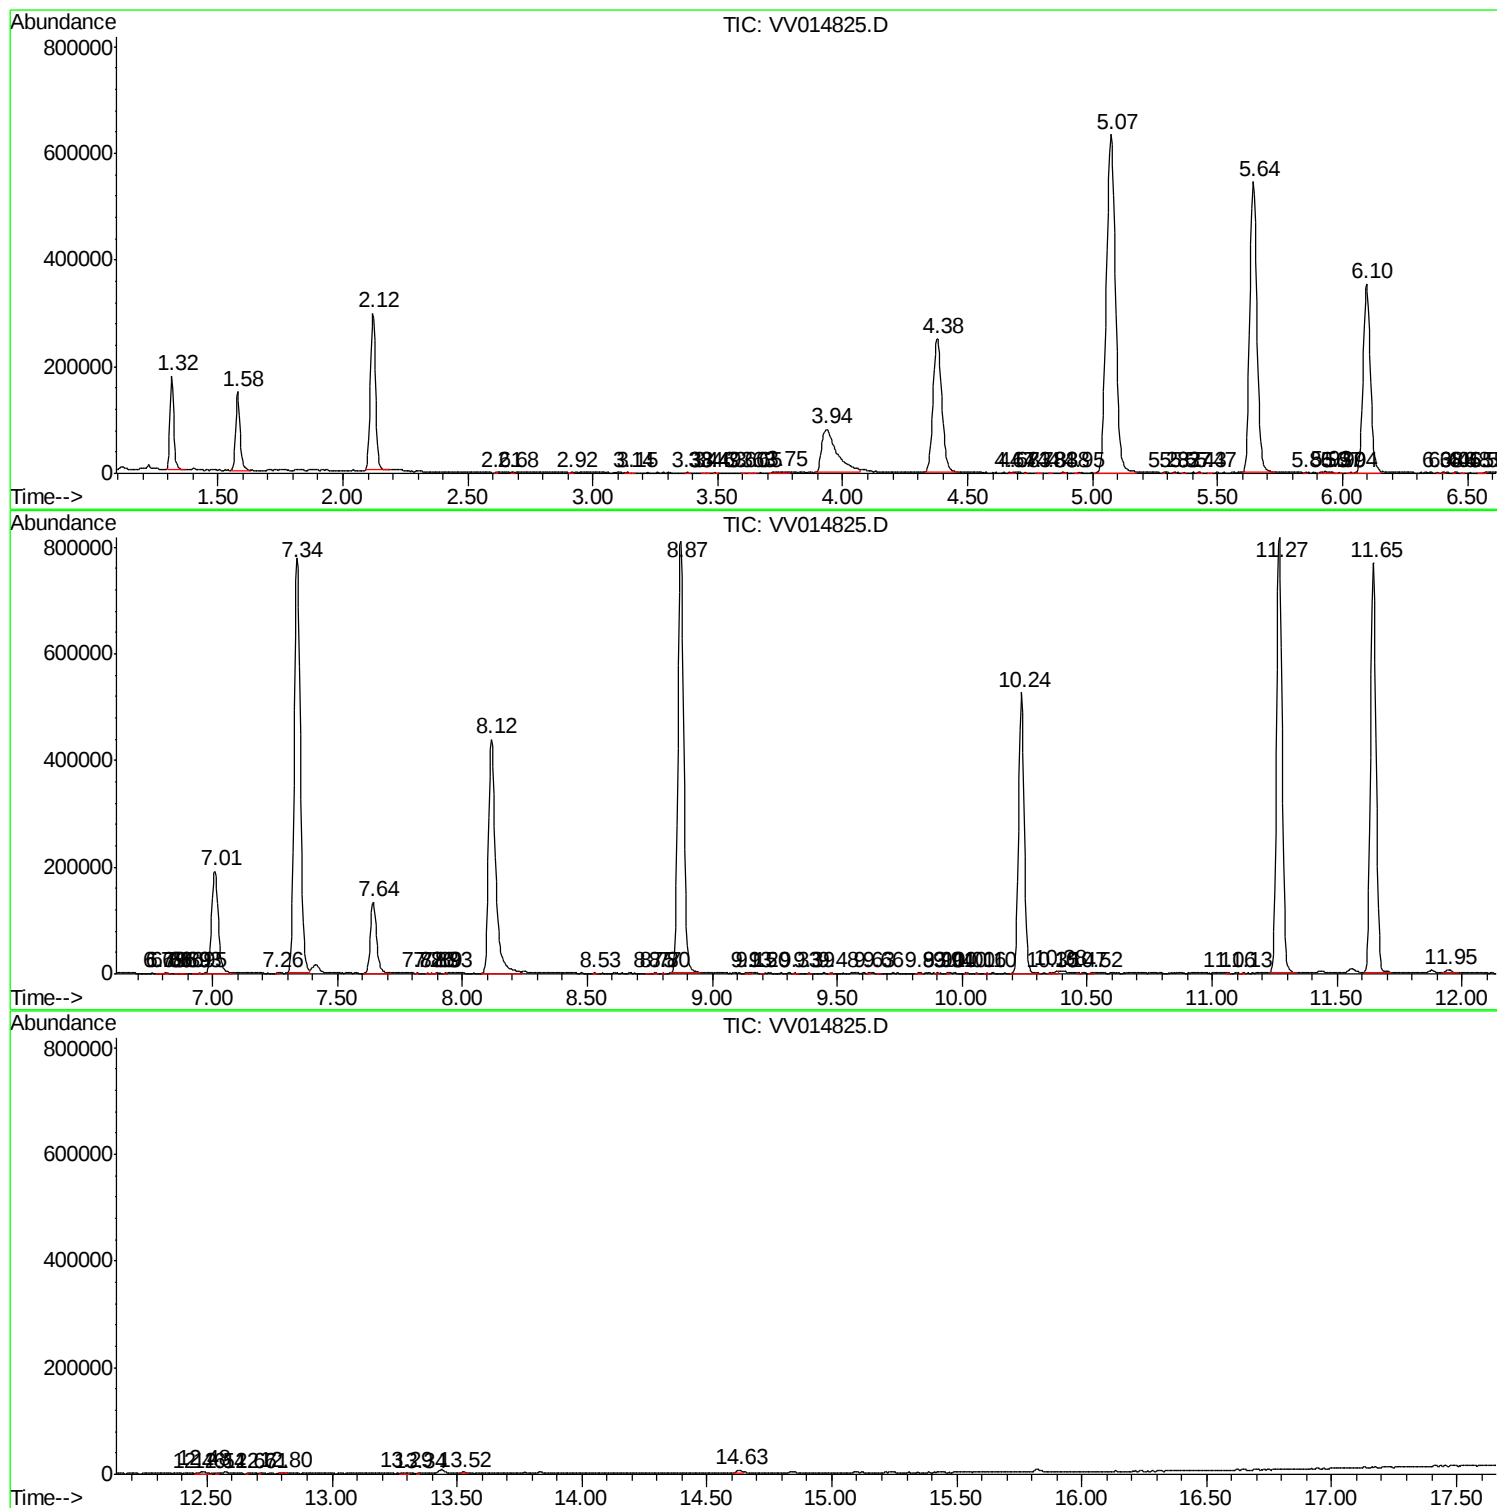

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014825.D
Acq On : 11 Mar 2020 00:41
Operator : SY/MD
Sample : L1840-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031020\
Data File : VV014825.D
Acq On : 11 Mar 2020 00:41
Operator : SY/MD
Sample : L1840-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBET6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc