


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031020\
 Data File : VV014789.D
 Acq On : 10 Mar 2020 09:12
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 11 03:49:31 2020

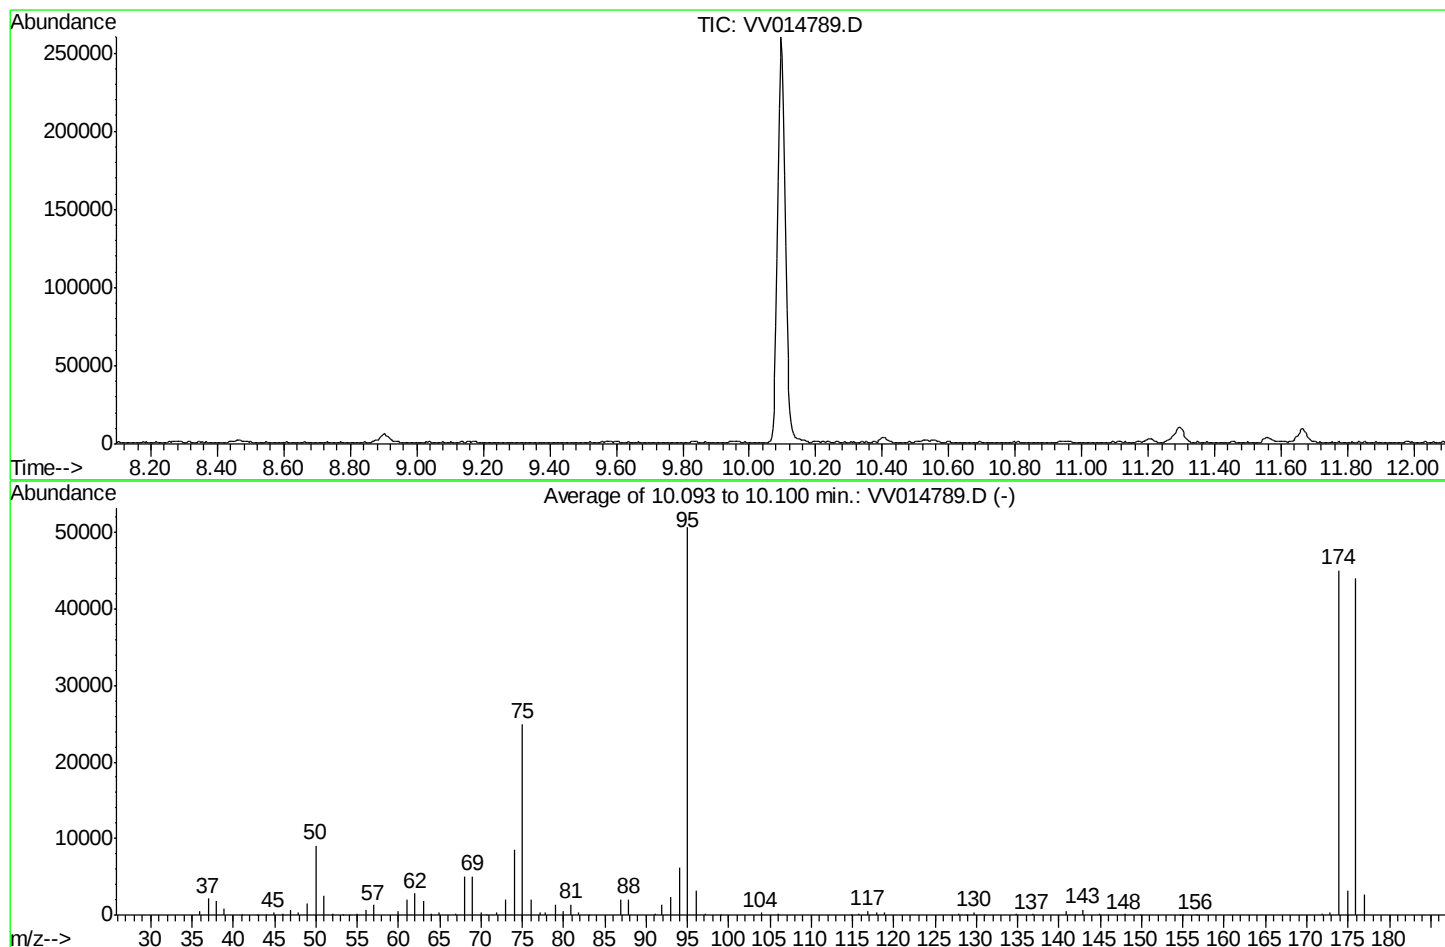

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	9109	PASS
75	95	30	80	49.2	24954	PASS
95	95	100	100	100.0	50690	PASS
96	95	5	9	6.3	3194	PASS
173	174	0.00	2	0.7	307	PASS
174	95	50	120	88.9	45077	PASS
175	174	5	9	7.0	3137	PASS
176	174	95	101	97.8	44101	PASS
177	176	5	9	6.2	2750	PASS

m/z	Abundance
35.90	562.0
37.00	2360.0
38.00	1772.0
38.90	730.0
39.90	385.0
41.10	143.0
42.90	125.0
44.00	552.0
44.90	375.0
46.00	170.0
46.90	685.0
48.00	340.0
49.00	1558.0
50.00	8603.0
51.00	2671.0
52.10	111.0
54.90	269.0
56.10	757.0
56.90	1239.0
59.90	468.0
61.00	1936.0
62.00	2769.0
63.00	1743.0
63.90	247.0
65.00	357.0
67.00	201.0
68.00	4875.0
69.00	5135.0
69.90	344.0
71.90	327.0
73.00	2203.0
74.00	8529.0
75.00	24888.0
76.00	1983.0
77.10	433.0
77.80	258.0
79.00	1356.0
79.90	506.0
80.90	1364.0
81.80	345.0
86.90	1841.0
87.90	1935.0
91.10	256.0
91.90	1343.0
93.00	2404.0
94.00	5943.0
95.00	49368.0
96.00	3462.0
97.20	196.0
99.00	145.0
103.90	264.0
106.00	157.0
114.80	103.0
115.80	194.0
116.80	471.0
117.90	283.0
118.80	313.0
127.80	170.0
129.70	362.0
134.80	154.0
136.80	182.0
140.90	489.0
141.90	109.0
142.90	753.0
144.90	169.0
147.90	156.0
149.80	116.0
155.00	120.0
172.00	199.0
173.90	43376.0
174.90	3033.0
175.90	42800.0
176.90	2666.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	518.0
37.00	2286.0
38.00	1854.0
38.90	786.0
39.90	373.0
41.10	126.0
42.90	120.0
44.00	639.0
44.90	325.0
46.00	177.0
46.90	648.0
47.90	276.0
49.00	1595.0
50.00	9415.0
51.00	2624.0
52.10	108.0
54.10	108.0
55.00	259.0
56.10	768.0
57.00	1309.0
59.90	432.0
61.00	2113.0
62.00	2961.0
63.00	1822.0
63.90	211.0
65.00	297.0
67.00	218.0
68.00	5213.0
69.00	5127.0
70.00	288.0
71.90	302.0
72.90	2080.0
74.00	8825.0
75.00	25864.0
76.00	2018.0
77.10	413.0
77.80	308.0
78.90	1400.0
79.90	478.0
80.90	1418.0
81.90	336.0
86.90	2087.0
87.90	2196.0
91.10	225.0
91.90	1281.0
92.90	2510.0
94.00	6380.0
95.00	52160.0
96.00	3280.0
97.20	180.0
99.00	114.0
103.90	317.0
106.00	159.0
115.80	256.0
116.90	545.0
117.90	312.0
118.90	268.0
127.80	186.0
128.70	118.0
129.80	371.0
134.80	120.0
136.80	150.0
140.90	419.0
142.90	733.0
144.90	158.0
147.90	127.0
154.70	110.0
156.60	108.0
171.90	208.0
172.90	479.0
173.90	46536.0
174.90	3287.0
175.90	45664.0
176.90	2798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	474.0
37.00	1982.0
38.00	1765.0
38.90	816.0
39.90	322.0
44.00	728.0
44.90	299.0
45.90	120.0
46.90	552.0
47.80	250.0
49.00	1551.0
50.00	9309.0
51.00	2446.0
52.10	133.0
53.30	111.0
55.00	230.0
56.00	660.0
57.00	1267.0
59.90	435.0
61.00	2088.0
62.00	2730.0
63.00	1749.0
64.00	170.0
64.90	236.0
66.90	213.0
68.00	4896.0
69.00	4814.0
70.00	367.0
70.70	103.0
71.90	254.0
72.90	1845.0
74.00	8344.0
75.00	24112.0
76.00	1942.0
77.10	322.0
77.80	294.0
78.90	1283.0
79.90	437.0
80.90	1353.0
81.90	351.0
83.00	119.0
86.90	1972.0
87.90	2122.0
91.00	192.0
91.90	1240.0
92.90	2368.0
94.00	6079.0
95.00	50544.0
96.00	2840.0
97.10	155.0
103.90	324.0
106.10	156.0
115.80	285.0
116.90	522.0
117.90	293.0
119.00	231.0
127.80	172.0
128.70	126.0
129.80	321.0
131.00	104.0
136.90	101.0
140.80	376.0
142.90	688.0
144.80	114.0
148.00	102.0
156.60	106.0
171.80	233.0
172.80	443.0
173.90	45320.0
174.90	3091.0
175.90	43840.0
176.90	2786.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

Scan 2788 (10.055 min): VV014789.D
BFB99

m/z	Abundance
36.80	111.0
39.90	414.0
43.90	576.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99