

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031021\
 Data File : VV020494.D
 Acq On : 10 Mar 2021 12:36
 Operator : SY/MD
 Sample : M1617-07DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0N3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VV020494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	27	rVB	12543	10795	1.30%	0.142%
2	1.307	74	83	95	rVB2	154755	182807	21.99%	2.410%
3	1.568	156	164	177	rVB	109910	123269	14.83%	1.625%
4	2.108	318	332	345	rBV	232965	332114	39.96%	4.378%
5	2.513	448	458	470	rVB	8511	14254	1.72%	0.188%
6	3.915	880	894	947	rBV3	273899	784848	94.43%	10.347%
7	4.355	1013	1031	1058	rBV2	141184	363206	43.70%	4.788%
8	5.053	1231	1248	1285	rBV3	337859	831133	100.00%	10.957%
9	5.622	1406	1425	1457	rBV	294402	598025	71.95%	7.884%
10	5.915	1502	1516	1536	rVB2	15046	32932	3.96%	0.434%
11	6.075	1552	1566	1585	rBV	183831	375073	45.13%	4.945%
12	6.992	1832	1851	1880	rBV2	86177	160690	19.33%	2.118%
13	7.320	1940	1953	1977	rBV	419421	736723	88.64%	9.712%
14	7.628	2039	2049	2074	rBV	50323	91513	11.01%	1.206%
15	8.095	2184	2194	2234	rBV2	275357	607335	73.07%	8.006%
16	8.857	2420	2431	2451	rBV	448878	735696	88.52%	9.699%
17	9.715	2690	2698	2715	rBV4	6623	13885	1.67%	0.183%
18	10.223	2845	2856	2872	rBV	120128	185102	22.27%	2.440%
19	11.255	3164	3177	3197	rBV	466173	724518	87.17%	9.551%
20	11.632	3282	3294	3312	rBV	430297	681628	82.01%	8.986%




Sum of corrected areas: 7585546

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031021\
Data File : VV020494.D
Acq On : 10 Mar 2021 12:36
Operator : SY/MD
Sample : M1617-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0N3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

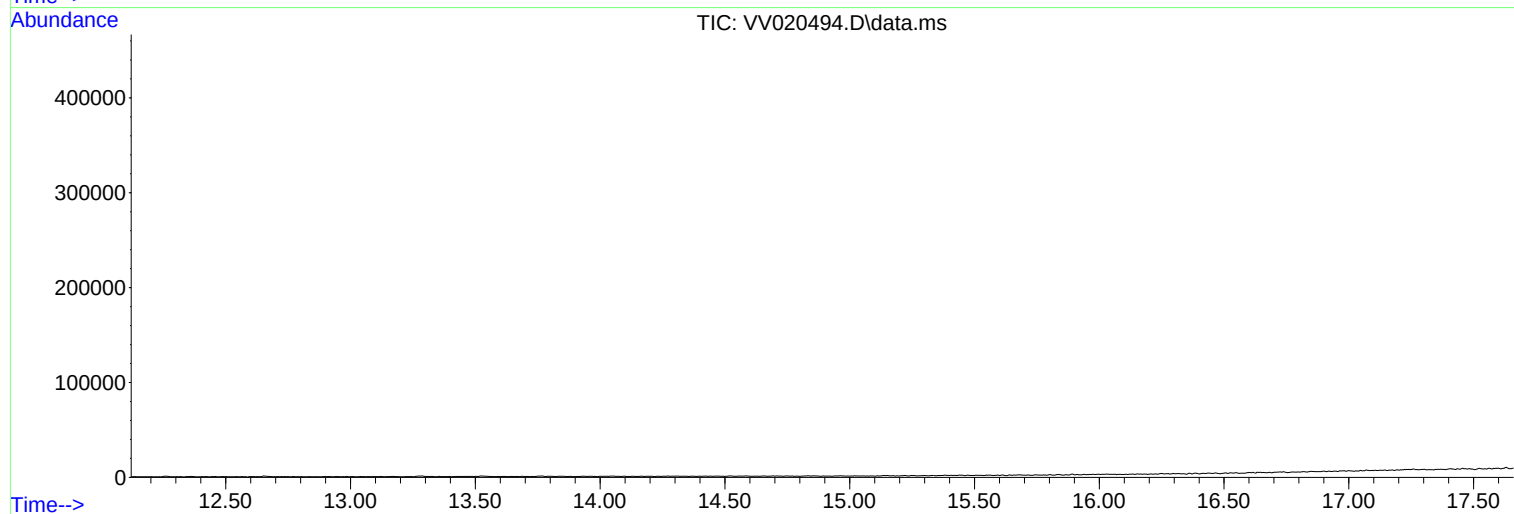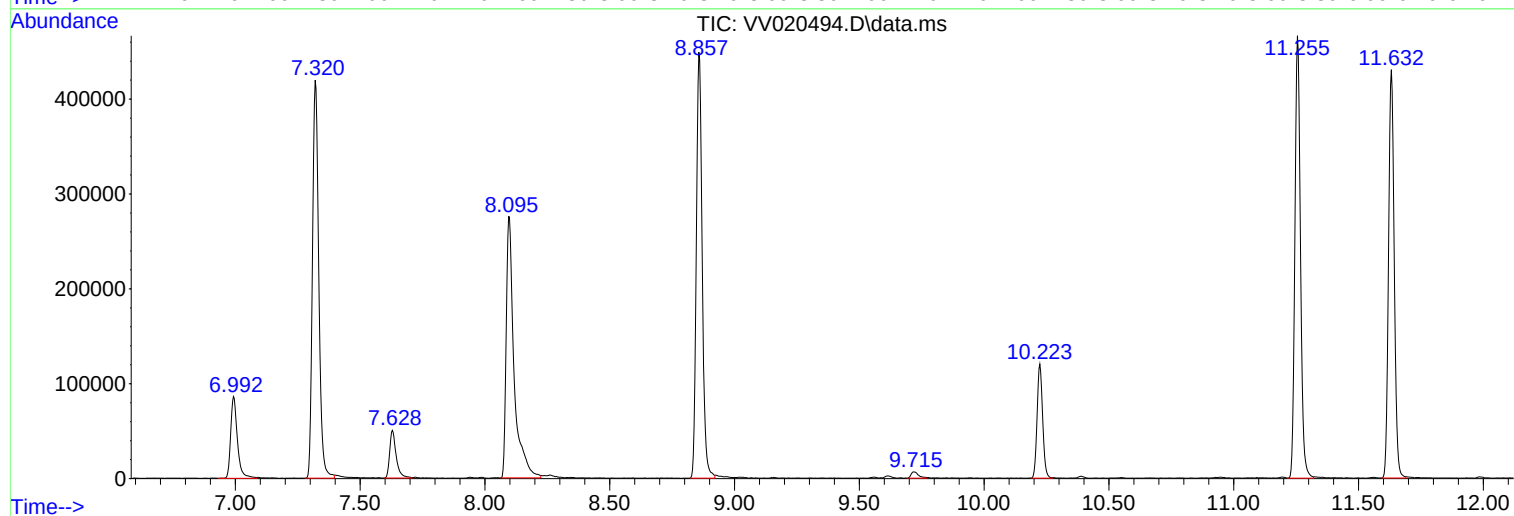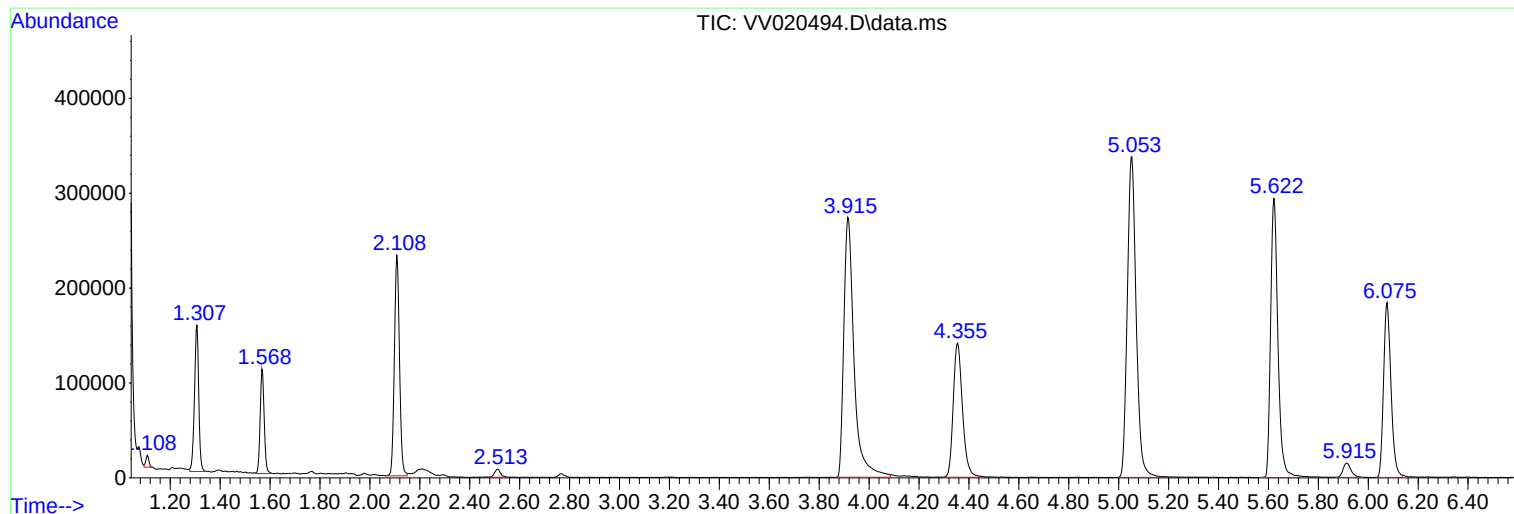

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031021\
Data File : VV020494.D
Acq On : 10 Mar 2021 12:36
Operator : SY/MD
Sample : M1617-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0N3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031021\
Data File : VV020494.D
Acq On : 10 Mar 2021 12:36
Operator : SY/MD
Sample : M1617-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0N3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
