
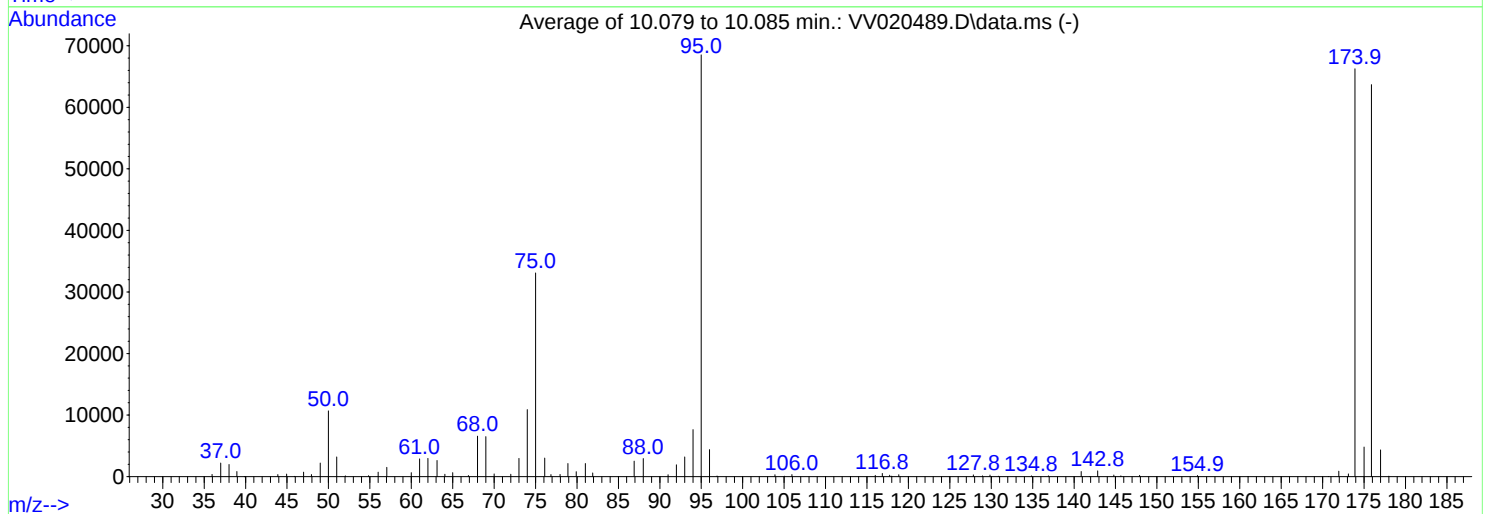


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031021\
 Data File : VV020489.D
 Acq On : 10 Mar 2021 08:55
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB35

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Mar 11 00:49:40 2021

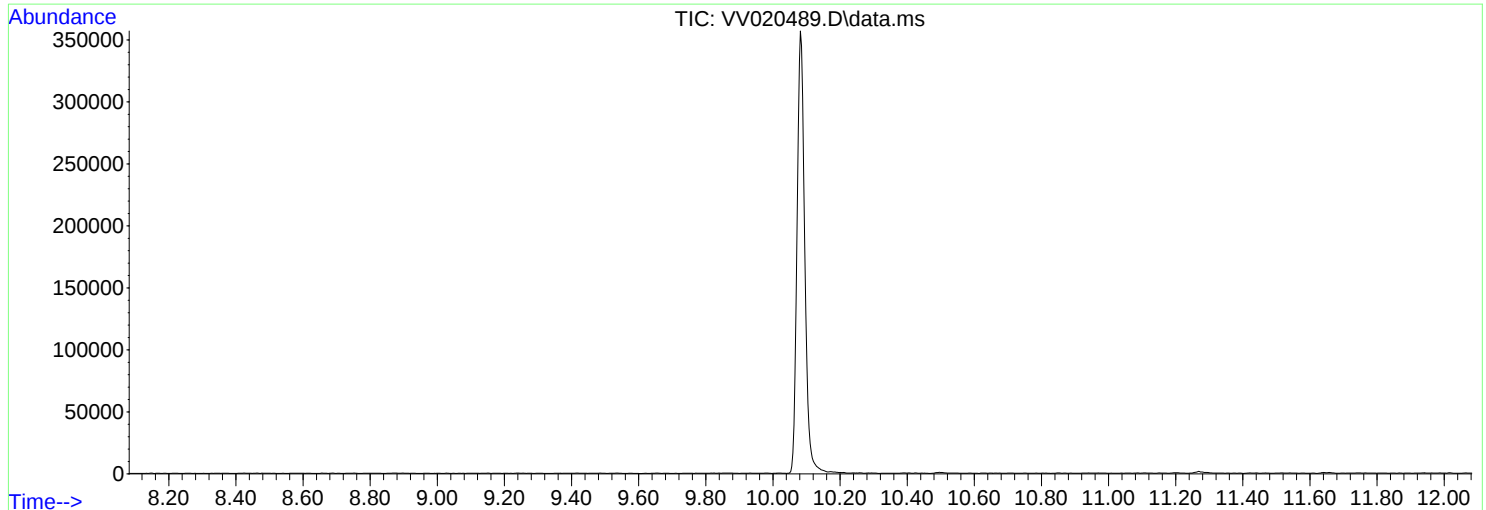

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	10690	PASS
75	95	30	80	48.3	33093	PASS
95	95	100	100	100.0	68523	PASS
96	95	5	9	6.4	4394	PASS
173	174	0.00	2	0.7	446	PASS
174	95	50	120	96.7	66245	PASS
175	174	5	9	7.3	4820	PASS
176	174	95	101	96.2	63696	PASS
177	176	5	9	6.8	4334	PASS

m/z	Abundance
36.00	398.0
37.00	2174.0
38.00	2029.0
39.00	856.0
39.90	175.0
44.00	615.0
44.90	395.0
45.90	125.0
47.00	807.0
47.90	343.0
49.00	2256.0
50.00	10320.0
51.00	2912.0
52.10	114.0
54.80	171.0
56.00	706.0
57.10	1600.0
60.00	588.0
61.00	2716.0
62.00	3040.0
63.10	2623.0
64.10	308.0
65.00	569.0
66.90	173.0
68.00	6550.0
69.00	6216.0
70.00	440.0
72.00	431.0
73.00	2888.0
74.00	10873.0
75.00	32264.0
76.10	3033.0
78.00	397.0
78.90	2124.0
79.90	740.0
81.00	2052.0
81.90	559.0
86.90	2366.0
88.00	2983.0
91.00	308.0
92.00	2010.0
93.00	3101.0
94.00	7558.0
95.00	67080.0
96.00	4232.0
96.90	120.0
103.90	309.0
105.90	352.0
116.00	226.0
116.90	476.0
117.90	273.0
118.80	315.0
127.80	272.0
129.00	145.0
129.80	271.0
134.80	123.0
136.80	112.0
140.90	841.0
142.90	925.0
144.80	281.0
145.60	136.0
147.90	230.0
155.00	222.0
172.00	892.0
173.90	62144.0
175.00	4485.0
175.90	60568.0
177.00	4159.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	373.0
37.00	2293.0
38.00	1995.0
39.00	837.0
39.90	177.0
44.00	596.0
44.90	419.0
47.00	766.0
48.00	347.0
49.00	2268.0
50.00	11080.0
51.00	3320.0
52.00	138.0
54.90	160.0
56.00	750.0
57.10	1535.0
60.00	688.0
61.00	2946.0
62.00	3112.0
63.10	2787.0
64.10	391.0
65.00	686.0
66.90	191.0
68.00	6885.0
69.00	6700.0
70.00	443.0
72.00	439.0
73.00	3084.0
74.00	11291.0
75.00	34160.0
76.10	3140.0
76.80	512.0
78.00	378.0
78.90	2236.0
79.90	846.0
81.00	2214.0
81.90	634.0
86.90	2571.0
88.00	3052.0
91.00	292.0
92.00	1945.0
93.00	3282.0
94.00	7841.0
95.00	70848.0
96.00	4534.0
96.90	117.0
103.90	324.0
105.00	113.0
106.00	355.0
113.00	103.0
116.00	218.0
116.80	502.0
117.70	256.0
118.90	326.0
127.80	303.0
129.00	148.0
129.80	261.0
130.80	101.0
134.90	147.0
136.90	126.0
140.90	859.0
141.90	104.0
142.90	978.0
144.80	284.0
145.70	150.0
147.90	231.0
154.90	195.0
161.00	105.0
171.90	907.0
173.10	659.0
173.90	68520.0
175.00	4996.0
175.90	65968.0
177.00	4517.0
178.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.90	314.0
37.00	2181.0
38.00	1886.0
38.90	795.0
39.90	206.0
44.00	571.0
45.00	399.0
47.00	644.0
48.00	323.0
49.00	2112.0
50.00	10669.0
51.00	3381.0
52.00	134.0
54.90	160.0
56.00	758.0
57.00	1365.0
60.00	664.0
61.00	3029.0
62.00	2755.0
63.10	2495.0
64.00	448.0
65.00	702.0
66.90	179.0
68.00	6274.0
69.00	6548.0
70.00	419.0
72.00	329.0
73.00	2908.0
74.00	10478.0
75.00	32856.0
76.10	2886.0
76.90	480.0
77.90	339.0
78.90	2081.0
79.90	855.0
81.00	2123.0
81.90	601.0
86.90	2621.0
88.00	2803.0
91.00	300.0
92.00	1830.0
93.00	3204.0
94.00	7530.0
95.00	67640.0
96.00	4415.0
96.90	108.0
103.90	308.0
105.10	113.0
106.00	322.0
116.00	219.0
116.80	549.0
117.70	211.0
118.00	214.0
118.90	333.0
127.90	282.0
128.90	131.0
129.90	264.0
130.90	109.0
134.90	149.0
137.00	123.0
140.80	775.0
142.80	947.0
144.80	253.0
145.70	131.0
147.90	209.0
154.80	161.0
170.70	106.0
171.90	866.0
173.10	680.0
173.90	68072.0
175.00	4978.0
175.90	64552.0
177.00	4325.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
39.80	183.0
43.80	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35