

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030151.D
 Acq On : 10 Mar 2023 13:39
 Operator : SY/MD
 Sample : 01868-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Quant Time: Mar 11 00:04:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 11 00:01:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	148756	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	149243	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	74213	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	32300	3.356	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.539	69	38321	4.241	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.800%	
11) 1,1-Dichloroethene-d2	2.066	63	54727	2.766	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.400%#	
20) 2-Butanone-d5	3.828	46	96788	54.540	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.080%	
24) Chloroform-d	4.259	84	98736	5.022	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.400%	
26) 1,2-Dichloroethane-d4	4.953	65	42841	5.337	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.800%	
32) Benzene-d6	4.969	84	162313	4.042	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.800%	
36) 1,2-Dichloropropane-d6	5.998	67	57814	4.785	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.800%	
41) Toluene-d8	7.252	98	131389	3.452	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.000%#	
43) trans-1,3-Dichloroprop...	7.561	79	17071	4.130	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.600%	
46) 2-Hexanone-d5	8.037	63	84857	49.624	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.240%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	46850	5.451	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.000%	
66) 1,2-Dichlorobenzene-d4	11.570	152	62899	5.009	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.200%	
Target Compounds						Qvalue
13) Acetone	2.159	43	2397	1.827	ug/L	99
16) Methylene chloride	2.455	84	6375	0.523	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030151.D
Acq On : 10 Mar 2023 13:39
Operator : SY/MD
Sample : 01868-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBD7

Quant Time: Mar 11 00:04:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 11 00:01:55 2023
Response via : Initial Calibration

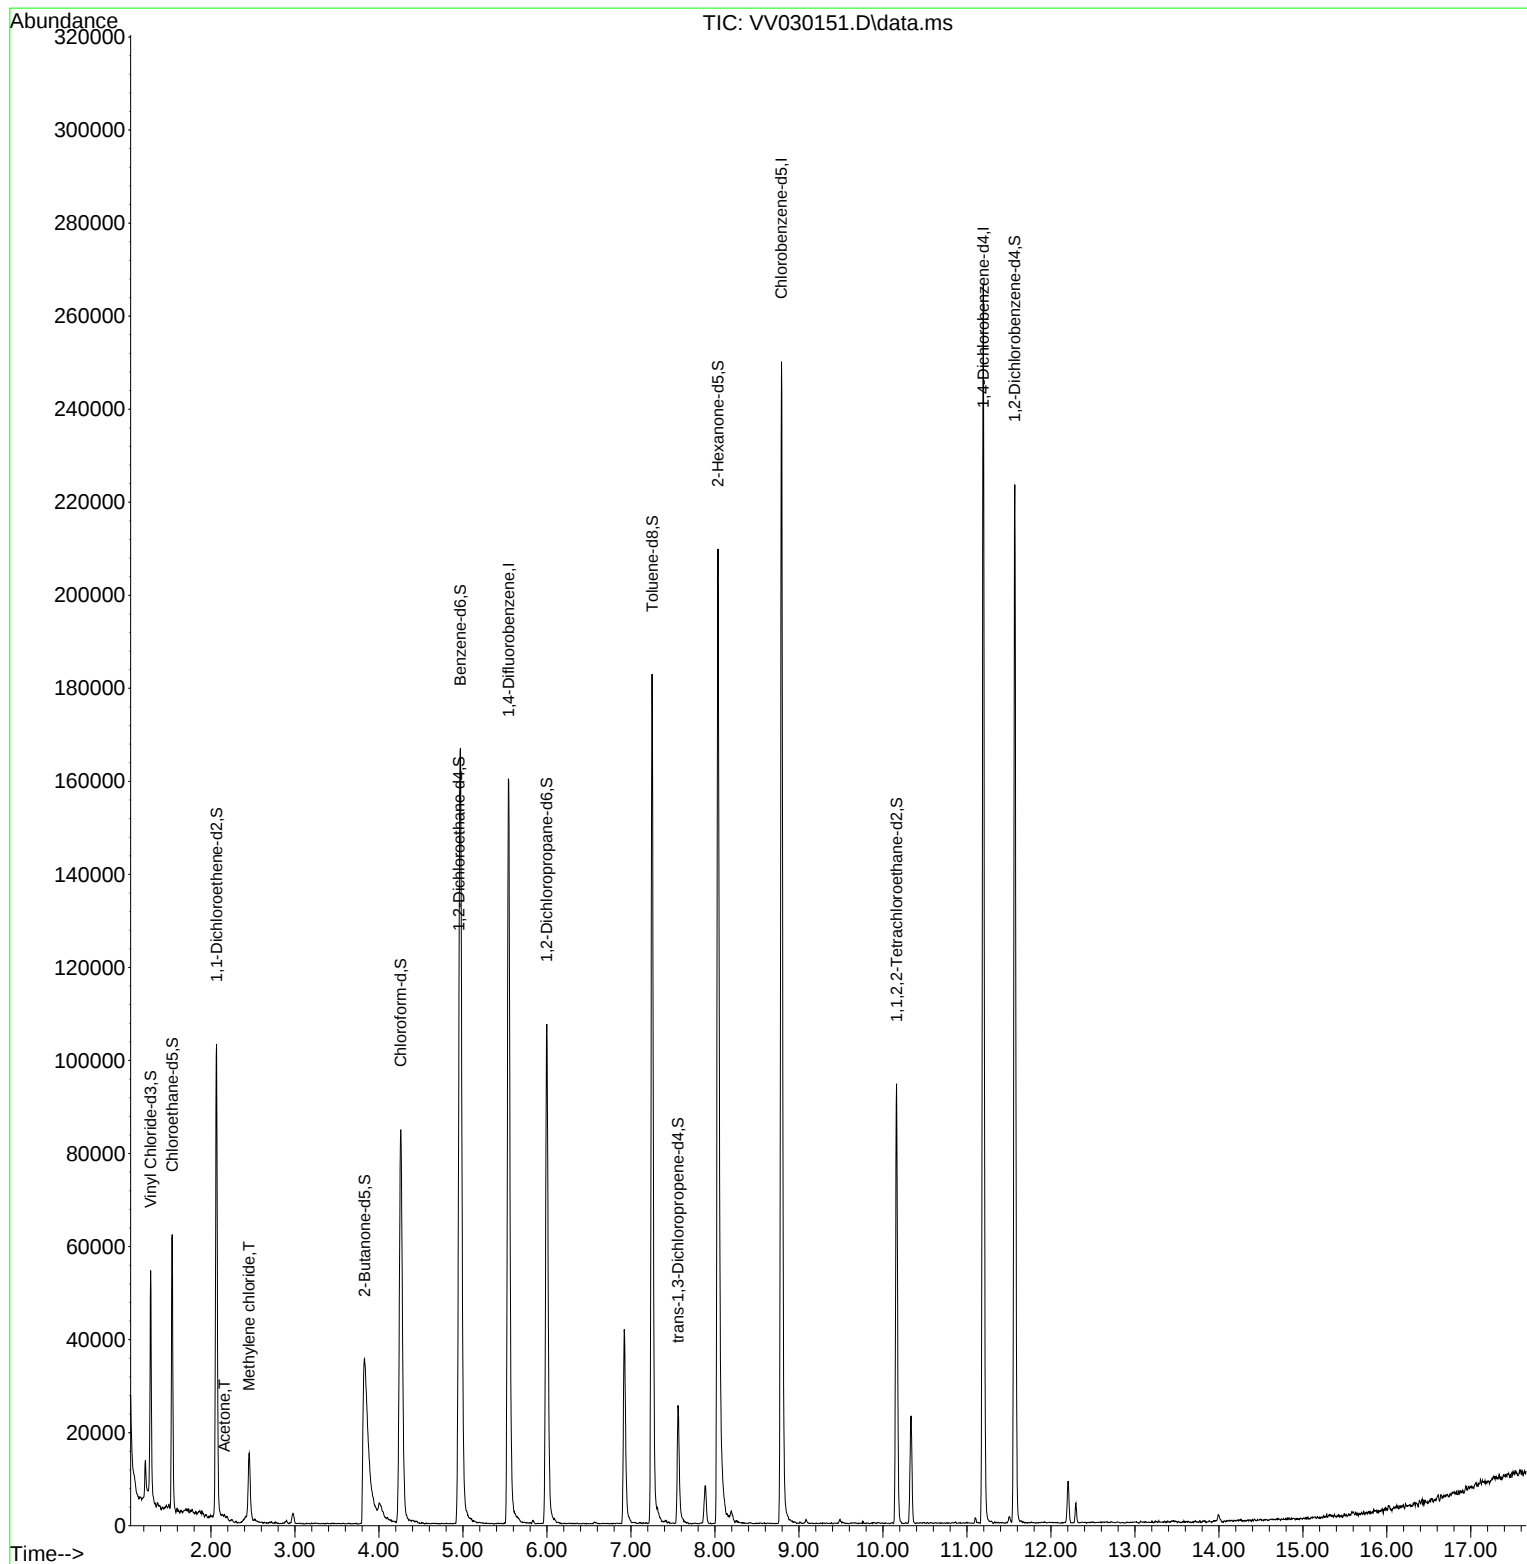

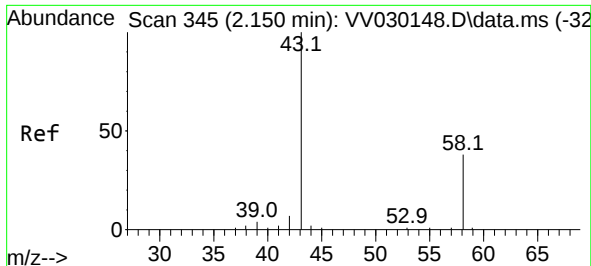

#13

Acetone

Concen: 1.827 ug/L

RT: 2.159 min Scan# 345

Delta R.T. 0.010 min

Lab File: VV030151.D

Acq: 10 Mar 2023 13:39

Instrument :

MSVOA_V

ClientSampleId :





C0BD7

Tgt Ion: 43 Resp: 2397

Ion Ratio Lower Upper

43 100

58 15.2 0.0 29.4

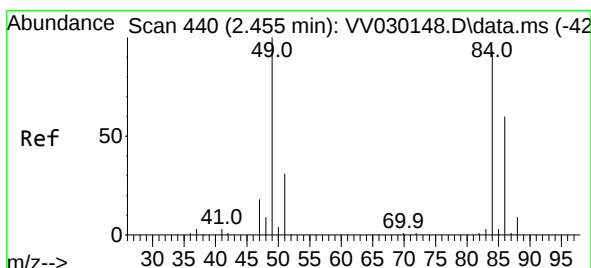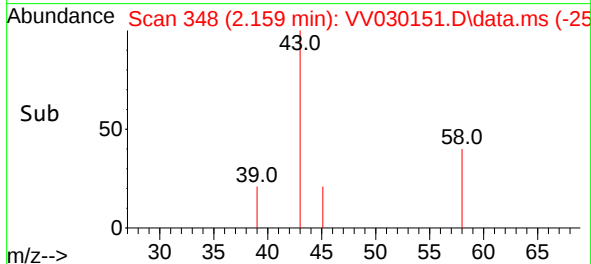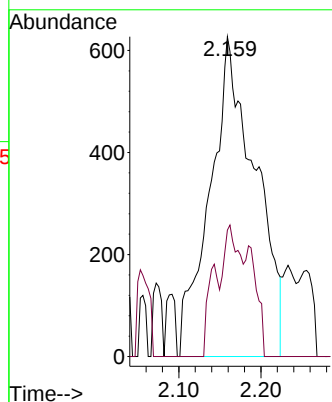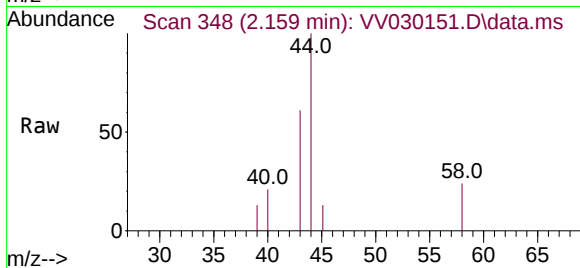

#16

Methylene chloride

Concen: 0.523 ug/L

RT: 2.455 min Scan# 440

Delta R.T. -0.000 min

Lab File: VV030151.D

Acq: 10 Mar 2023 13:39

Tgt Ion: 84 Resp: 6375

Ion Ratio Lower Upper

84 100

86 61.5 44.7 83.1

49 110.0 78.8 146.3

