

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030152.D
 Acq On : 10 Mar 2023 14:03
 Operator : SY/MD
 Sample : 01868-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD8

Quant Time: Mar 11 00:04:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 11 00:01:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	150122	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	149328	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	73365	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	29913	3.079	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.600%	
7) Chloroethane-d5	1.535	69	36925	4.050	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.000%	
11) 1,1-Dichloroethene-d2	2.066	63	53580	2.683	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	53.600%#	
20) 2-Butanone-d5	3.838	46	99362	55.481	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	110.960%	
24) Chloroform-d	4.262	84	96720	4.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	4.953	65	41739	5.153	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.000%	
32) Benzene-d6	4.973	84	157503	3.920	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.400%	
36) 1,2-Dichloropropane-d6	5.998	67	55330	4.577	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.600%	
41) Toluene-d8	7.252	98	126683	3.326	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	66.600%#	
43) trans-1,3-Dichloroprop...	7.561	79	16919	4.091	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.800%	
46) 2-Hexanone-d5	8.037	63	86760	50.708	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.420%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	47053	5.471	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152	60237	4.853	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.000%	
Target Compounds						Qvalue
16) Methylene chloride	2.455	84	4312	0.350	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030152.D
Acq On : 10 Mar 2023 14:03
Operator : SY/MD
Sample : 01868-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Time: Mar 11 00:04:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 11 00:01:55 2023
Response via : Initial Calibration

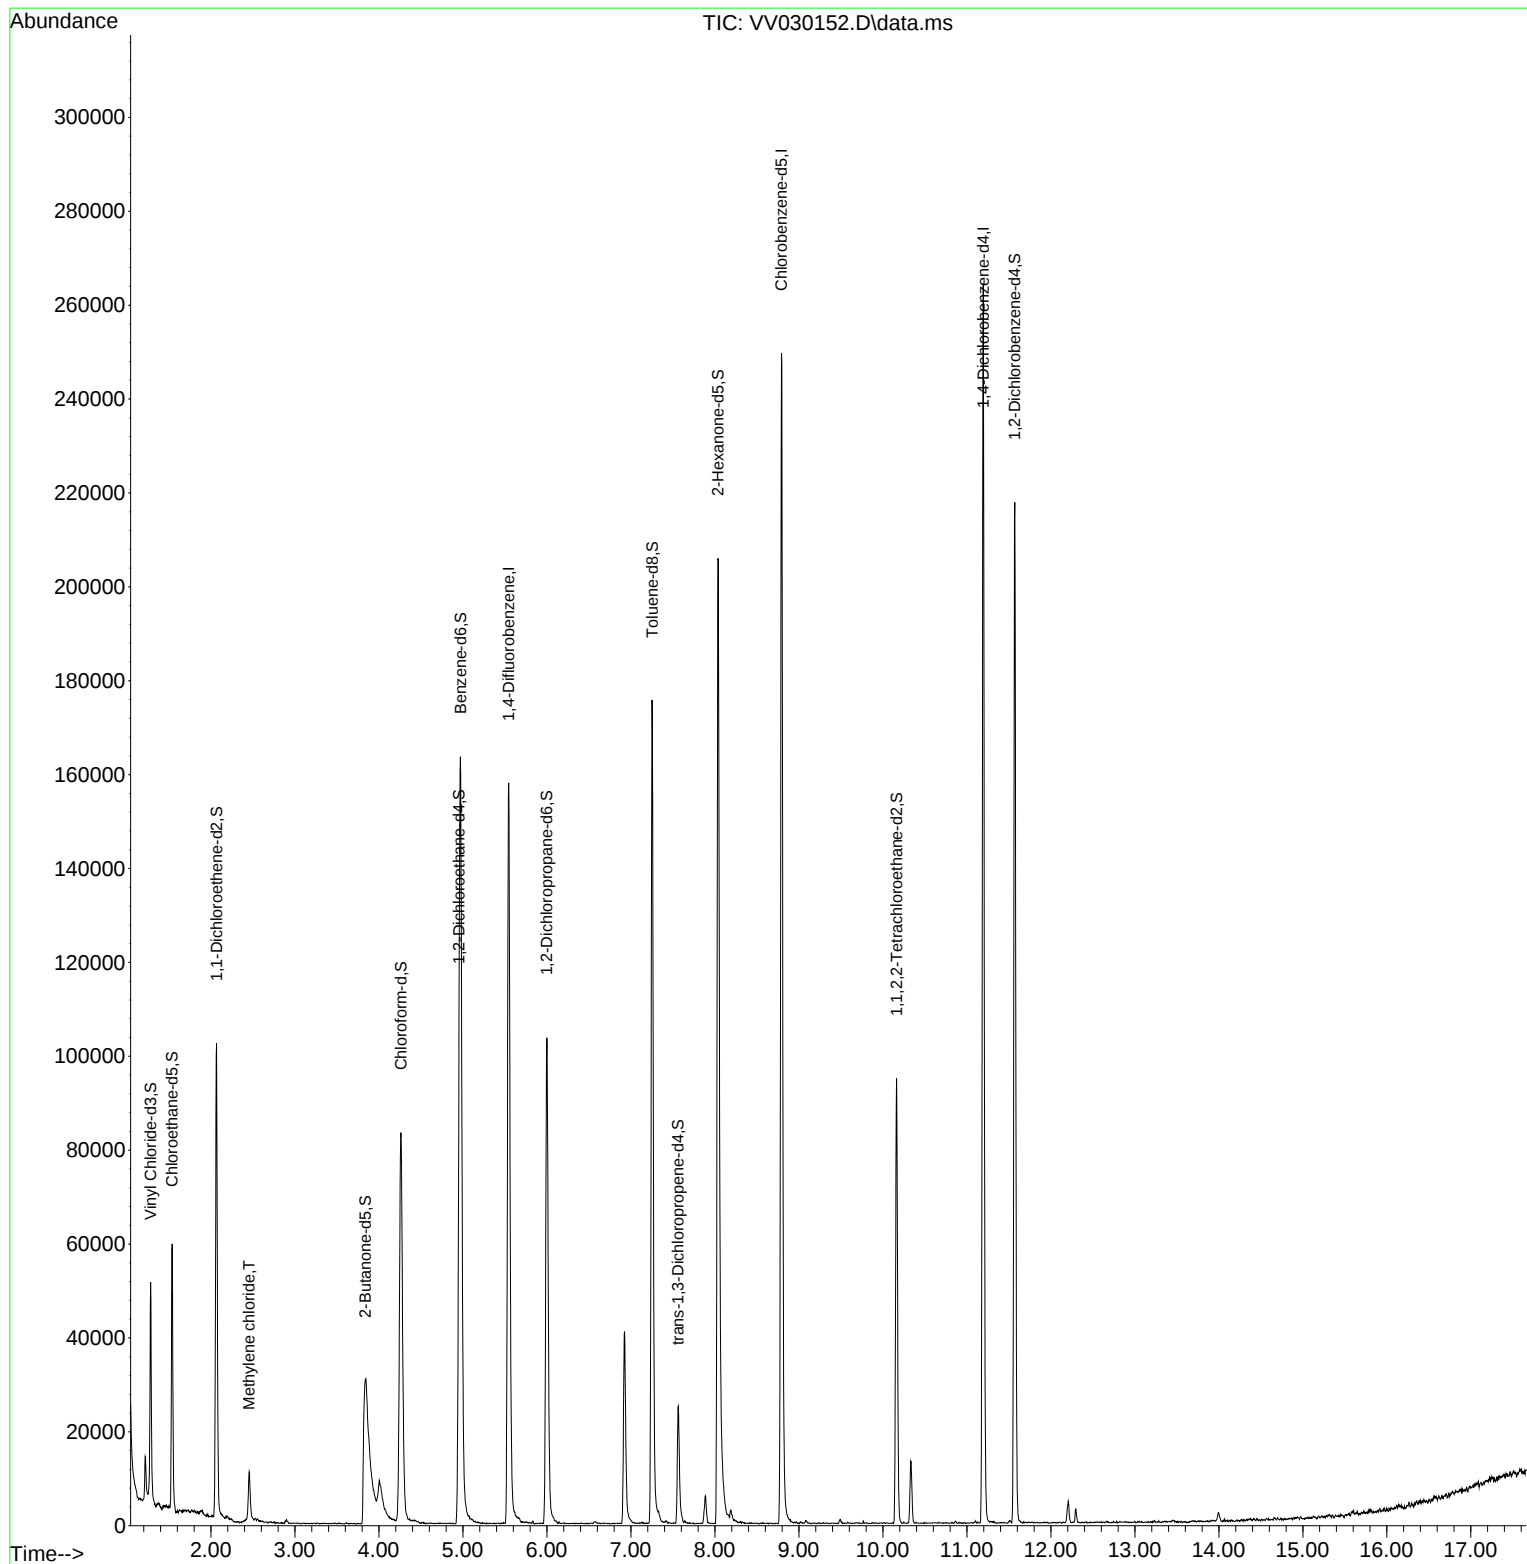

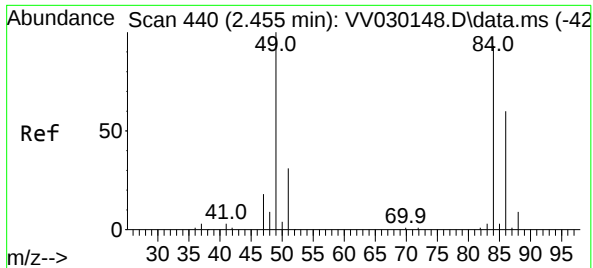

#16
Methylene chloride
Concen: 0.350 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.000 min
Lab File: VV030152.D
Acq: 10 Mar 2023 14:03

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Tgt Ion:	84	Resp:	4312
Ion	Ratio	Lower	Upper
84	100		
86	60.6	44.7	83.1
49	107.6	78.8	146.3

