

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030150.D
 Acq On : 10 Mar 2023 13:12
 Operator : SY/MD
 Sample : 01838-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1173

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	64	rBV2	7745	9834	2.13%	0.240%
2	1.282	69	75	90	rVB	52580	59444	12.86%	1.451%
3	1.536	147	154	171	rVB	61766	75042	16.24%	1.832%
4	2.066	309	319	333	rBV	108397	157102	33.99%	3.834%
5	2.140	333	342	359	rVB5	2637	6715	1.45%	0.164%
6	2.455	431	440	454	rVB2	6733	11698	2.53%	0.286%
7	3.815	851	863	900	rBV	46099	170063	36.80%	4.151%
8	4.256	983	1000	1030	rBV3	92255	240952	52.14%	5.881%
9	4.966	1200	1221	1262	rBV2	175870	462136	100.00%	11.279%
10	5.542	1387	1400	1423	rBV	147594	307549	66.55%	7.506%
11	5.995	1525	1541	1561	rBV	113959	234805	50.81%	5.731%
12	6.921	1818	1829	1856	rBV2	44482	82751	17.91%	2.020%
13	7.249	1915	1931	1954	rBV	190120	345270	74.71%	8.427%
14	7.561	2018	2028	2054	rBV	27478	49499	10.71%	1.208%
15	7.883	2113	2128	2142	rBV3	9935	19006	4.11%	0.464%
16	8.034	2163	2175	2206	rBV	223810	423721	91.69%	10.342%
17	8.191	2215	2224	2237	rVB7	4133	9082	1.97%	0.222%
18	8.793	2397	2411	2433	rBV	230608	386950	83.73%	9.444%
19	10.162	2826	2837	2856	rVB	98528	154997	33.54%	3.783%
20	10.333	2879	2890	2903	rBV	30612	49749	10.77%	1.214%
21	11.098	3122	3128	3136	rBV5	3691	5074	1.10%	0.124%
22	11.194	3147	3158	3184	rBV	248604	389041	84.18%	9.495%
23	11.497	3242	3252	3264	rBV2	11964	22921	4.96%	0.559%
24	11.571	3264	3275	3294	rVB	240020	378025	81.80%	9.227%
25	12.204	3461	3472	3482	rBV2	9804	14955	3.24%	0.365%
26	12.297	3491	3501	3511	rBV3	21130	30777	6.66%	0.751%




Sum of corrected areas: 4097158

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030150.D
Acq On : 10 Mar 2023 13:12
Operator : SY/MD
Sample : 01838-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

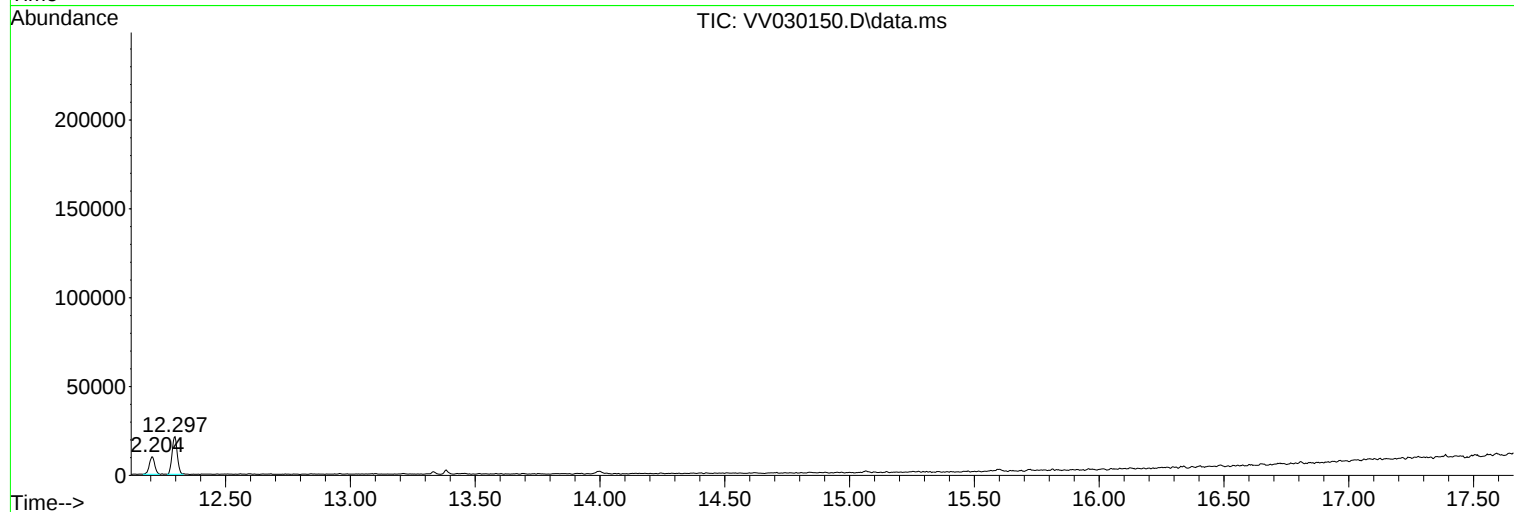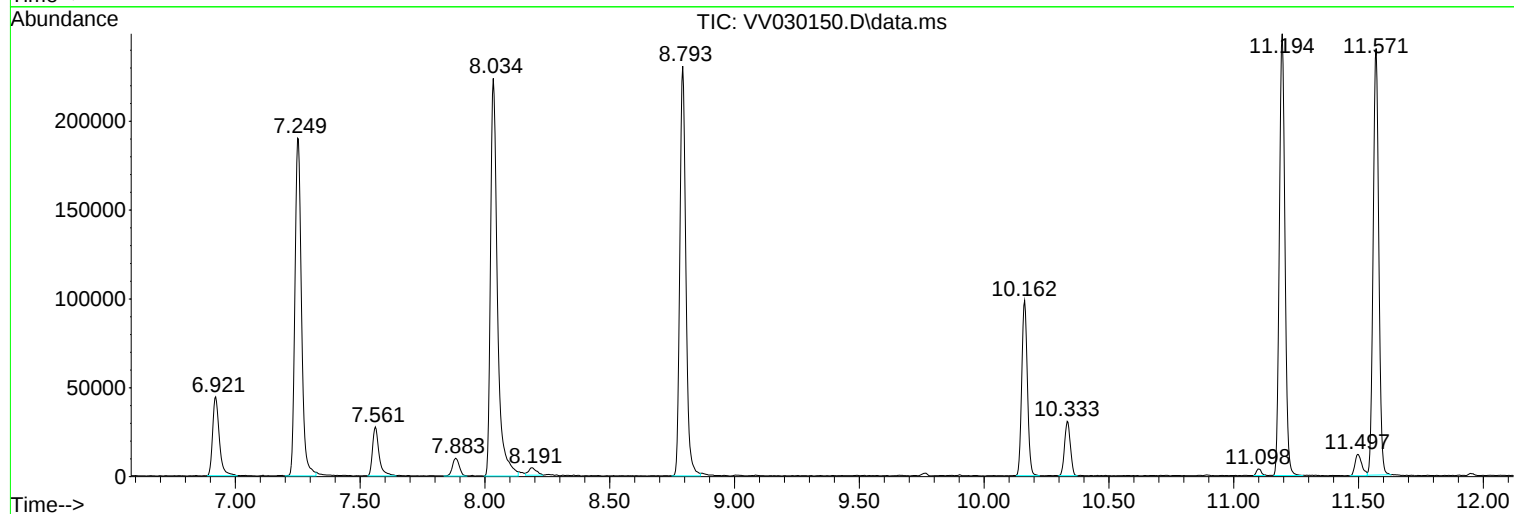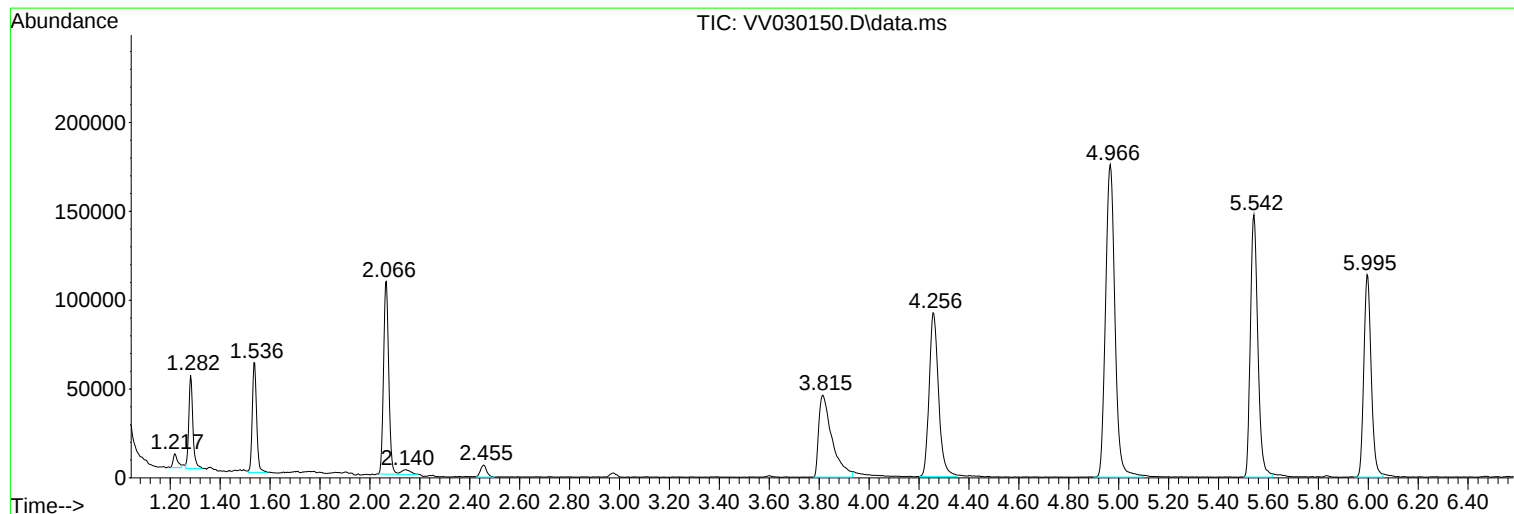

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030150.D
Acq On : 10 Mar 2023 13:12
Operator : SY/MD
Sample : 01838-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030150.D
Acq On : 10 Mar 2023 13:12
Operator : SY/MD
Sample : 01838-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------