

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030151.D
 Acq On : 10 Mar 2023 13:39
 Operator : SY/MD
 Sample : 01868-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	64	rBV	7506	9326	2.15%	0.236%
2	1.281	67	75	91	rVB	50206	60351	13.94%	1.526%
3	1.539	147	155	169	rVB	59750	70990	16.40%	1.795%
4	2.066	306	319	335	rBV	101656	150196	34.69%	3.798%
5	2.455	429	440	454	rVB	14480	26105	6.03%	0.660%
6	3.828	855	867	905	rBV2	35462	157193	36.31%	3.975%
7	4.259	984	1001	1031	rBV2	84501	220555	50.95%	5.577%
8	4.969	1205	1222	1257	rBV2	166647	432917	100.00%	10.947%
9	5.542	1387	1400	1430	rBV	159913	337587	77.98%	8.537%
10	5.998	1528	1542	1569	rBV	107304	226238	52.26%	5.721%
11	6.921	1819	1829	1856	rBV	41738	78459	18.12%	1.984%
12	7.252	1915	1932	1950	rBV	182585	323696	74.77%	8.185%
13	7.561	2014	2028	2053	rBV2	25412	46318	10.70%	1.171%
14	7.886	2118	2129	2145	rVB	8160	15163	3.50%	0.383%
15	8.037	2162	2176	2207	rBV	209533	411853	95.13%	10.415%
16	8.194	2219	2225	2239	rVB5	2508	5037	1.16%	0.127%
17	8.792	2397	2411	2440	rBV	249762	415607	96.00%	10.510%
18	10.162	2825	2837	2857	rBV	94541	149259	34.48%	3.774%
19	10.336	2880	2891	2904	rBV	23120	37217	8.60%	0.941%
20	11.194	3147	3158	3184	rBV	266513	412001	95.17%	10.418%
21	11.570	3263	3275	3294	rBV	223049	349776	80.80%	8.845%
22	12.204	3462	3472	3483	rVB	8984	13555	3.13%	0.343%
23	12.297	3494	3501	3512	rVB4	4268	5182	1.20%	0.131%




Sum of corrected areas: 3954581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030151.D
Acq On : 10 Mar 2023 13:39
Operator : SY/MD
Sample : 01868-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

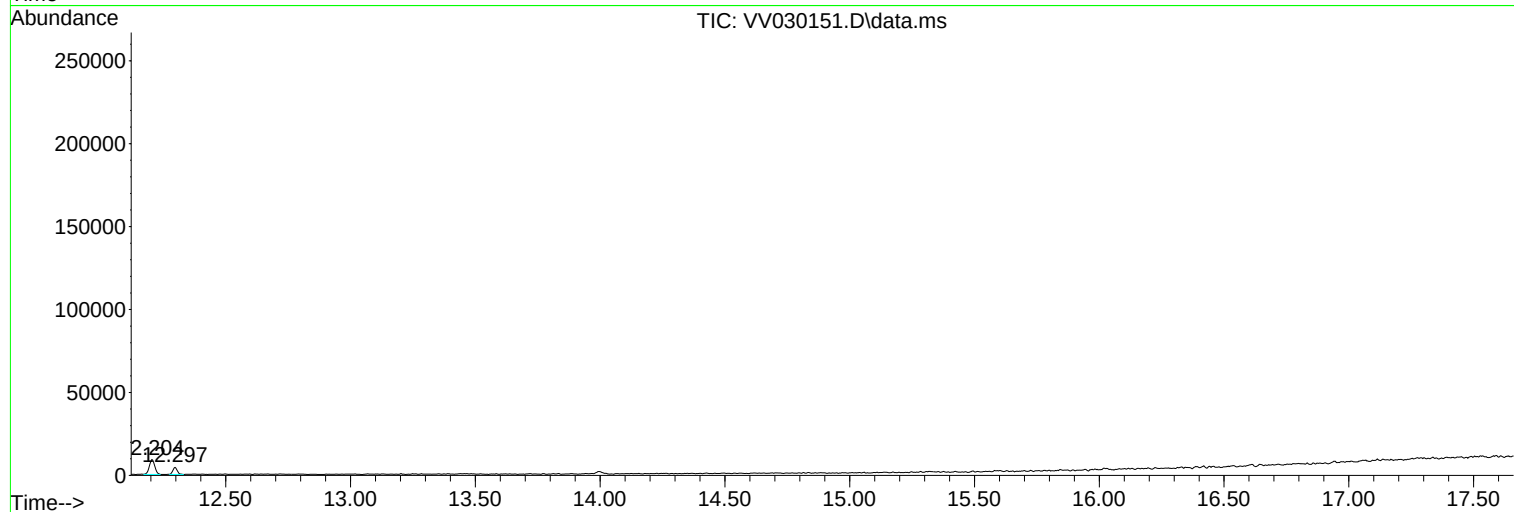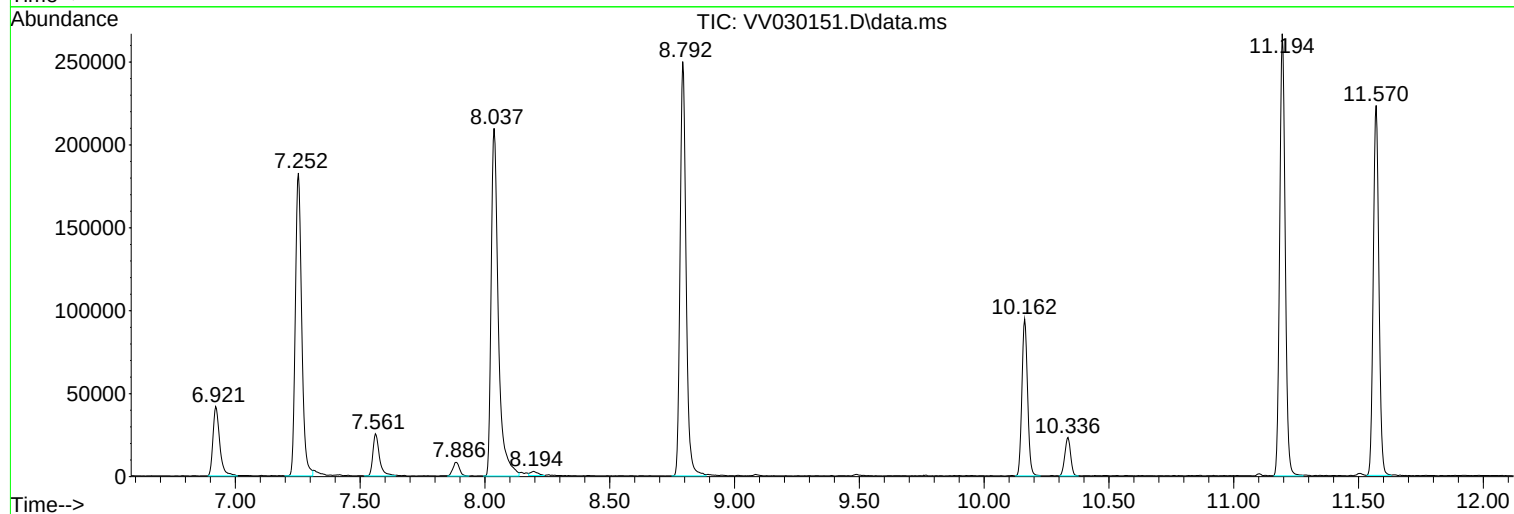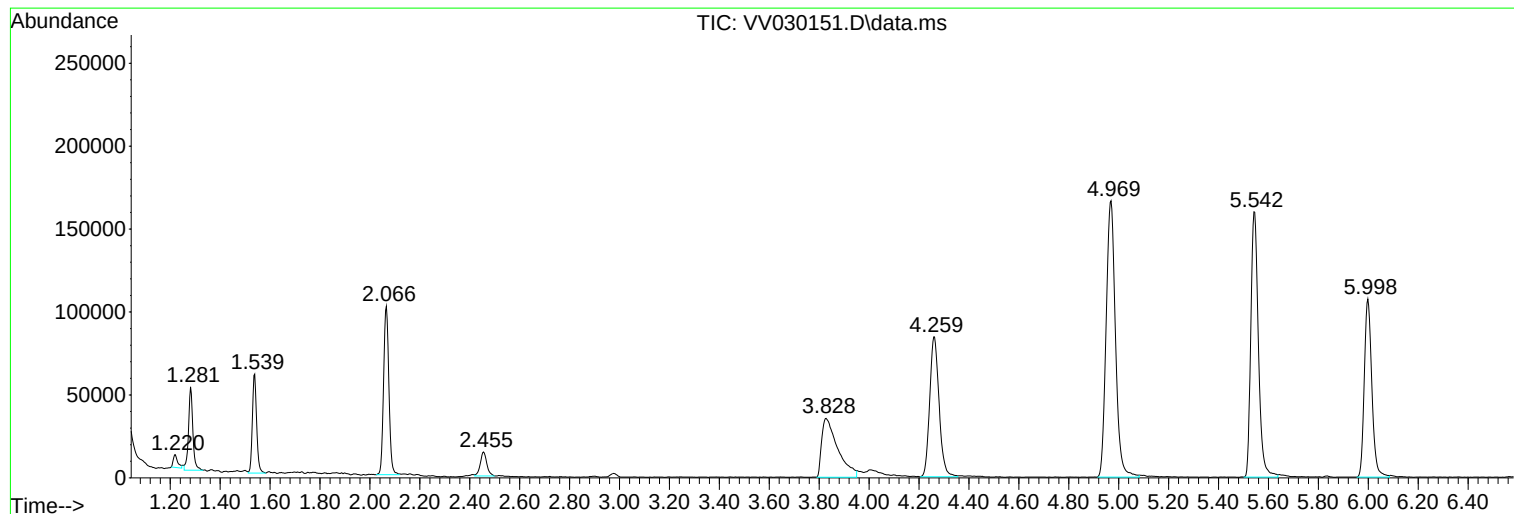

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030151.D
Acq On : 10 Mar 2023 13:39
Operator : SY/MD
Sample : 01868-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030151.D
Acq On : 10 Mar 2023 13:39
Operator : SY/MD
Sample : 01868-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc