

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030152.D
 Acq On : 10 Mar 2023 14:03
 Operator : SY/MD
 Sample : 01868-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	66	rBV2	8880	11768	2.81%	0.306%
2	1.281	67	75	95	rVB	47829	59287	14.14%	1.543%
3	1.539	147	155	169	rVB	57301	69017	16.46%	1.796%
4	2.066	308	319	334	rBV	100800	147137	35.08%	3.829%
5	2.455	428	440	458	rVB2	10306	17167	4.09%	0.447%
6	3.844	857	872	911	rBV2	30868	156051	37.21%	4.061%
7	4.262	983	1002	1031	rBV	82718	213248	50.84%	5.549%
8	4.969	1205	1222	1251	rBV2	163380	419411	100.00%	10.915%
9	5.545	1388	1401	1426	rBV	157704	328813	78.40%	8.557%
10	5.998	1527	1542	1572	rBV	103540	217685	51.90%	5.665%
11	6.924	1818	1830	1855	rBV	40917	77567	18.49%	2.019%
12	7.252	1920	1932	1954	rBV	175389	312296	74.46%	8.127%
13	7.564	2019	2029	2049	rBV2	24915	45331	10.81%	1.180%
14	7.886	2118	2129	2139	rBV2	5906	10069	2.40%	0.262%
15	8.037	2165	2176	2209	rBV	205664	419230	99.96%	10.910%
16	8.792	2398	2411	2440	rBV	249416	417481	99.54%	10.864%
17	10.162	2826	2837	2856	rBV	94794	150309	35.84%	3.912%
18	10.333	2880	2890	2904	rVB2	13274	21262	5.07%	0.553%
19	11.194	3146	3158	3181	rBV	264043	404906	96.54%	10.537%
20	11.570	3264	3275	3293	rBV	217328	337260	80.41%	8.777%
21	12.207	3462	3473	3486	rVB3	4584	7379	1.76%	0.192%




Sum of corrected areas: 3842674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030152.D
Acq On : 10 Mar 2023 14:03
Operator : SY/MD
Sample : 01868-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

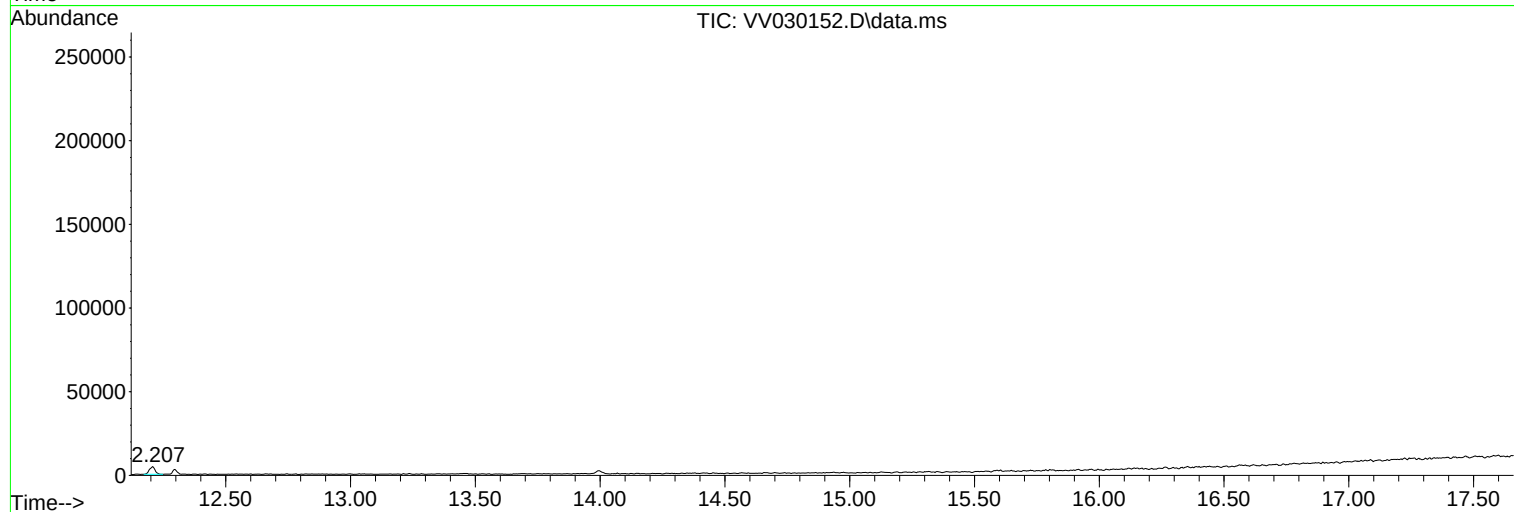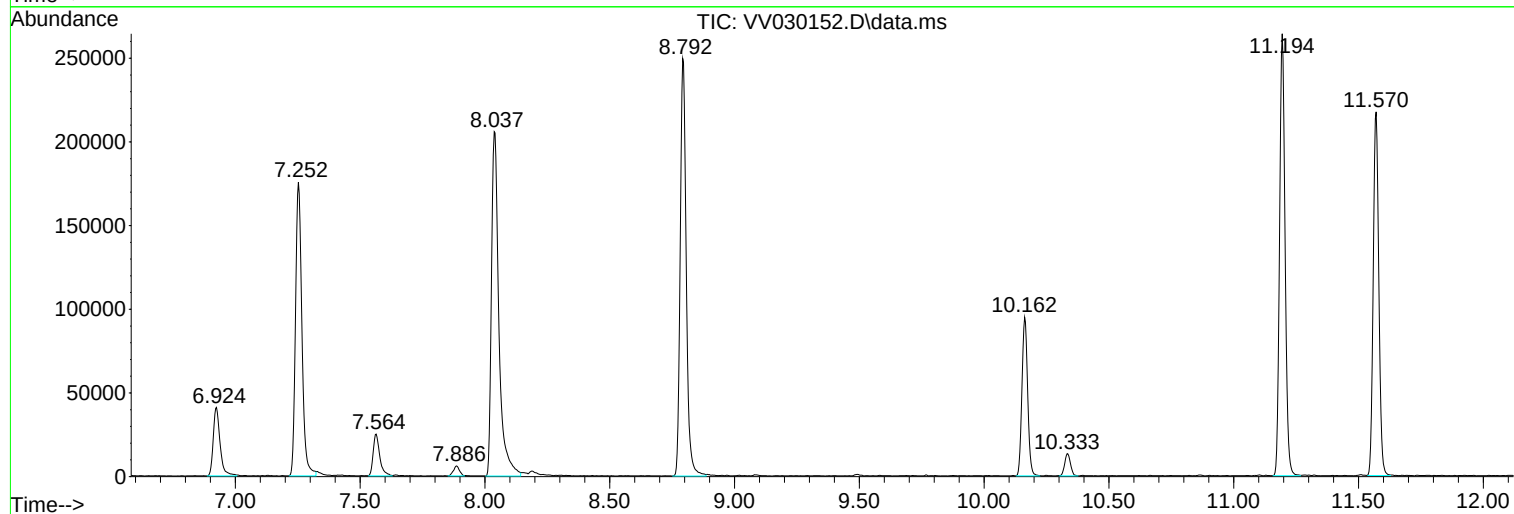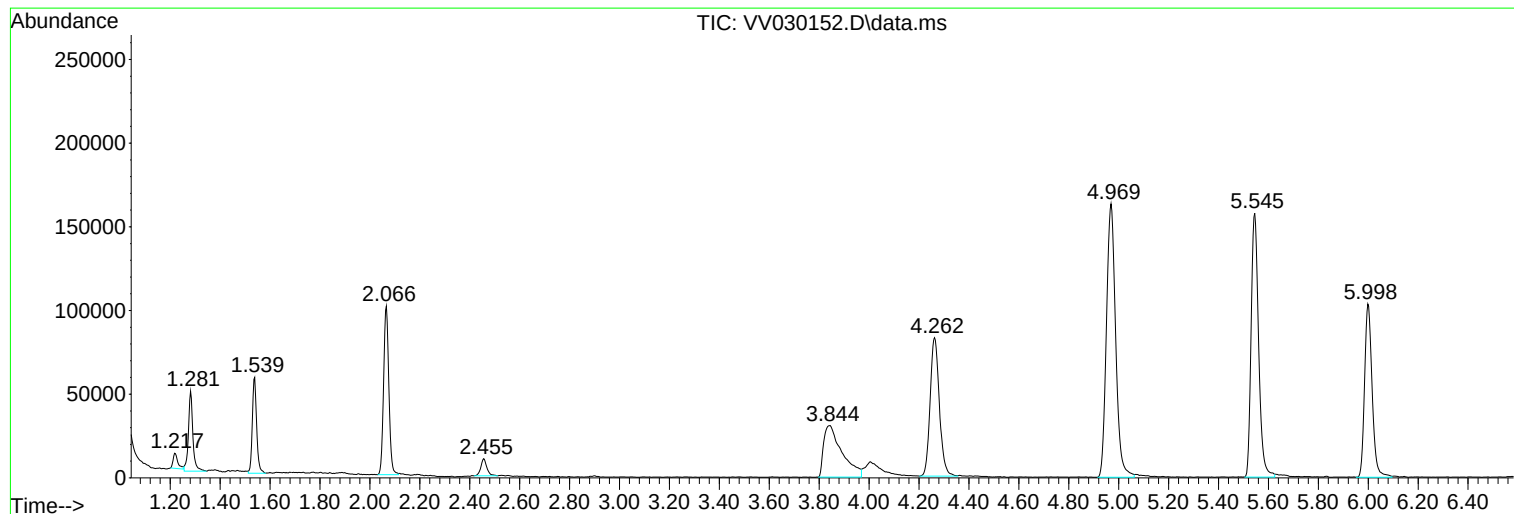

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030152.D
Acq On : 10 Mar 2023 14:03
Operator : SY/MD
Sample : 01868-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030152.D
Acq On : 10 Mar 2023 14:03
Operator : SY/MD
Sample : 01868-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc