

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030154.D
 Acq On : 10 Mar 2023 14:49
 Operator : SY/MD
 Sample : 01868-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.101	14	19	38	rVB	22913	31397	7.57%	0.824%
2	1.217	50	55	65	rBV	11699	15206	3.67%	0.399%
3	1.282	69	75	95	rVB	47137	56257	13.56%	1.476%
4	1.539	147	155	168	rVB	54760	65542	15.80%	1.720%
5	2.066	309	319	333	rVB	96673	139196	33.56%	3.653%
6	3.825	854	866	908	rBV	38044	160831	38.77%	4.221%
7	4.005	912	922	956	rVB4	7728	29028	7.00%	0.762%
8	4.262	984	1002	1028	rBV	80389	205595	49.56%	5.396%
9	4.969	1203	1222	1251	rBV2	157676	408724	98.53%	10.727%
10	5.545	1388	1401	1423	rBV	156476	316812	76.37%	8.315%
11	5.998	1526	1542	1568	rBV2	102087	213866	51.56%	5.613%
12	6.921	1816	1829	1848	rBV	39345	73354	17.68%	1.925%
13	7.252	1920	1932	1954	rBV	168178	303851	73.25%	7.975%
14	7.564	2019	2029	2049	rBV	24680	45888	11.06%	1.204%
15	7.886	2118	2129	2141	rBV2	6568	11989	2.89%	0.315%
16	8.037	2165	2176	2213	rBV	213105	414827	100.00%	10.887%
17	8.792	2399	2411	2441	rBV	240068	400187	96.47%	10.503%
18	10.162	2825	2837	2857	rVB	91415	145020	34.96%	3.806%
19	10.333	2879	2890	2904	rBV2	19192	31517	7.60%	0.827%
20	11.194	3143	3158	3181	rBV	253910	390804	94.21%	10.257%
21	11.571	3264	3275	3293	rBV	210335	329669	79.47%	8.652%
22	12.204	3461	3472	3483	rBV	10502	16176	3.90%	0.425%
23	13.995	4021	4029	4039	rVB	2810	4444	1.07%	0.117%




Sum of corrected areas: 3810180

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030154.D
Acq On : 10 Mar 2023 14:49
Operator : SY/MD
Sample : 01868-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

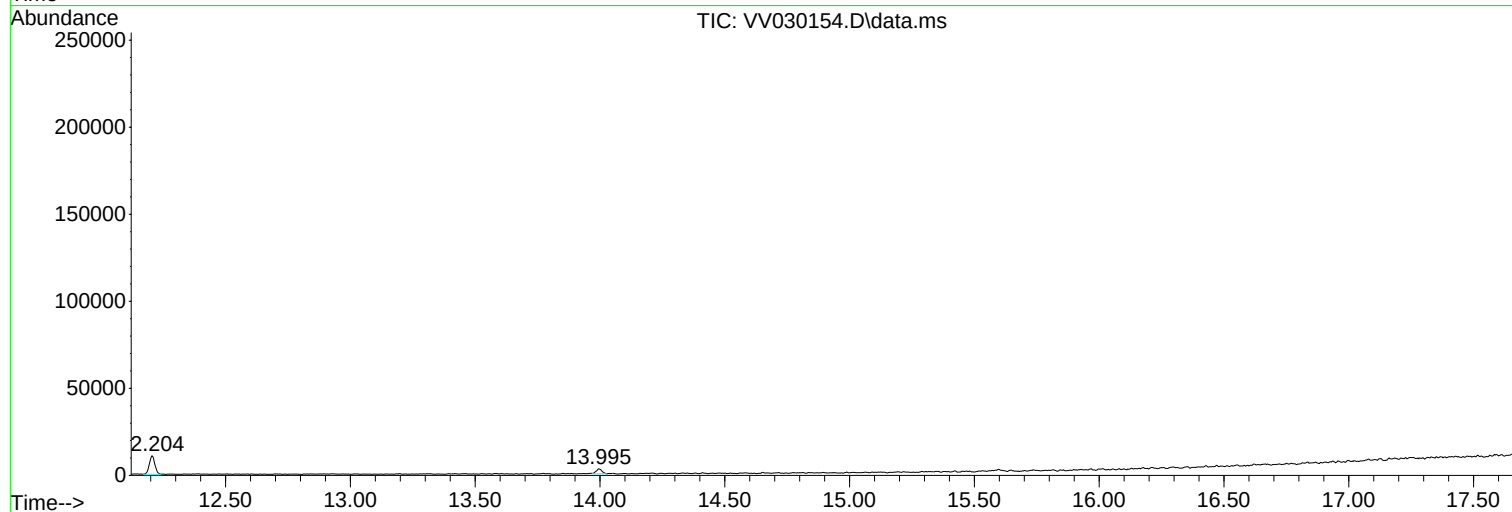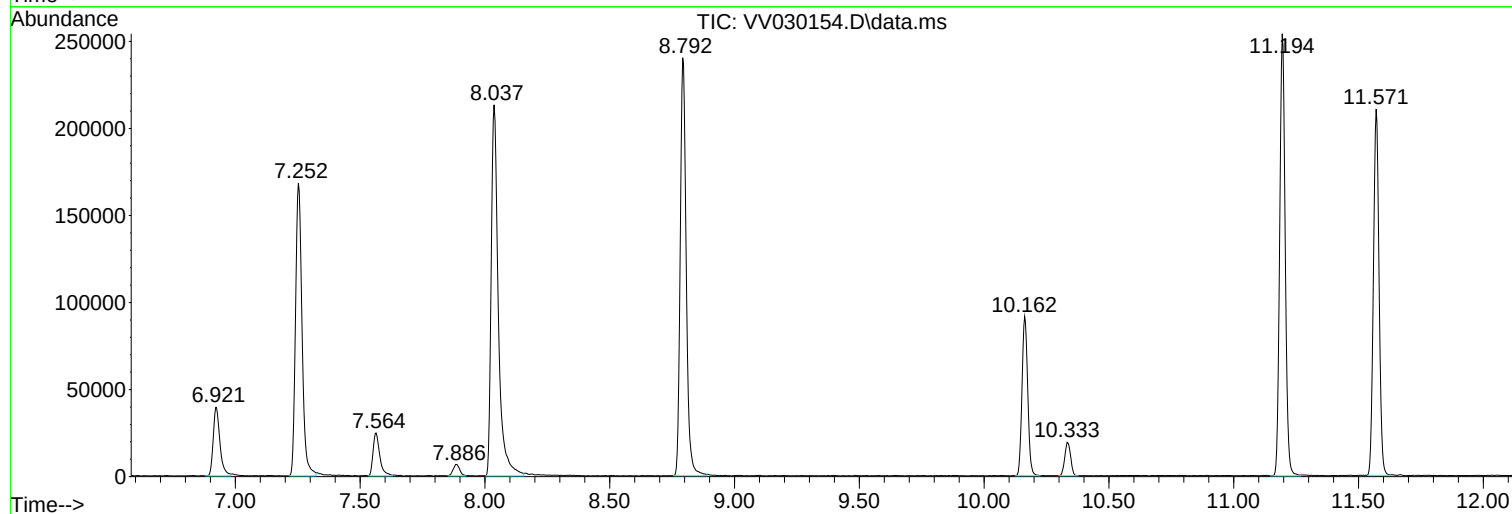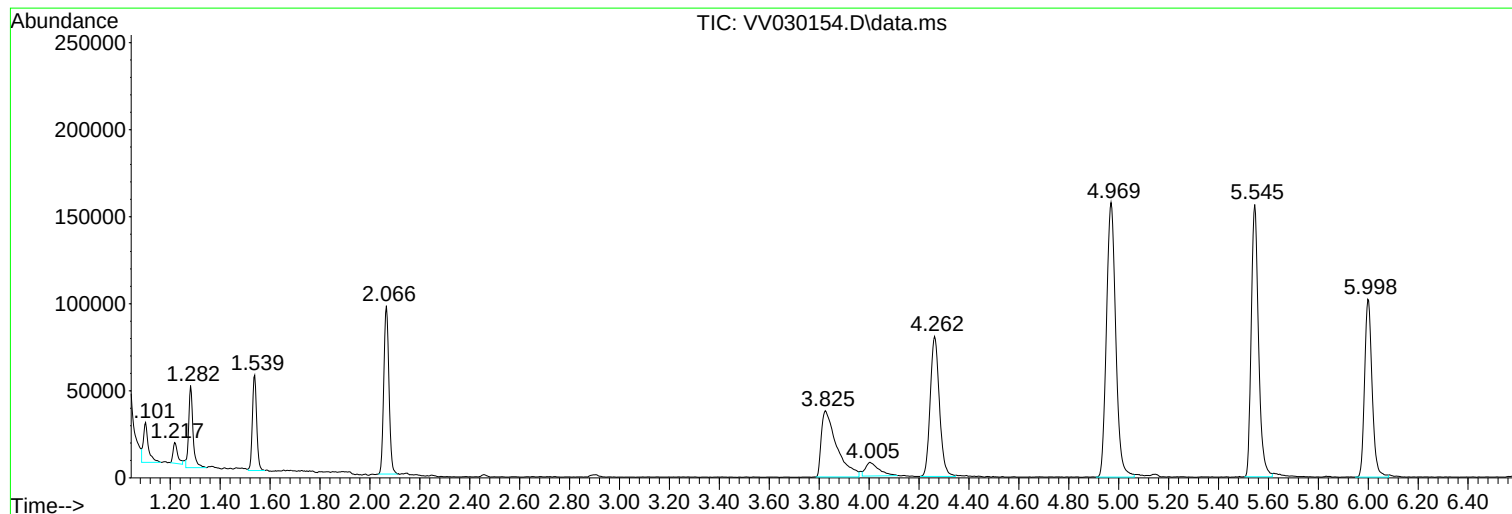

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030154.D
Acq On : 10 Mar 2023 14:49
Operator : SY/MD
Sample : 01868-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030154.D
Acq On : 10 Mar 2023 14:49
Operator : SY/MD
Sample : 01868-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc