

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030157.D
 Acq On : 10 Mar 2023 16:02
 Operator : SY/MD
 Sample : 01838-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	63	rBV2	4227	4983	1.22%	0.133%
2	1.282	69	75	93	rVB	46412	52838	12.94%	1.413%
3	1.539	147	155	168	rVB	56647	66720	16.34%	1.784%
4	2.066	308	319	333	rBV	97743	142816	34.98%	3.819%
5	2.455	430	440	452	rBV2	8016	12777	3.13%	0.342%
6	3.825	855	866	904	rBV	37296	155007	37.97%	4.145%
7	4.262	985	1002	1026	rBV	80062	206097	50.48%	5.511%
8	4.970	1205	1222	1246	rBV2	159029	408265	100.00%	10.916%
9	5.545	1387	1401	1424	rBV	156431	320969	78.62%	8.582%
10	5.998	1525	1542	1568	rBV	101569	214296	52.49%	5.730%
11	6.921	1817	1829	1855	rBV	39111	74514	18.25%	1.992%
12	7.252	1920	1932	1955	rBV	171592	304870	74.67%	8.151%
13	7.564	2020	2029	2046	rBV2	23928	42677	10.45%	1.141%
14	7.886	2118	2129	2139	rBV3	5459	9384	2.30%	0.251%
15	8.037	2165	2176	2206	rBV	211912	407803	99.89%	10.904%
16	8.793	2399	2411	2445	rBV	239590	403593	98.86%	10.791%
17	10.162	2826	2837	2854	rBV	90752	145268	35.58%	3.884%
18	10.336	2880	2891	2907	rVB	14373	22827	5.59%	0.610%
19	11.194	3147	3158	3181	rBV	252099	392456	96.13%	10.493%
20	11.571	3259	3275	3291	rBV	208416	328195	80.39%	8.775%
21	12.204	3461	3472	3483	rBV2	11707	18482	4.53%	0.494%
22	13.998	4020	4030	4041	rVB2	3403	5216	1.28%	0.139%




Sum of corrected areas: 3740053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030157.D
Acq On : 10 Mar 2023 16:02
Operator : SY/MD
Sample : 01838-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

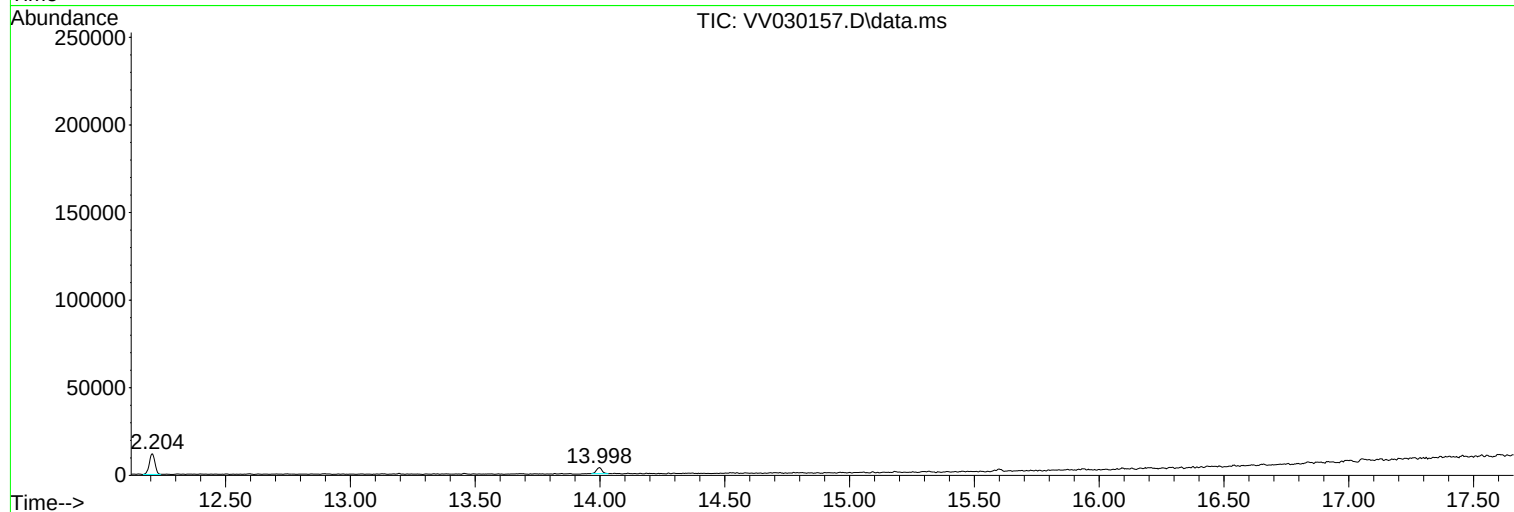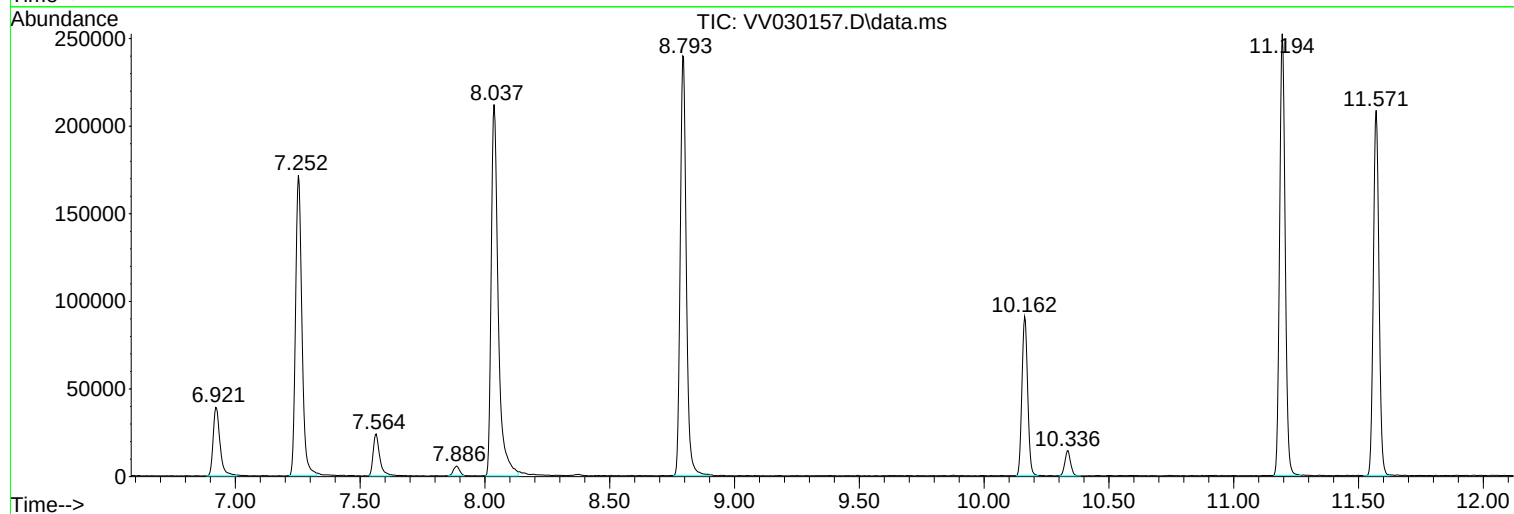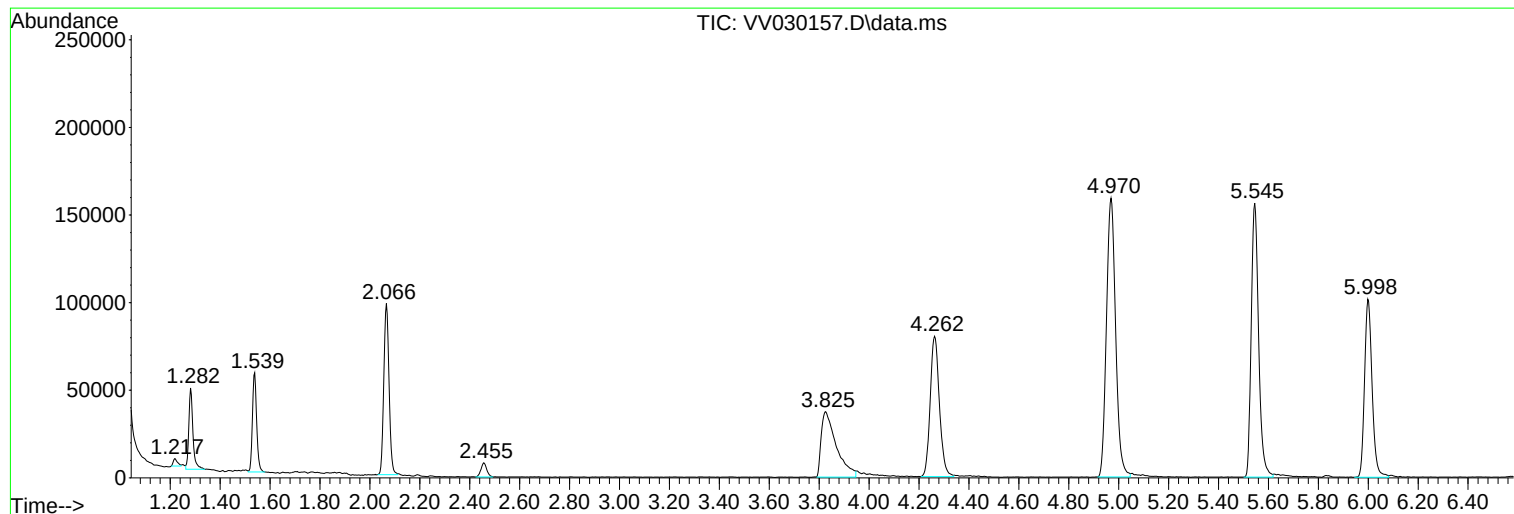

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030157.D
Acq On : 10 Mar 2023 16:02
Operator : SY/MD
Sample : 01838-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030157.D
Acq On : 10 Mar 2023 16:02
Operator : SY/MD
Sample : 01838-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------