

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030158.D
 Acq On : 10 Mar 2023 16:27
 Operator : SY/MD
 Sample : 01868-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	63	rBV	8255	8938	1.73%	0.200%
2	1.281	69	75	95	rVB	54163	65267	12.66%	1.458%
3	1.539	147	155	172	rVB	67308	80757	15.66%	1.804%
4	2.066	308	319	334	rBV	113414	167201	32.43%	3.736%
5	3.822	851	865	908	rBV2	51915	202586	39.29%	4.527%
6	4.262	984	1002	1027	rBV	98770	252170	48.90%	5.635%
7	4.969	1205	1222	1249	rBV2	191008	490054	95.04%	10.950%
8	5.545	1387	1401	1425	rBV	178578	369531	71.66%	8.257%
9	5.998	1529	1542	1560	rBV	122683	256421	49.73%	5.730%
10	6.921	1818	1829	1851	rBV	48060	88770	17.22%	1.984%
11	7.252	1920	1932	1951	rBV	202467	363111	70.42%	8.114%
12	7.564	2019	2029	2050	rBV	29498	54511	10.57%	1.218%
13	7.886	2117	2129	2146	rVB2	4843	9300	1.80%	0.208%
14	8.037	2165	2176	2205	rBV	273354	515653	100.00%	11.522%
15	8.792	2400	2411	2440	rBV	276333	467524	90.67%	10.447%
16	10.162	2826	2837	2855	rBV	113262	178281	34.57%	3.984%
17	10.336	2880	2891	2906	rBV2	14426	23339	4.53%	0.522%
18	11.194	3146	3158	3185	rBV	300686	456644	88.56%	10.204%
19	11.570	3261	3275	3297	rBV	257768	403767	78.30%	9.022%
20	12.204	3462	3472	3483	rBV	9185	14220	2.76%	0.318%
21	13.995	4020	4029	4041	rVB2	4446	7300	1.42%	0.163%




Sum of corrected areas: 4475345

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030158.D
Acq On : 10 Mar 2023 16:27
Operator : SY/MD
Sample : 01868-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

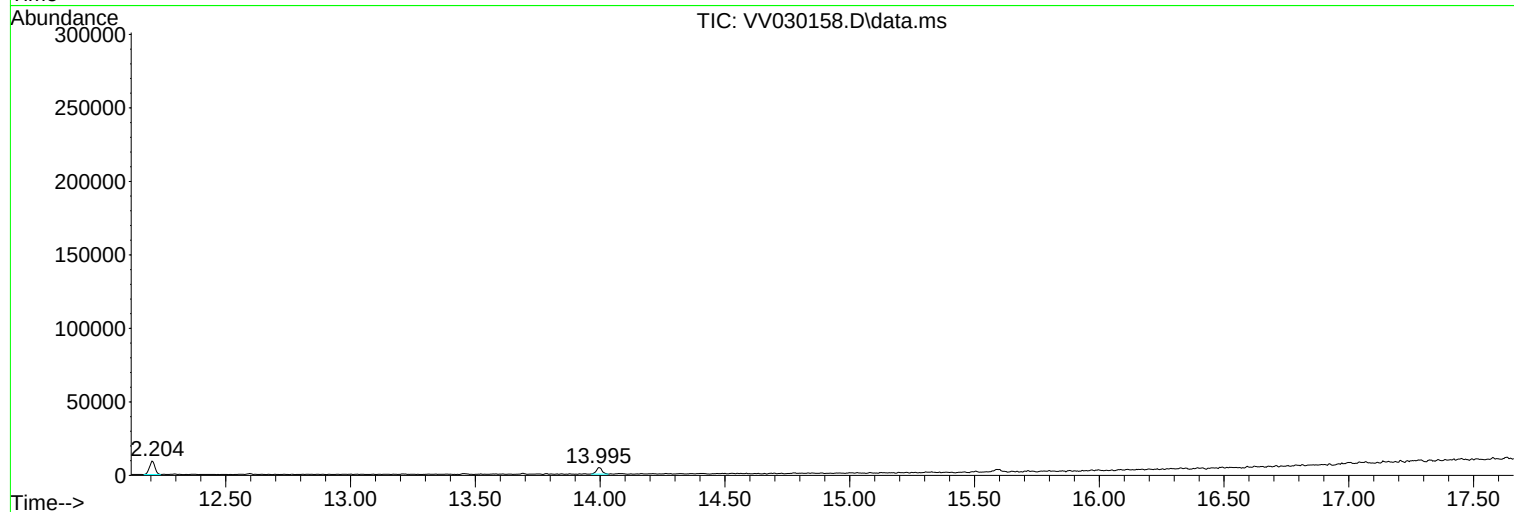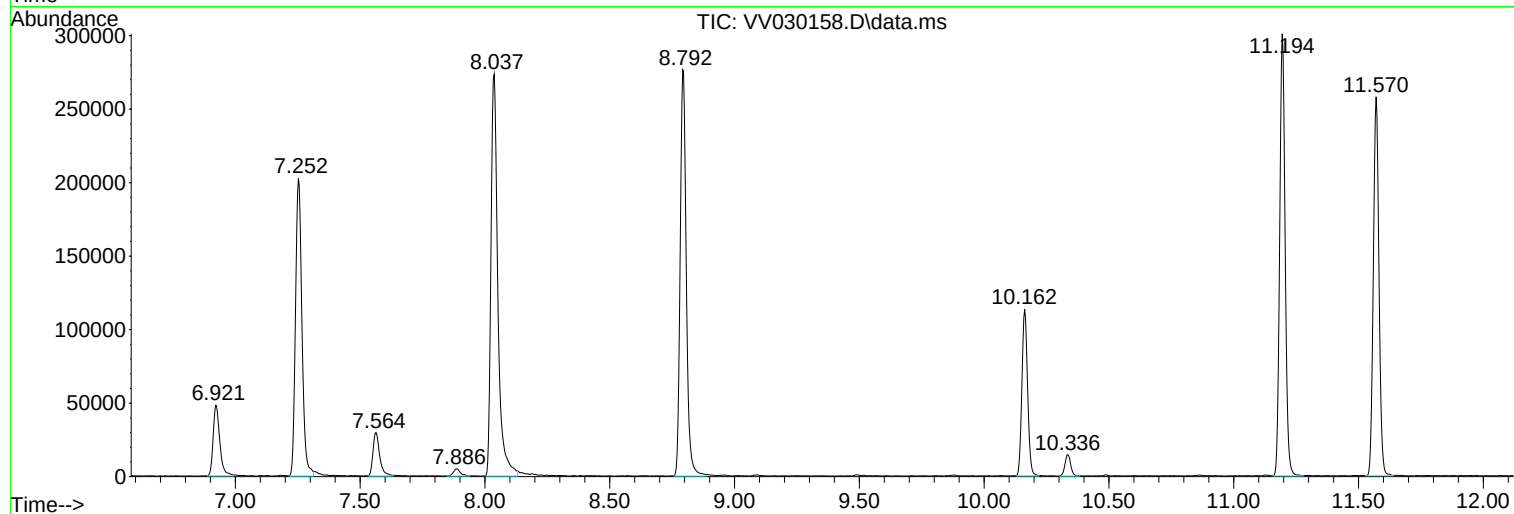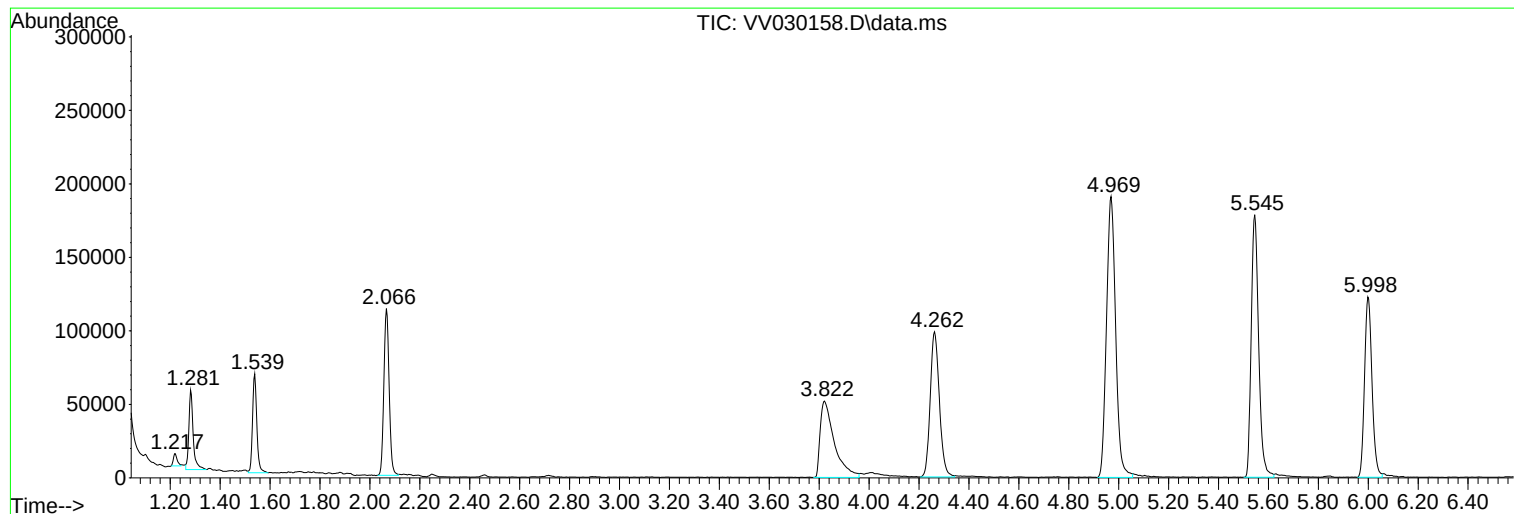

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030158.D
Acq On : 10 Mar 2023 16:27
Operator : SY/MD
Sample : 01868-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030158.D
Acq On : 10 Mar 2023 16:27
Operator : SY/MD
Sample : 01868-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
