

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030160.D
 Acq On : 10 Mar 2023 17:15
 Operator : SY/MD
 Sample : 01868-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	63	rBV	8751	10496	2.10%	0.237%
2	1.282	67	75	89	rVB	49700	58051	11.62%	1.309%
3	1.539	147	155	169	rVB	60446	71754	14.36%	1.618%
4	2.066	309	319	331	rBV	104846	152746	30.57%	3.444%
5	2.455	431	440	459	rVB3	10540	20384	4.08%	0.460%
6	3.822	853	865	908	rBV	45436	186474	37.32%	4.205%
7	4.002	910	921	939	rVB3	9894	28428	5.69%	0.641%
8	4.262	983	1002	1030	rBV2	90349	231029	46.24%	5.210%
9	4.969	1204	1222	1252	rBV3	174957	453130	90.70%	10.218%
10	5.545	1386	1401	1429	rBV	192902	398067	79.67%	8.977%
11	5.998	1528	1542	1564	rBV	113858	235845	47.21%	5.318%
12	6.924	1819	1830	1857	rBV	43632	82338	16.48%	1.857%
13	7.252	1919	1932	1953	rBV	189532	342535	68.56%	7.724%
14	7.561	2018	2028	2049	rBV	27068	49708	9.95%	1.121%
15	7.886	2115	2129	2142	rBV	14882	27145	5.43%	0.612%
16	8.037	2164	2176	2212	rBV	246316	469665	94.00%	10.591%
17	8.792	2399	2411	2442	rBV	300947	499618	100.00%	11.267%
18	10.162	2826	2837	2851	rBV2	103297	161867	32.40%	3.650%
19	10.336	2878	2891	2905	rVB	38901	62269	12.46%	1.404%
20	11.194	3146	3158	3178	rBV	310665	482805	96.63%	10.887%
21	11.570	3263	3275	3293	rBV	238966	374346	74.93%	8.442%
22	12.204	3461	3472	3486	rVB2	17605	28782	5.76%	0.649%
23	13.995	4020	4029	4040	rVB2	4569	7058	1.41%	0.159%




Sum of corrected areas: 4434540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030160.D
Acq On : 10 Mar 2023 17:15
Operator : SY/MD
Sample : 01868-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

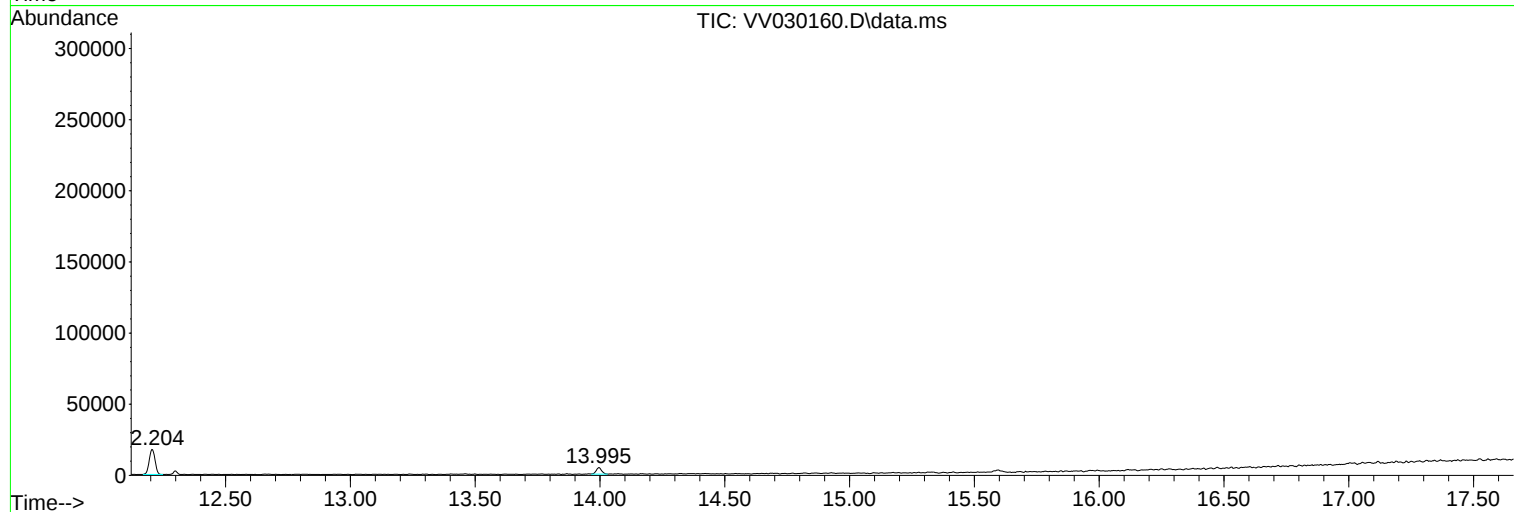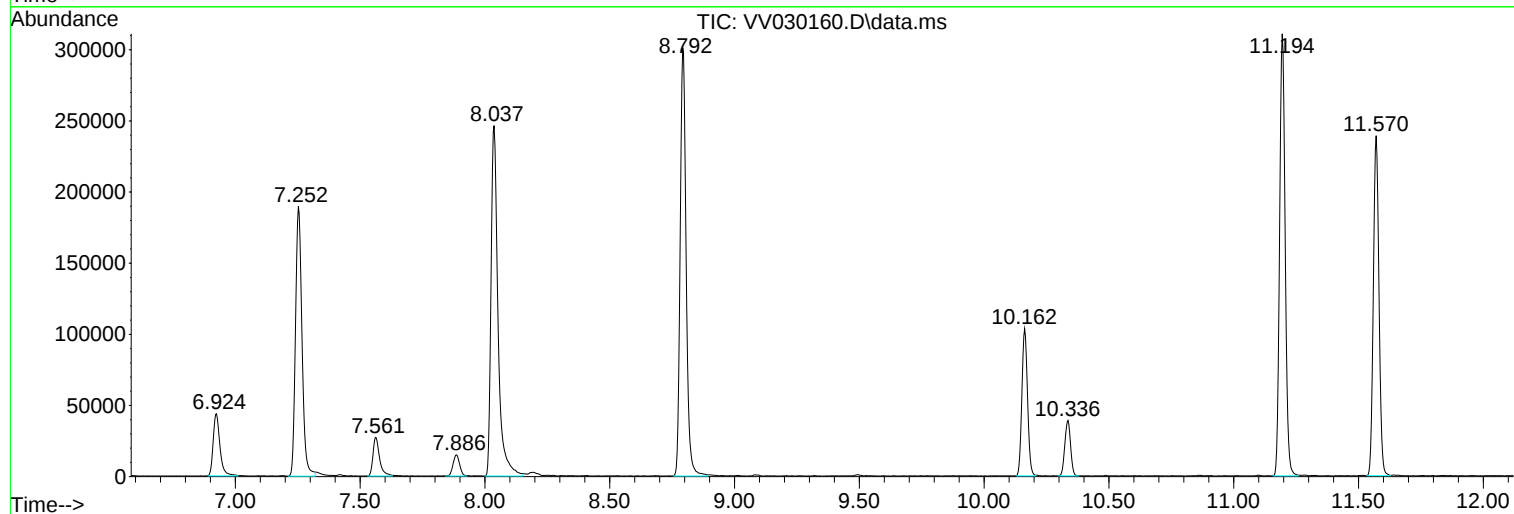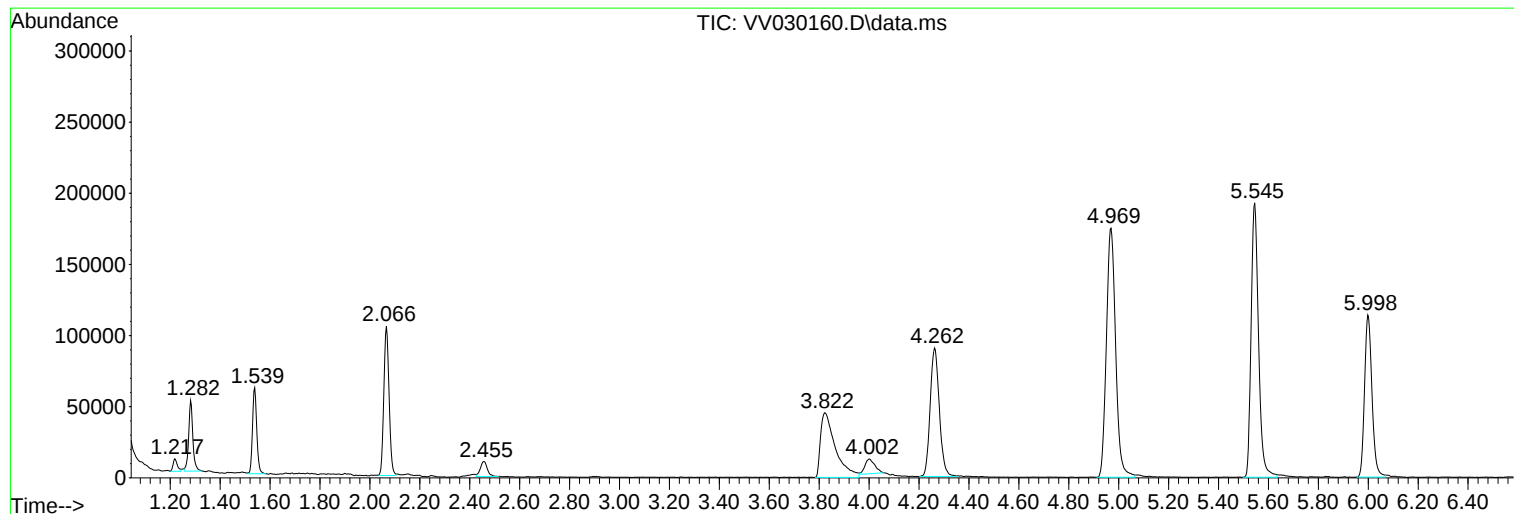

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030160.D
Acq On : 10 Mar 2023 17:15
Operator : SY/MD
Sample : 01868-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030160.D
Acq On : 10 Mar 2023 17:15
Operator : SY/MD
Sample : 01868-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------