

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030162.D
 Acq On : 10 Mar 2023 18:04
 Operator : SY/MD
 Sample : 01868-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	62	rBV	8386	8982	2.26%	0.240%
2	1.281	70	75	91	rVB	43570	49503	12.48%	1.324%
3	1.539	148	155	165	rVB	53900	61703	15.55%	1.650%
4	2.066	308	319	333	rBV	91602	132420	33.38%	3.541%
5	3.822	852	865	906	rBV2	41971	162401	40.93%	4.343%
6	4.002	912	921	948	rVB2	8802	27047	6.82%	0.723%
7	4.262	985	1002	1029	rBV2	78521	205745	51.86%	5.502%
8	4.969	1205	1222	1245	rBV2	152666	391496	98.67%	10.468%
9	5.545	1388	1401	1422	rBV	151452	311245	78.45%	8.323%
10	5.998	1528	1542	1560	rBV	100102	205612	51.82%	5.498%
11	6.924	1819	1830	1858	rBV	37496	70681	17.81%	1.890%
12	7.252	1920	1932	1963	rBV	160811	290076	73.11%	7.757%
13	7.561	2019	2028	2044	rBV	23332	42444	10.70%	1.135%
14	7.915	2118	2138	2151	rBV3	26632	62165	15.67%	1.662%
15	8.037	2164	2176	2213	rBV	206270	396444	99.92%	10.601%
16	8.792	2399	2411	2435	rBV	239418	396758	100.00%	10.609%
17	9.024	2478	2483	2493	rVB	5663	4422	1.11%	0.118%
18	10.162	2825	2837	2858	rVB	89506	142627	35.95%	3.814%
19	10.336	2877	2891	2904	rVB	27692	45630	11.50%	1.220%
20	11.194	3145	3158	3178	rBV	248191	383108	96.56%	10.244%
21	11.570	3263	3275	3295	rBV	198050	313116	78.92%	8.373%
22	12.204	3460	3472	3486	rBB2	15365	24499	6.17%	0.655%
23	13.995	4015	4029	4038	rBV	4101	6641	1.67%	0.178%
24	15.593	4515	4526	4539	rBV10	2148	5000	1.26%	0.134%




Sum of corrected areas: 3739765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030162.D
Acq On : 10 Mar 2023 18:04
Operator : SY/MD
Sample : 01868-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

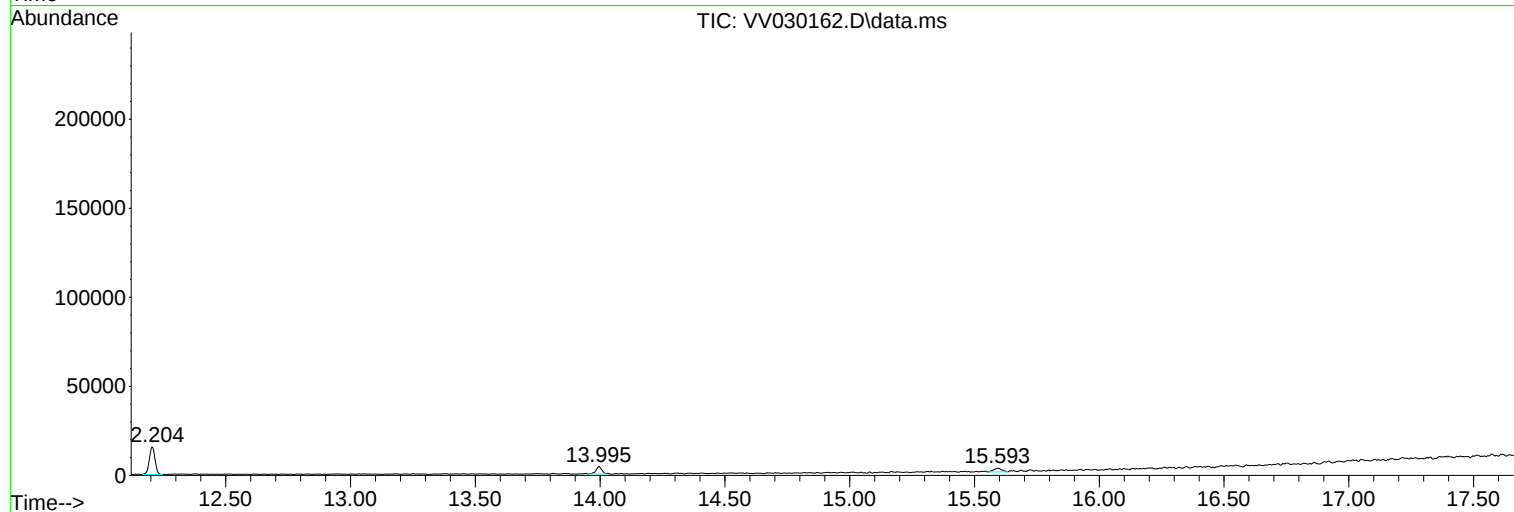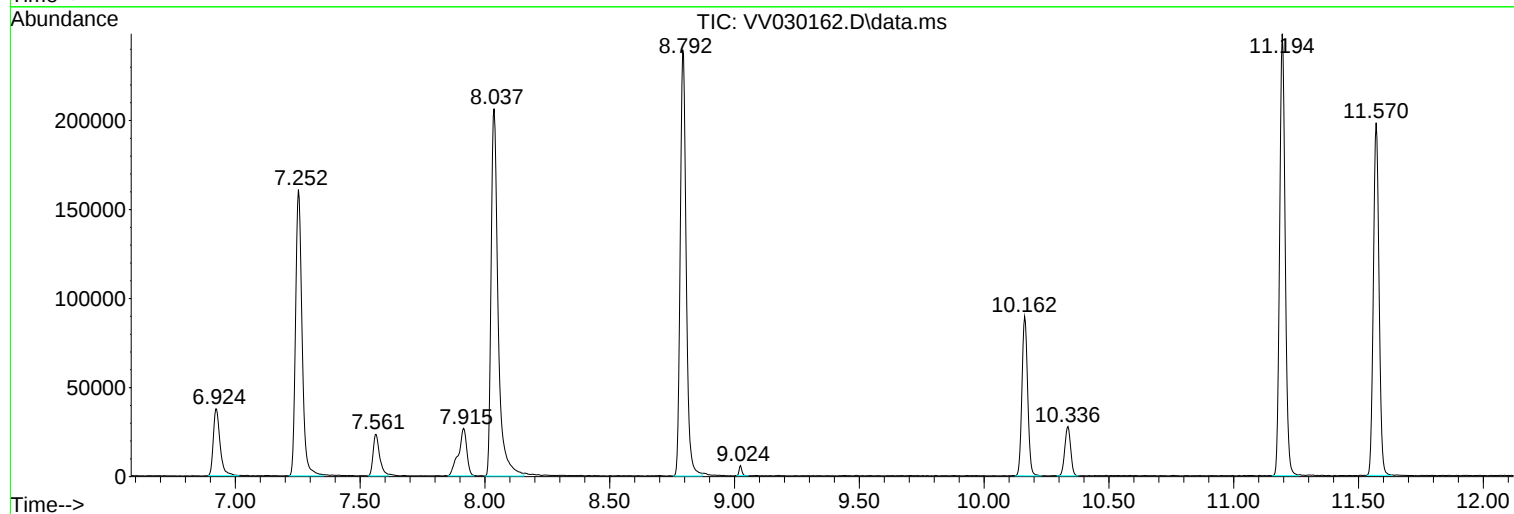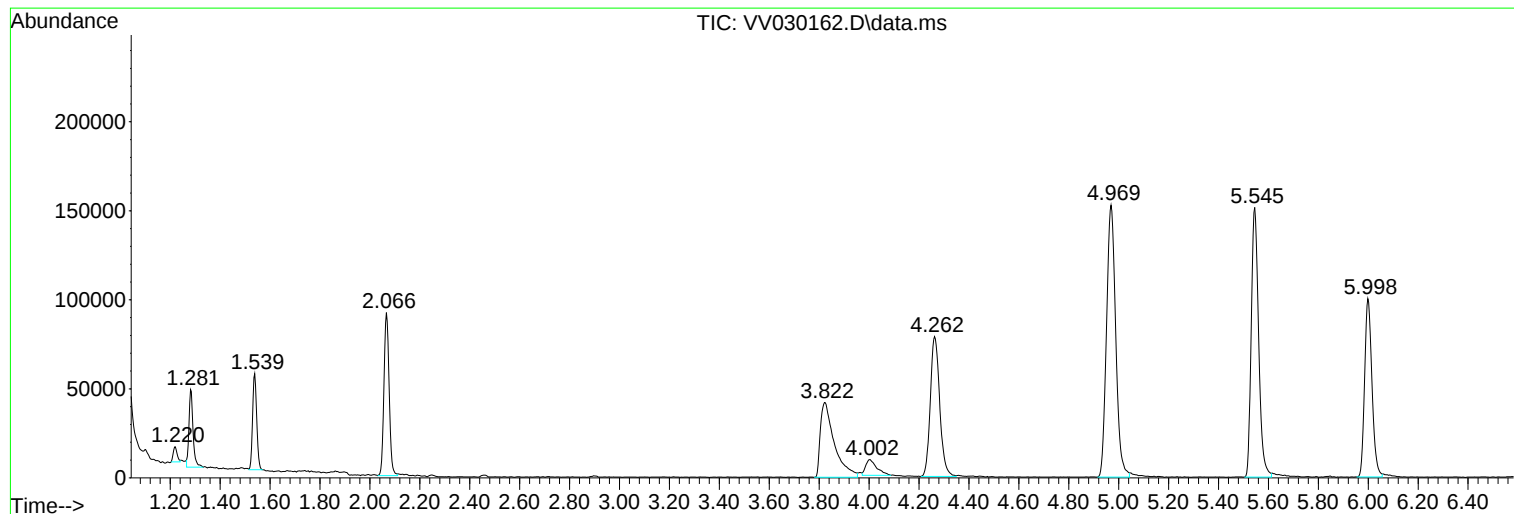

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030162.D
Acq On : 10 Mar 2023 18:04
Operator : SY/MD
Sample : 01868-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030162.D
Acq On : 10 Mar 2023 18:04
Operator : SY/MD
Sample : 01868-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc