

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030163.D
 Acq On : 10 Mar 2023 18:28
 Operator : SY/MD
 Sample : 01868-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	65	rBV2	9045	11898	2.81%	0.320%
2	1.282	68	75	93	rVB	46651	55755	13.16%	1.500%
3	1.539	147	155	165	rVB	53619	62600	14.77%	1.684%
4	2.066	308	319	336	rBV	94908	136915	32.30%	3.682%
5	3.825	853	866	910	rBV2	41636	170268	40.17%	4.579%
6	4.008	913	923	941	rVB3	5637	17164	4.05%	0.462%
7	4.262	984	1002	1024	rBV2	80137	205815	48.56%	5.536%
8	4.970	1204	1222	1248	rBV2	155207	400083	94.40%	10.761%
9	5.545	1387	1401	1422	rBV	147249	306197	72.25%	8.235%
10	5.998	1529	1542	1575	rBV	102217	212009	50.02%	5.702%
11	6.921	1818	1829	1847	rBV2	38642	72363	17.07%	1.946%
12	7.252	1921	1932	1963	rBV	166449	297639	70.23%	8.005%
13	7.561	2018	2028	2046	rBV	24084	43028	10.15%	1.157%
14	7.886	2117	2129	2135	rBV2	7867	14038	3.31%	0.378%
15	8.037	2165	2176	2214	rBV	219576	423828	100.00%	11.399%
16	8.793	2399	2411	2451	rBV	228509	386758	91.25%	10.402%
17	10.162	2825	2837	2856	rBV	94222	147681	34.84%	3.972%
18	10.336	2879	2891	2902	rBV	22497	36772	8.68%	0.989%
19	11.194	3147	3158	3183	rBV	241668	371617	87.68%	9.995%
20	11.571	3263	3275	3294	rBV	203457	320587	75.64%	8.622%
21	12.207	3461	3473	3482	rBV2	11571	18508	4.37%	0.498%
22	12.297	3494	3501	3508	rBV4	5277	6542	1.54%	0.176%




Sum of corrected areas: 3718065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030163.D
Acq On : 10 Mar 2023 18:28
Operator : SY/MD
Sample : 01868-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

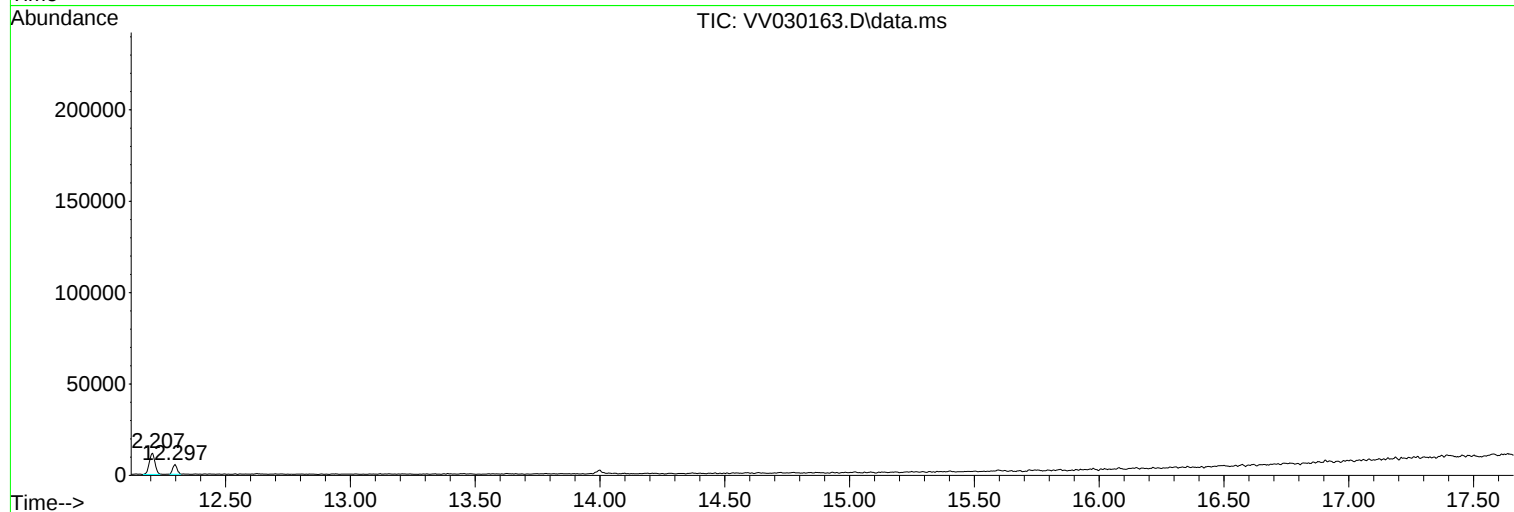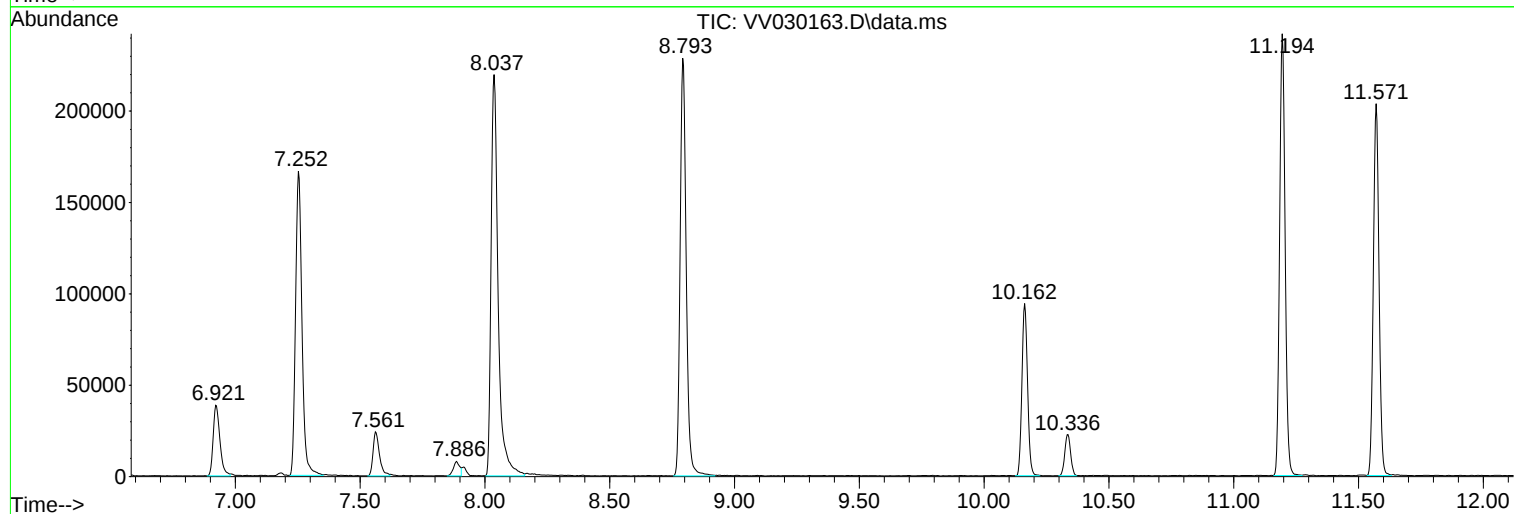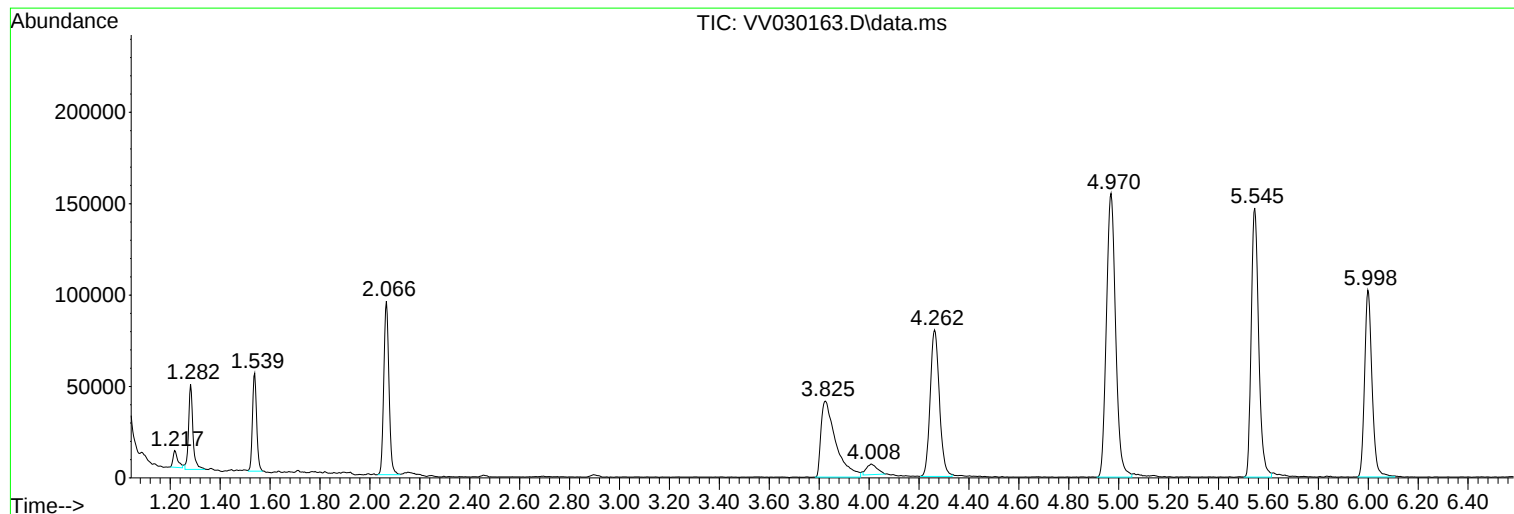

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030163.D
Acq On : 10 Mar 2023 18:28
Operator : SY/MD
Sample : 01868-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030163.D
Acq On : 10 Mar 2023 18:28
Operator : SY/MD
Sample : 01868-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------