

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
 Data File : VV030168.D
 Acq On : 10 Mar 2023 20:29
 Operator : SY/MD
 Sample : VIBLK277
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK277

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	61	rBV2	4307	4698	1.10%	0.123%
2	1.282	69	75	93	rVB	47909	54709	12.82%	1.430%
3	1.539	147	155	172	rVB	59408	70970	16.64%	1.855%
4	2.066	309	319	334	rBV	102783	149568	35.06%	3.909%
5	2.458	431	441	454	rBV3	7753	13243	3.10%	0.346%
6	3.822	853	865	904	rBV2	43417	166652	39.07%	4.356%
7	4.262	985	1002	1025	rBV	85501	216438	50.74%	5.657%
8	4.969	1204	1222	1255	rBV2	163890	426595	100.00%	11.150%
9	5.545	1388	1401	1424	rBV	140074	290330	68.06%	7.589%
10	5.998	1528	1542	1570	rBV	106827	223014	52.28%	5.829%
11	6.921	1818	1829	1856	rBV2	40478	77084	18.07%	2.015%
12	7.252	1917	1932	1960	rBV	178743	320627	75.16%	8.380%
13	7.561	2018	2028	2050	rBV2	24954	45719	10.72%	1.195%
14	7.915	2120	2138	2164	rBV	56980	106270	24.91%	2.778%
15	8.037	2164	2176	2207	rBV2	218806	416059	97.53%	10.875%
16	8.371	2270	2280	2294	rVB2	3125	5642	1.32%	0.147%
17	8.792	2399	2411	2444	rBV	220828	370480	86.85%	9.683%
18	10.162	2823	2837	2862	rBB	97769	151747	35.57%	3.966%
19	10.336	2882	2891	2901	rBV	5962	9463	2.22%	0.247%
20	11.194	3147	3158	3178	rBV	231422	357430	83.79%	9.342%
21	11.571	3263	3275	3294	rBV	217420	339898	79.68%	8.884%
22	12.204	3463	3472	3484	rBV3	6045	9260	2.17%	0.242%




Sum of corrected areas: 3825896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030168.D
Acq On : 10 Mar 2023 20:29
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

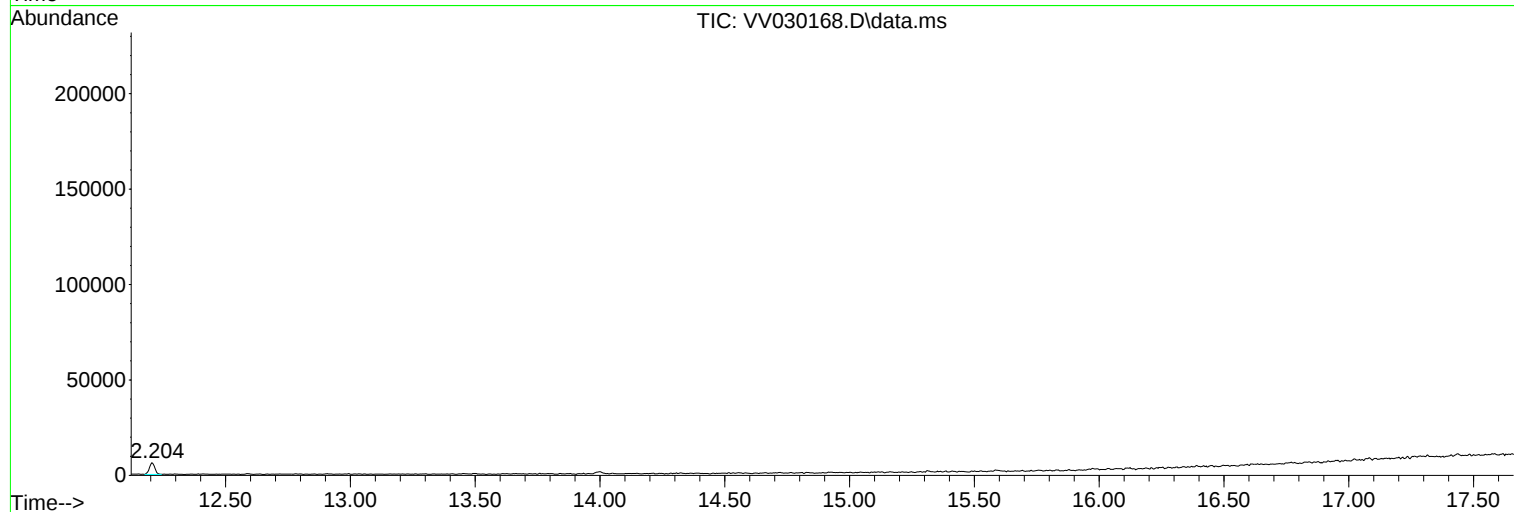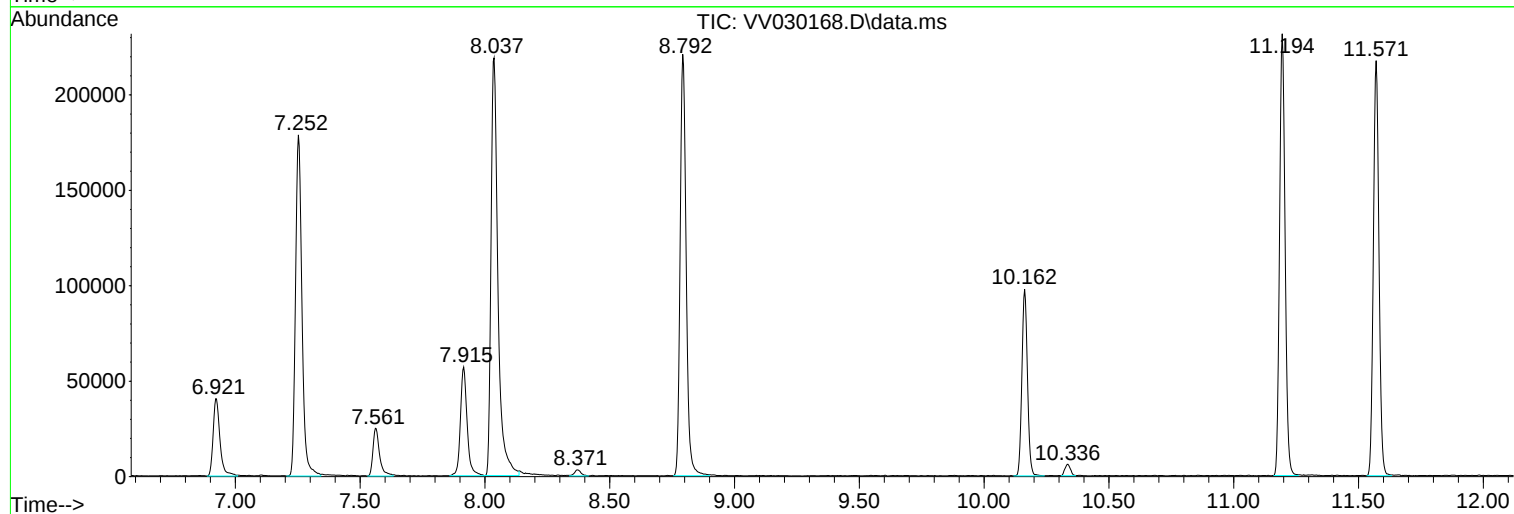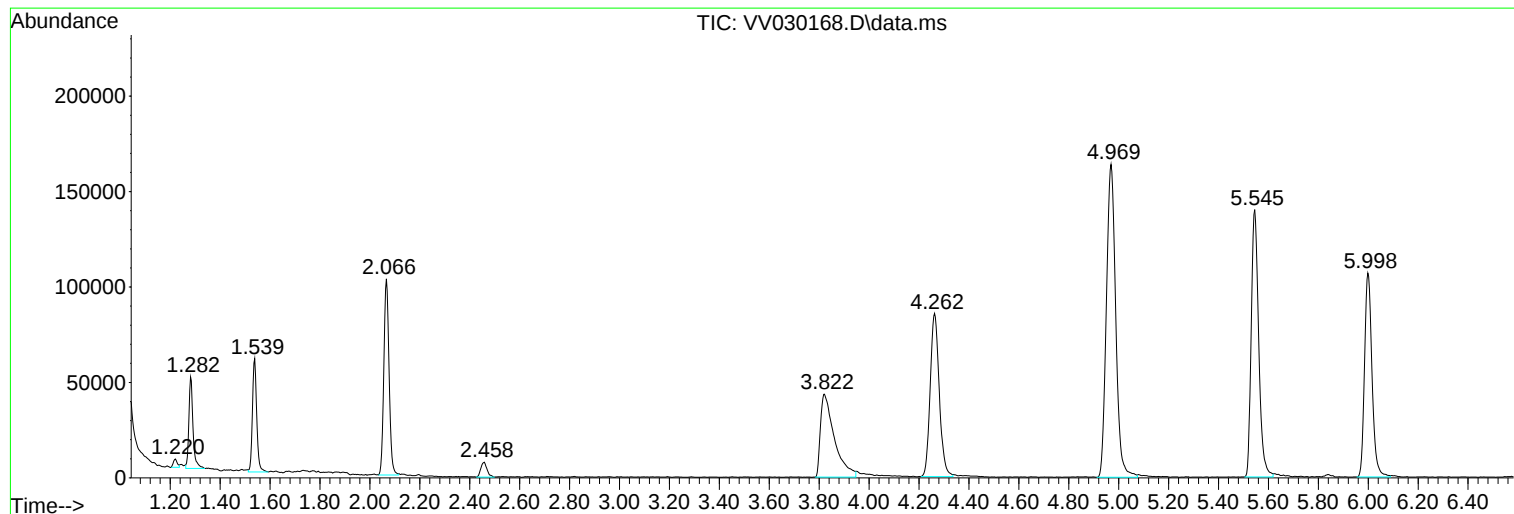

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030168.D
Acq On : 10 Mar 2023 20:29
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030168.D
Acq On : 10 Mar 2023 20:29
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc