


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031023\
Data File : VV030147.D
Acq On : 10 Mar 2023 10:15
Operator : SY/MD
Sample : BFB229
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB229

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Mar 11 00:01:55 2023

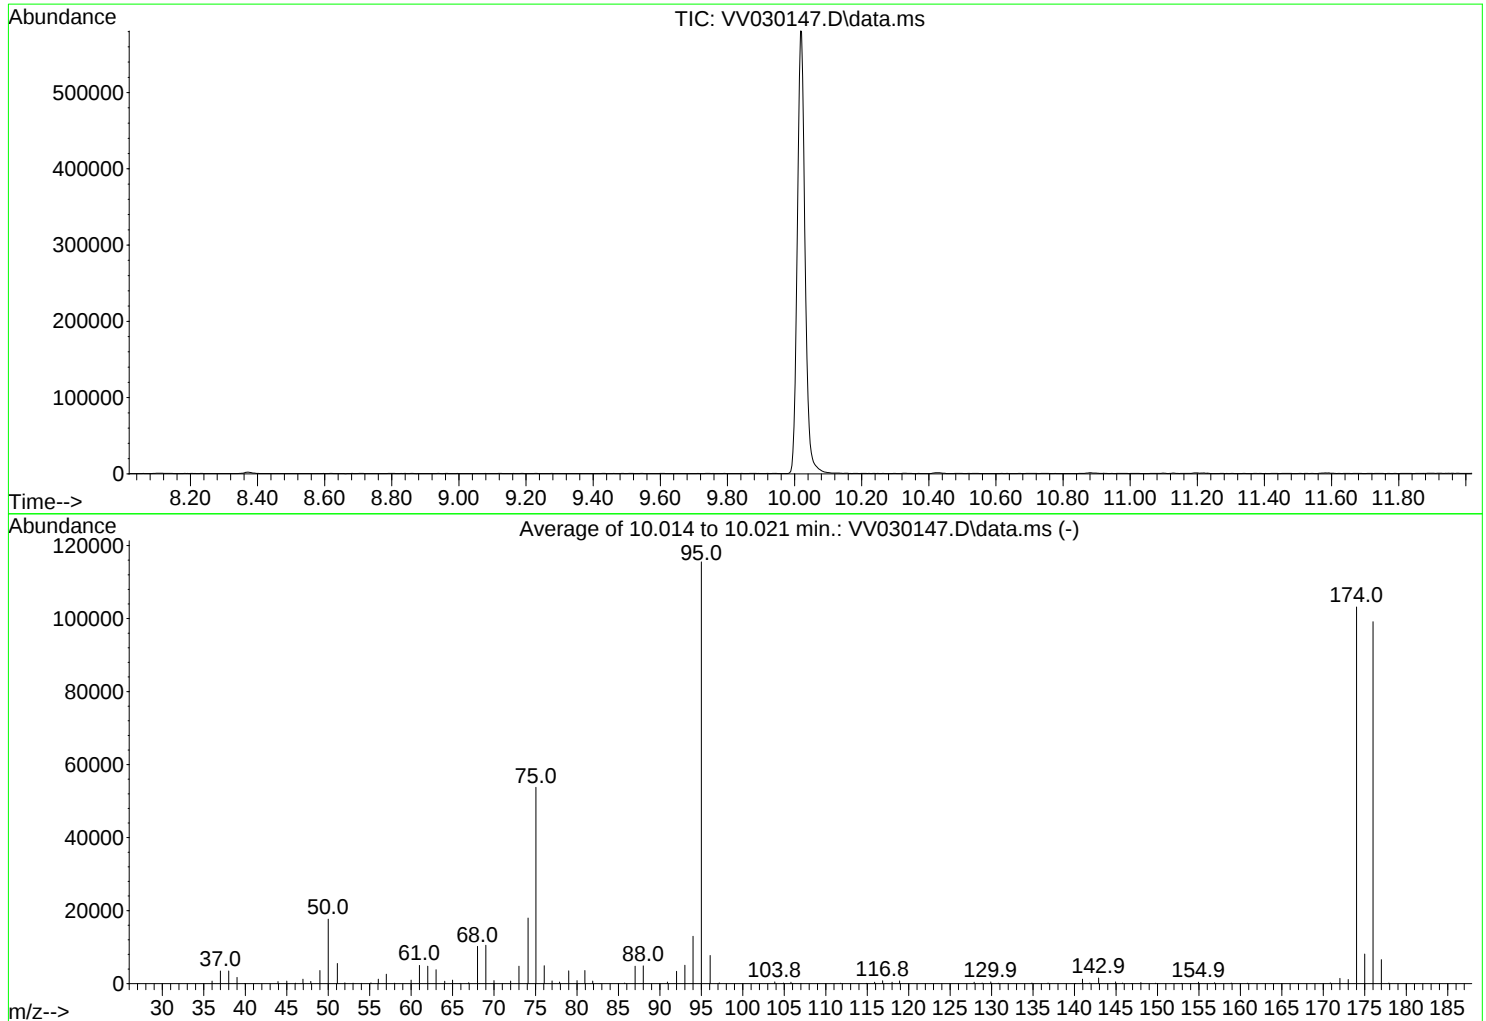

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	17659	PASS
75	95	30	80	46.5	53768	PASS
95	95	100	100	100.0	115539	PASS
96	95	5	9	6.7	7728	PASS
173	174	0.00	2	1.1	1135	PASS
174	95	50	120	89.3	103152	PASS
175	174	5	9	7.9	8131	PASS
176	174	95	105	96.1	99149	PASS
177	176	5	10	6.6	6593	PASS

m/z	Abundance
40.00	155.0
43.90	276.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	714.0
37.00	3328.0
38.00	3281.0
39.00	1646.0
40.00	195.0
44.00	784.0
45.00	639.0
46.00	137.0
46.90	1150.0
47.90	480.0
49.00	3217.0
50.00	16736.0
51.10	5286.0
52.00	238.0
53.00	114.0
55.10	213.0
56.00	1164.0
57.00	2495.0
58.00	136.0
60.00	930.0
61.00	4709.0
62.00	4522.0
63.00	3763.0
64.00	590.0
65.00	844.0
67.00	237.0
68.00	9862.0
69.00	10186.0
70.00	864.0
71.00	109.0
72.00	720.0
73.00	4366.0
74.10	17128.0
75.00	50600.0
76.00	4659.0
77.00	680.0
77.90	378.0
79.00	3358.0
80.00	789.0
81.00	3428.0
81.90	634.0
82.80	123.0
85.80	181.0
87.00	4344.0
88.00	4509.0
90.90	437.0
92.00	3083.0
93.00	4921.0
94.00	11990.0
95.00	107896.0
96.10	7550.0
97.20	224.0
103.80	456.0
104.90	183.0
105.80	337.0
111.80	105.0
115.90	325.0
116.80	748.0
118.00	352.0
118.90	673.0
127.90	410.0
128.80	194.0
129.90	449.0
130.70	132.0
134.80	164.0
136.80	186.0
140.90	1101.0
141.90	151.0
142.90	1437.0
144.90	489.0
145.80	154.0
148.00	279.0
149.80	122.0
154.90	347.0
156.90	215.0
158.90	165.0
160.90	125.0
170.80	240.0
172.00	1303.0
173.00	1075.0
174.00	93752.0
175.00	7602.0
176.00	90000.0
177.00	6057.0
177.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	699.0
37.00	3573.0
38.00	3622.0
39.00	1803.0
39.90	185.0
44.00	879.0
45.00	733.0
46.10	157.0
47.00	1281.0
47.90	646.0
49.00	3748.0
50.00	18336.0
51.10	5720.0
52.00	235.0
53.00	126.0
54.00	107.0
55.20	235.0
56.00	1260.0
57.00	2698.0
58.00	164.0
60.00	1038.0
61.00	5196.0
62.00	4948.0
63.00	3954.0
64.10	708.0
65.00	1005.0
65.90	107.0
67.00	250.0
68.00	10532.0
69.00	10792.0
70.00	865.0
72.00	730.0
73.00	5019.0
74.10	18616.0
75.00	55600.0
76.00	5068.0
77.00	773.0
77.90	446.0
79.00	3621.0
80.00	876.0
80.90	3719.0
81.90	735.0
85.70	205.0
87.00	4938.0
88.00	5098.0
90.90	437.0
92.00	3529.0
93.00	5211.0
94.00	13440.0
95.00	119760.0
96.10	8018.0
97.20	225.0
103.90	473.0
104.90	221.0
105.80	418.0
107.00	102.0
111.80	130.0
114.90	106.0
115.90	385.0
116.90	810.0
118.00	416.0
118.90	804.0
127.90	445.0
128.90	209.0
129.90	505.0
130.80	138.0
134.80	200.0
136.80	168.0
140.90	1258.0
141.80	171.0
142.90	1580.0
145.00	513.0
145.80	198.0
146.90	102.0
148.00	310.0
149.80	136.0
152.90	103.0
155.00	388.0
156.90	262.0
158.90	213.0
160.90	162.0
170.90	237.0
172.00	1553.0
173.00	1175.0
174.00	106784.0
175.00	8439.0
176.00	102904.0
177.00	6867.0
177.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	653.0
37.00	3482.0
38.00	3470.0
39.00	1740.0
39.90	190.0
44.00	863.0
45.00	757.0
46.10	141.0
47.00	1293.0
47.90	732.0
49.00	3871.0
50.00	17904.0
51.10	5614.0
52.00	216.0
53.00	122.0
54.00	119.0
55.10	244.0
56.10	1253.0
57.00	2560.0
58.00	147.0
60.00	981.0
61.00	5125.0
62.00	4857.0
63.00	3776.0
64.10	744.0
65.00	1067.0
65.90	128.0
66.90	269.0
68.00	10227.0
69.00	10581.0
70.00	805.0
72.00	644.0
73.00	5004.0
74.10	18152.0
75.10	55104.0
76.10	4972.0
77.00	778.0
77.90	457.0
79.00	3615.0
80.00	889.0
80.90	3693.0
81.90	723.0
85.70	201.0
87.00	5079.0
88.00	4966.0
90.90	409.0
92.00	3472.0
93.00	5032.0
94.00	13555.0
95.00	118960.0
96.00	7616.0
97.10	223.0
103.90	463.0
104.90	191.0
105.80	459.0
107.00	114.0
111.80	120.0
113.00	119.0
114.90	134.0
115.90	423.0
116.90	862.0
118.00	388.0
118.90	760.0
127.90	399.0
128.90	181.0
129.90	467.0
130.90	164.0
134.90	206.0
136.80	170.0
140.10	131.0
141.00	1285.0
141.80	170.0
142.90	1535.0
145.00	496.0
145.80	219.0
148.00	277.0
149.80	139.0
152.90	103.0
155.00	407.0
156.90	265.0
158.90	213.0
160.80	161.0
170.90	223.0
172.00	1551.0
173.00	1155.0
174.00	108920.0
175.00	8353.0
176.00	104544.0
177.00	6855.0
177.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229