

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031119\
 Data File : VV009587.D
 Acq On : 11 Mar 2019 11:51
 Operator : SY/MD
 Sample : K1818-17
 Misc : 6.06G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0R7

Quant Time: Mar 12 03:58:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 11 12:01:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	148949	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	140187	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61848	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31354	17.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.96%
7) Chloroethane-d5	1.58	69	64167	24.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.00%
10) 1,1-Dichloroethene-d2	2.13	63	73957	15.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.40%
20) 2-Butanone-d5	3.95	46	26500	43.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.74%
24) Chloroform-d	4.40	84	84338	23.77	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.08%
26) 1,2-Dichloroethane-d4	5.08	65	49509	24.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.12%
29) Benzene-d6	5.10	84	162306	23.38	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.52%
33) 1,2-Dichloropropane-d6	6.12	67	52134	25.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.76%
37) Toluene-d8	7.36	98	156347	23.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.40%
38) trans-1,3-Dichloropropene-	7.66	79	21260	21.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.64%
39) 2-Hexanone-d5	8.14	63	20043	41.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.82%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	49336	22.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.36%
61) 1,2-Dichlorobenzene-d4	11.68	152	55947	24.78	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.12%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Methylene chloride	2.53	84	3694	1.890	ug/L	93




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031119\
Data File : VV009587.D
Acq On : 11 Mar 2019 11:51
Operator : SY/MD
Sample : K1818-17
Misc : 6.06G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0R7

Quant Time: Mar 12 03:58:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 12:01:50 2019
Response via : Initial Calibration

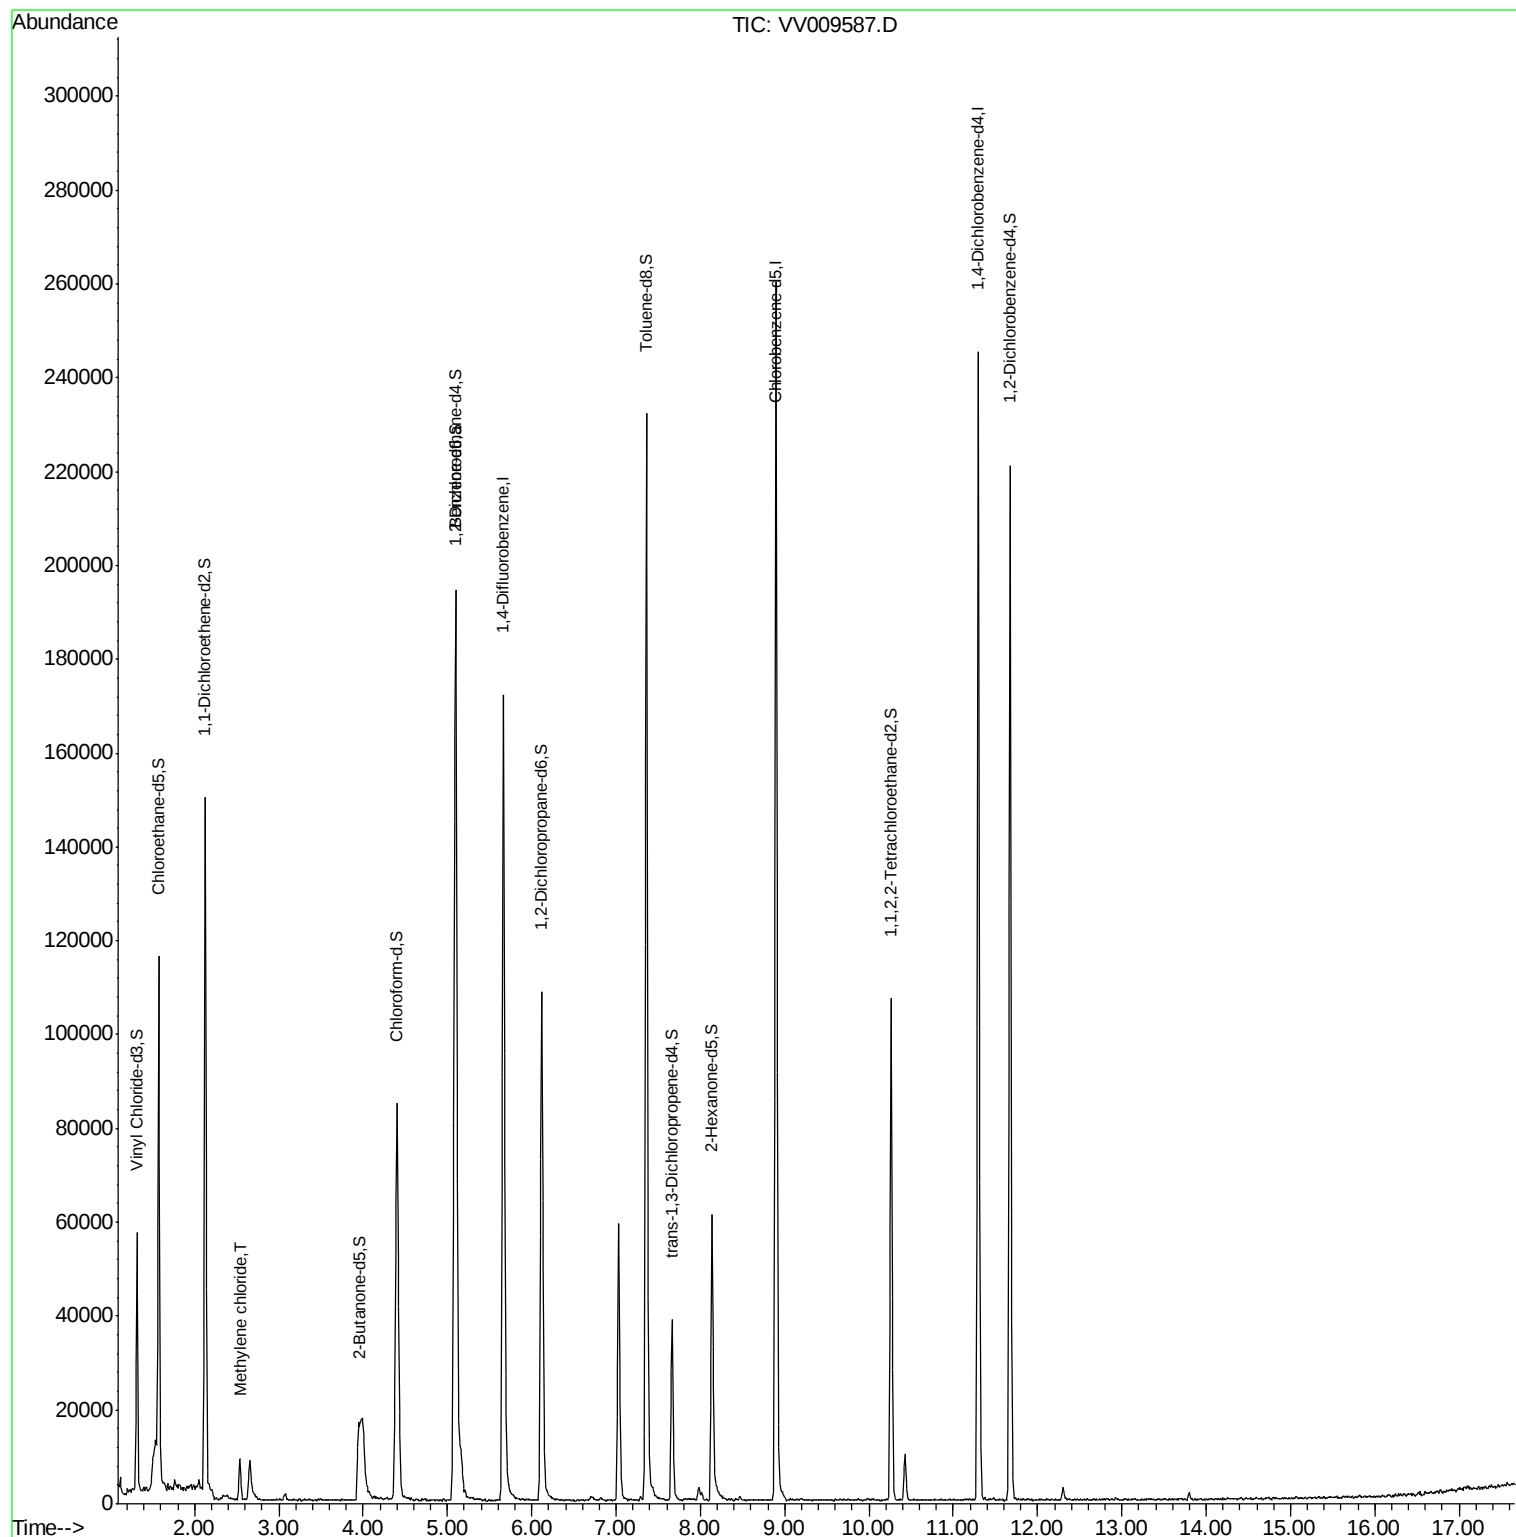

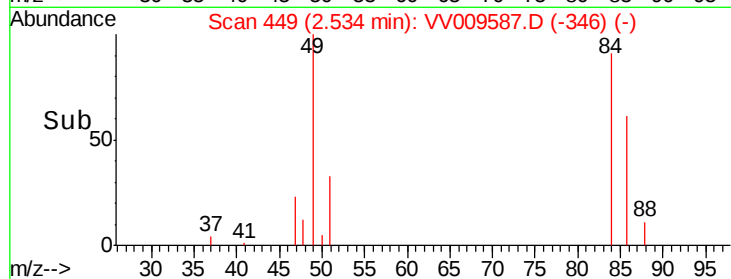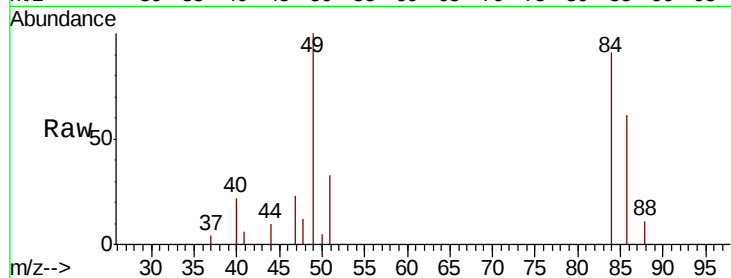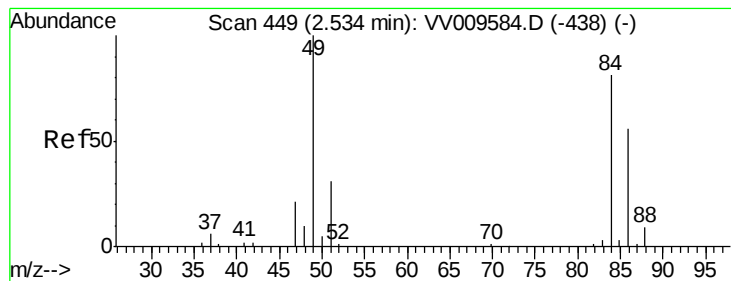

#16
Methylene chloride
Concen: 1.890 ug/L
RT: 2.53 min Scan# 449
Delta R.T. 0.00 min
Lab File: VV009587.D
Acq: 11 Mar 2019 11:51

Instrument :
MSVOA_V
ClientSampleId :
BF0R7

Tgt Ion: 84 Resp: 3694
Ion Ratio Lower Upper
84 100
49 110.4 84.6 157.0
86 67.4 46.1 85.7

