


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031119\
Data File : VV009583.D
Acq On : 11 Mar 2019 08:45
Operator : SY/MD
Sample : BFB74
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
Title : VOC Analysis
Last Update : Tue Mar 12 04:11:52 2019

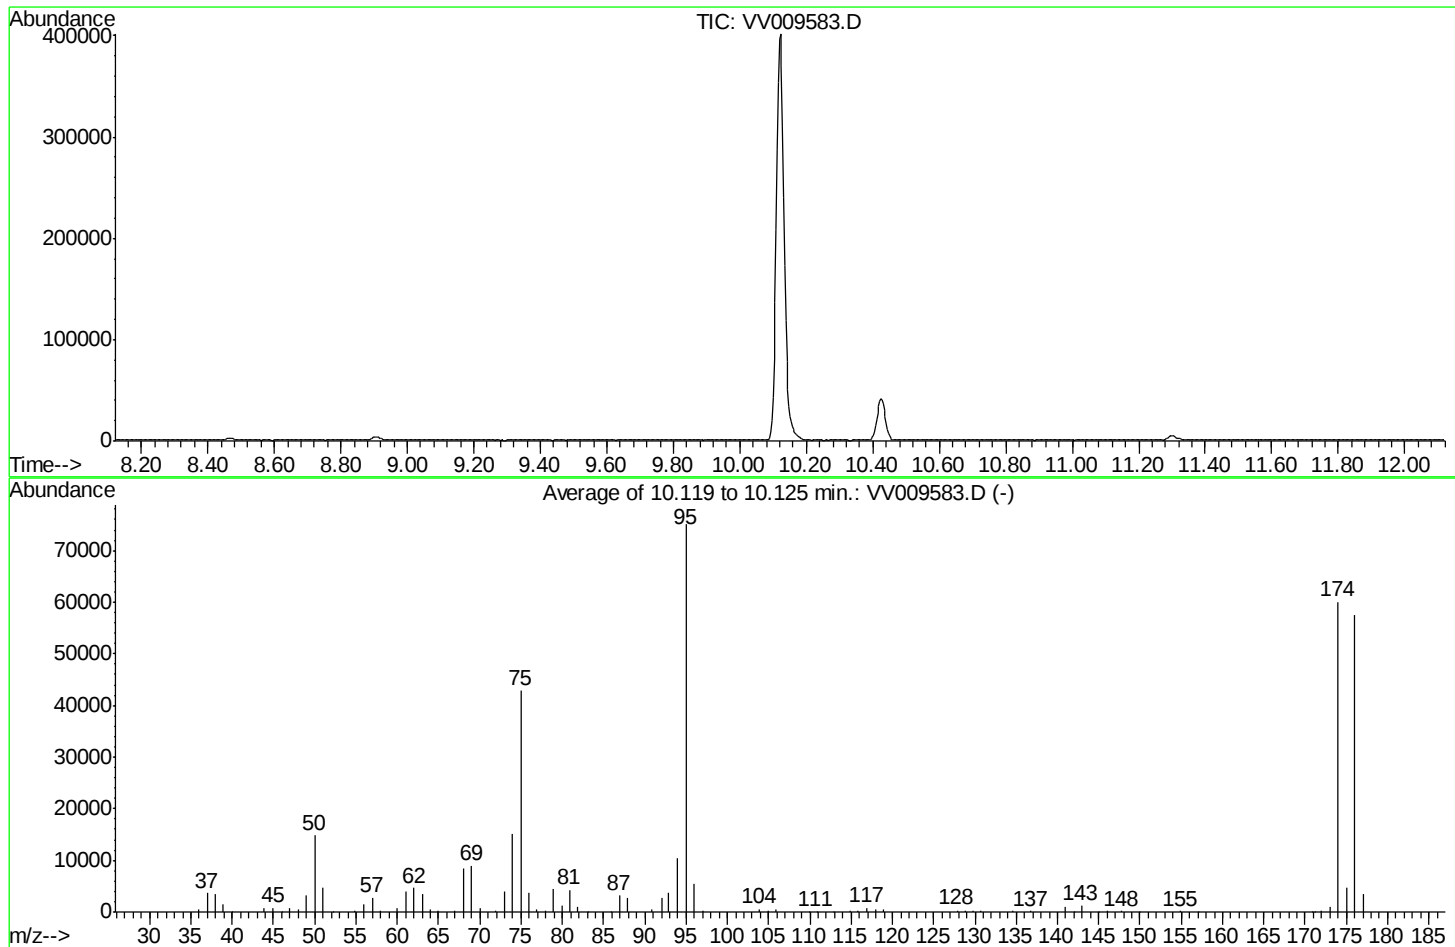

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14828	PASS
75	95	30	80	57.0	42786	PASS
95	95	100	100	100.0	75074	PASS
96	95	5	9	7.3	5466	PASS
173	174	0.00	2	1.7	1043	PASS
174	95	50	120	79.9	60010	PASS
175	174	5	9	7.9	4723	PASS
176	174	95	101	95.9	57565	PASS
177	176	5	9	6.1	3505	PASS

m/z	Abundance
39.90	563.0
43.90	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	522.0
37.00	3365.0
37.90	3130.0
39.00	1251.0
39.90	631.0
43.90	812.0
45.00	760.0
45.90	131.0
46.90	677.0
47.90	407.0
49.00	3074.0
50.00	14101.0
51.00	4592.0
54.90	193.0
55.90	1371.0
56.90	2685.0
58.00	146.0
60.00	790.0
61.00	3765.0
62.00	4507.0
63.00	3447.0
64.00	432.0
64.90	165.0
67.00	293.0
68.00	8082.0
69.00	8534.0
70.00	597.0
72.00	304.0
73.00	3708.0
74.00	13997.0
75.00	39928.0
76.00	3580.0
76.90	458.0
78.00	324.0
78.90	4230.0
79.90	1064.0
80.90	3868.0
81.90	925.0
83.10	101.0
87.00	3129.0
87.90	2591.0
90.80	439.0
92.00	2564.0
92.90	3412.0
94.00	9870.0
95.00	71584.0
96.00	4949.0
97.10	169.0
103.90	479.0
104.90	138.0
105.90	486.0
110.80	130.0
112.80	121.0
114.90	127.0
115.70	310.0
116.90	744.0
117.90	454.0
118.90	444.0
127.90	298.0
128.80	150.0
129.80	315.0
130.70	107.0
134.60	139.0
136.80	203.0
140.90	968.0
142.00	157.0
142.90	1117.0
144.90	117.0
146.00	141.0
147.80	167.0
154.80	157.0
157.00	121.0
170.90	129.0
171.20	129.0
171.90	391.0
173.00	984.0
174.00	58160.0
175.00	4458.0
176.00	56032.0
177.00	3286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	562.0
37.00	3796.0
37.90	3487.0
38.90	1491.0
39.90	642.0
43.90	856.0
45.00	815.0
46.00	105.0
46.90	691.0
47.90	479.0
49.00	3463.0
50.00	15304.0
51.00	4864.0
52.20	125.0
54.80	204.0
55.90	1552.0
56.90	2899.0
58.00	193.0
60.00	816.0
61.00	4246.0
62.00	4828.0
63.00	3696.0
64.00	427.0
64.90	202.0
67.00	291.0
68.00	8775.0
69.00	9331.0
70.00	672.0
71.90	349.0
73.00	4096.0
74.00	15502.0
75.00	44104.0
76.00	3907.0
76.90	454.0
78.00	328.0
78.90	4469.0
79.90	1222.0
80.90	4403.0
81.90	1016.0
83.10	104.0
85.90	155.0
87.00	3175.0
87.90	2914.0
90.90	450.0
92.00	2761.0
92.90	3835.0
94.00	10857.0
95.00	77472.0
96.00	5705.0
97.10	131.0
103.90	566.0
105.00	154.0
105.90	529.0
110.80	122.0
112.80	125.0
114.80	149.0
115.80	293.0
116.90	805.0
117.90	475.0
118.90	565.0
127.80	359.0
128.80	210.0
129.80	299.0
130.70	162.0
134.60	175.0
136.80	246.0
140.90	1025.0
142.10	168.0
142.90	1212.0
146.00	143.0
147.80	189.0
155.00	193.0
157.00	108.0
170.80	130.0
171.90	354.0
173.00	1072.0
174.00	62048.0
175.00	4906.0
176.00	59160.0
177.00	3596.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	606.0
37.00	3906.0
37.90	3606.0
38.90	1594.0
39.90	673.0
43.90	878.0
45.00	757.0
47.00	651.0
48.00	446.0
49.00	3424.0
50.00	15080.0
51.00	4802.0
52.10	141.0
54.70	235.0
55.90	1599.0
57.00	2782.0
58.00	182.0
60.00	728.0
61.00	4273.0
62.00	4544.0
63.00	3667.0
64.00	431.0
64.90	254.0
67.00	236.0
68.00	8756.0
69.00	9087.0
70.00	765.0
71.90	433.0
73.00	4027.0
74.00	15667.0
75.00	44328.0
76.00	3826.0
77.00	380.0
77.90	321.0
78.90	4505.0
79.90	1190.0
80.90	4565.0
81.90	1050.0
83.10	104.0
85.90	207.0
86.90	3061.0
87.90	2986.0
90.90	477.0
92.00	2599.0
92.90	3914.0
94.00	10802.0
95.00	76168.0
96.00	5746.0
97.10	100.0
103.90	594.0
105.00	162.0
105.90	546.0
109.90	106.0
110.80	135.0
112.90	137.0
114.80	149.0
115.80	294.0
116.90	743.0
117.90	455.0
118.90	631.0
127.80	394.0
128.80	214.0
129.80	327.0
130.70	186.0
134.60	183.0
136.80	213.0
140.90	1037.0
142.90	1210.0
146.00	150.0
147.80	187.0
149.90	117.0
155.00	210.0
170.80	105.0
172.00	391.0
173.00	1073.0
174.00	59824.0
175.00	4807.0
176.00	57504.0
177.00	3633.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74