

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020500.D
 Acq On : 10 Mar 2021 17:07
 Operator : SY/MD
 Sample : M1610-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG506

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	321214	324870	17.08%	2.219%
2	1.568	157	164	178	rVB	232290	264214	13.89%	1.805%
3	2.108	321	332	370	rVB	510066	765053	40.22%	5.227%
4	2.294	383	390	402	rVB5	824	1521	0.08%	0.010%
5	2.343	403	405	408	rBV2	266	182	0.01%	0.001%
6	2.510	451	457	462	rBV2	1276	1652	0.09%	0.011%
7	2.568	472	475	480	rBV3	272	248	0.01%	0.002%
8	2.629	492	494	497	rBV3	324	205	0.01%	0.001%
9	2.709	514	519	521	rBV3	377	290	0.02%	0.002%
10	2.764	533	536	539	rVB2	289	210	0.01%	0.001%
11	2.809	544	550	553	rBV2	269	306	0.02%	0.002%
12	2.870	566	569	572	rBV	193	174	0.01%	0.001%
13	2.902	576	579	582	rBV2	236	162	0.01%	0.001%
14	2.931	582	588	593	rBV2	253	403	0.02%	0.003%
15	2.966	595	599	609	rVB4	450	629	0.03%	0.004%
16	3.378	722	727	738	rBV2	365	647	0.03%	0.004%
17	3.487	758	761	764	rBV2	251	181	0.01%	0.001%
18	3.590	787	793	797	rVB2	230	280	0.01%	0.002%
19	3.770	847	849	855	rVB	192	173	0.01%	0.001%
20	3.892	873	887	928	rBV	99383	319528	16.80%	2.183%
21	4.349	1011	1029	1060	rBV	298816	759956	39.95%	5.192%
22	4.532	1083	1086	1090	rVB2	416	343	0.02%	0.002%
23	4.635	1112	1118	1120	rBV2	366	333	0.02%	0.002%
24	4.648	1120	1122	1127	rVV2	232	215	0.01%	0.001%
25	4.683	1131	1133	1137	rVB3	600	375	0.02%	0.003%
26	4.706	1137	1140	1144	rBV2	213	233	0.01%	0.002%
27	4.748	1150	1153	1156	rBV	321	239	0.01%	0.002%
28	4.831	1176	1179	1182	rBV2	182	195	0.01%	0.001%
29	4.928	1203	1209	1212	rVV3	286	333	0.02%	0.002%
30	4.953	1212	1217	1222	rVB3	287	263	0.01%	0.002%
31	5.047	1229	1246	1289	rBV2	744666	1902333	100.00%	12.996%
32	5.265	1311	1314	1317	rVB3	405	265	0.01%	0.002%
33	5.323	1329	1332	1336	rBV3	256	287	0.02%	0.002%
34	5.420	1360	1362	1365	rVB2	501	260	0.01%	0.002%
35	5.487	1379	1383	1384	rBV	257	169	0.01%	0.001%
36	5.497	1384	1386	1391	rVB2	415	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020500.D
 Acq On : 10 Mar 2021 17:07
 Operator : SY/MD
 Sample : M1610-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG506

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.619	1411	1424	1458	rBV	553739	1122632	59.01%	7.670%
38	5.796	1477	1479	1490	rVB4	519	626	0.03%	0.004%
39	5.905	1501	1513	1539	rBV	78867	162920	8.56%	1.113%
40	6.072	1551	1565	1596	rBV	404643	814883	42.84%	5.567%
41	6.204	1603	1606	1607	rBV	515	349	0.02%	0.002%
42	6.320	1637	1642	1644	rBV3	217	154	0.01%	0.001%
43	6.333	1644	1646	1648	rVB	427	178	0.01%	0.001%
44	6.352	1648	1652	1654	rBV	376	283	0.01%	0.002%
45	6.391	1660	1664	1667	rBV	220	180	0.01%	0.001%
46	6.519	1698	1704	1705	rBV2	714	655	0.03%	0.004%
47	6.638	1737	1741	1744	rBV	236	205	0.01%	0.001%
48	6.773	1780	1783	1789	rBV2	215	208	0.01%	0.001%
49	6.989	1838	1850	1876	rBV	216186	398924	20.97%	2.725%
50	7.143	1896	1898	1905	rVB6	561	369	0.02%	0.003%
51	7.204	1915	1917	1922	rVB3	441	283	0.01%	0.002%
52	7.230	1922	1925	1927	rBV2	304	187	0.01%	0.001%
53	7.320	1940	1953	1974	rBV	940073	1621984	85.26%	11.081%
54	7.567	2026	2030	2032	rVB2	331	240	0.01%	0.002%
55	7.625	2036	2048	2068	rBV	153699	268355	14.11%	1.833%
56	7.841	2112	2115	2117	rBV2	355	248	0.01%	0.002%
57	7.944	2132	2147	2155	rBV2	4600	7745	0.41%	0.053%
58	8.095	2182	2194	2228	rBV2	331097	721651	37.94%	4.930%
59	8.413	2290	2293	2296	rVB3	255	163	0.01%	0.001%
60	8.471	2307	2311	2315	rBV2	349	378	0.02%	0.003%
61	8.632	2358	2361	2366	rVB3	325	184	0.01%	0.001%
62	8.857	2418	2431	2462	rBV	847837	1395294	73.35%	9.532%
63	9.554	2645	2648	2655	rBV2	203	218	0.01%	0.001%
64	9.587	2655	2658	2662	rVB2	315	187	0.01%	0.001%
65	9.741	2703	2706	2709	rBV2	212	155	0.01%	0.001%
66	9.841	2731	2737	2740	rBV2	225	240	0.01%	0.002%
67	10.082	2808	2812	2820	rBV2	300	498	0.03%	0.003%
68	10.114	2820	2822	2827	rVB2	246	187	0.01%	0.001%
69	10.140	2827	2830	2836	rBV	225	206	0.01%	0.001%
70	10.220	2843	2855	2882	rVV	474711	742865	39.05%	5.075%
71	10.390	2898	2908	2917	rBV2	6509	10252	0.54%	0.070%
72	10.545	2952	2956	2963	rVB3	751	762	0.04%	0.005%
73	10.860	3050	3054	3056	rBV2	411	289	0.02%	0.002%
74	10.902	3062	3067	3070	rBV2	249	245	0.01%	0.002%
75	10.976	3087	3090	3092	rBV2	215	167	0.01%	0.001%
76	11.255	3165	3177	3202	rBV	920071	1410898	74.17%	9.639%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020500.D
 Acq On : 10 Mar 2021 17:07
 Operator : SY/MD
 Sample : M1610-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG506

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	11.542	3264	3266	3269	rBV	322	152	0.01%	0.001%
78	11.632	3281	3294	3314	rBV	1021189	1592925	83.74%	10.882%
79	11.847	3357	3361	3365	rVV2	250	203	0.01%	0.001%
80	11.879	3368	3371	3375	rVB	270	198	0.01%	0.001%
81	12.037	3418	3420	3424	rVB2	384	212	0.01%	0.001%
82	12.223	3475	3478	3483	rVB3	300	244	0.01%	0.002%
83	12.259	3483	3489	3498	rBV4	1047	1666	0.09%	0.011%
84	12.394	3529	3531	3535	rBV2	260	159	0.01%	0.001%
85	12.477	3554	3557	3561	rBV2	338	295	0.02%	0.002%
86	12.622	3598	3602	3605	rBV2	319	227	0.01%	0.002%
87	12.657	3608	3613	3620	rBV3	639	975	0.05%	0.007%
88	12.715	3626	3631	3633	rBV2	372	316	0.02%	0.002%
89	13.014	3721	3724	3726	rBV	292	154	0.01%	0.001%
90	13.088	3744	3747	3751	rVB2	306	256	0.01%	0.002%
91	13.233	3789	3792	3799	rBV3	327	478	0.03%	0.003%
92	13.271	3800	3804	3813	rVB4	1336	1683	0.09%	0.011%
93	13.522	3874	3882	3886	rBV3	877	1362	0.07%	0.009%
94	13.750	3950	3953	3954	rBV2	438	270	0.01%	0.002%
95	13.824	3974	3976	3982	rVB3	409	289	0.02%	0.002%
96	14.004	4030	4032	4038	rVB3	480	308	0.02%	0.002%
97	14.918	4314	4316	4319	rBV3	421	233	0.01%	0.002%
98	15.120	4376	4379	4383	rBV2	586	513	0.03%	0.004%
99	15.191	4397	4401	4402	rBV2	689	484	0.03%	0.003%
100	15.303	4434	4436	4439	rBV2	771	509	0.03%	0.003%




Sum of corrected areas: 14637612

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020500.D
Acq On : 10 Mar 2021 17:07
Operator : SY/MD
Sample : M1610-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG506

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

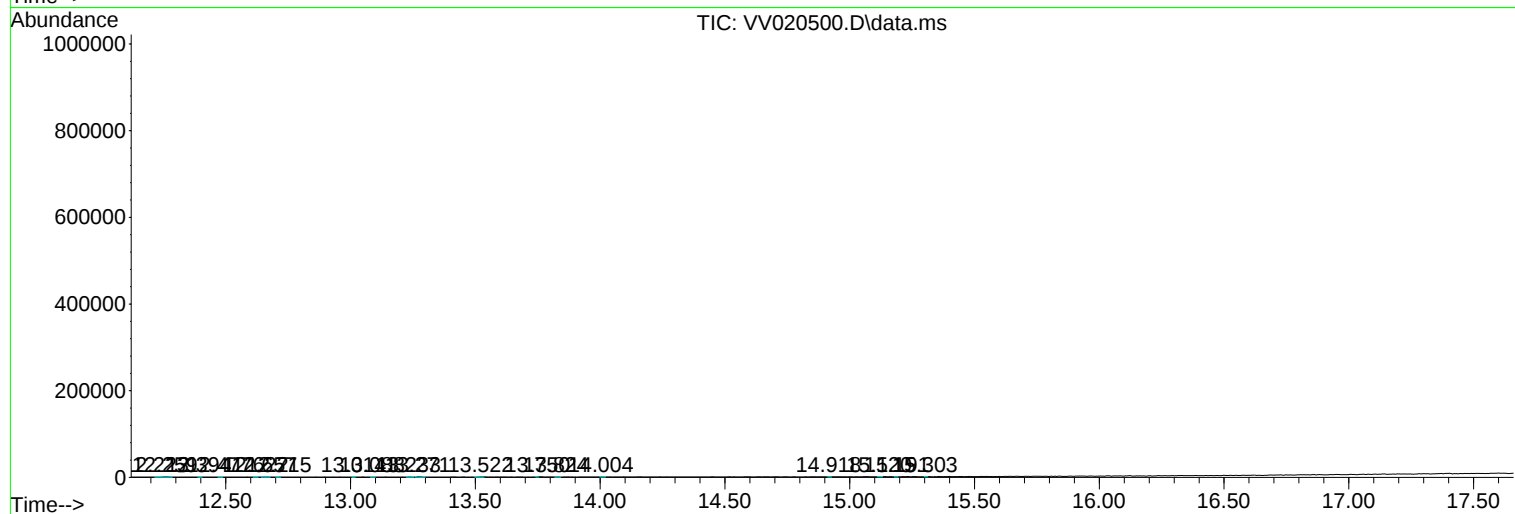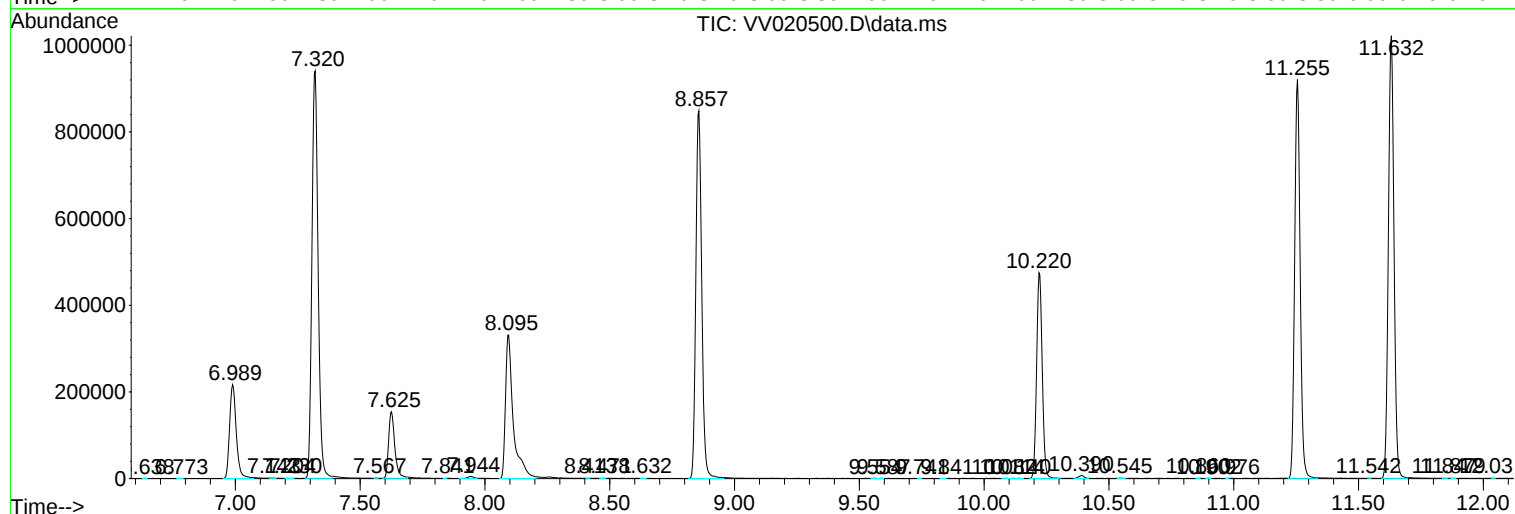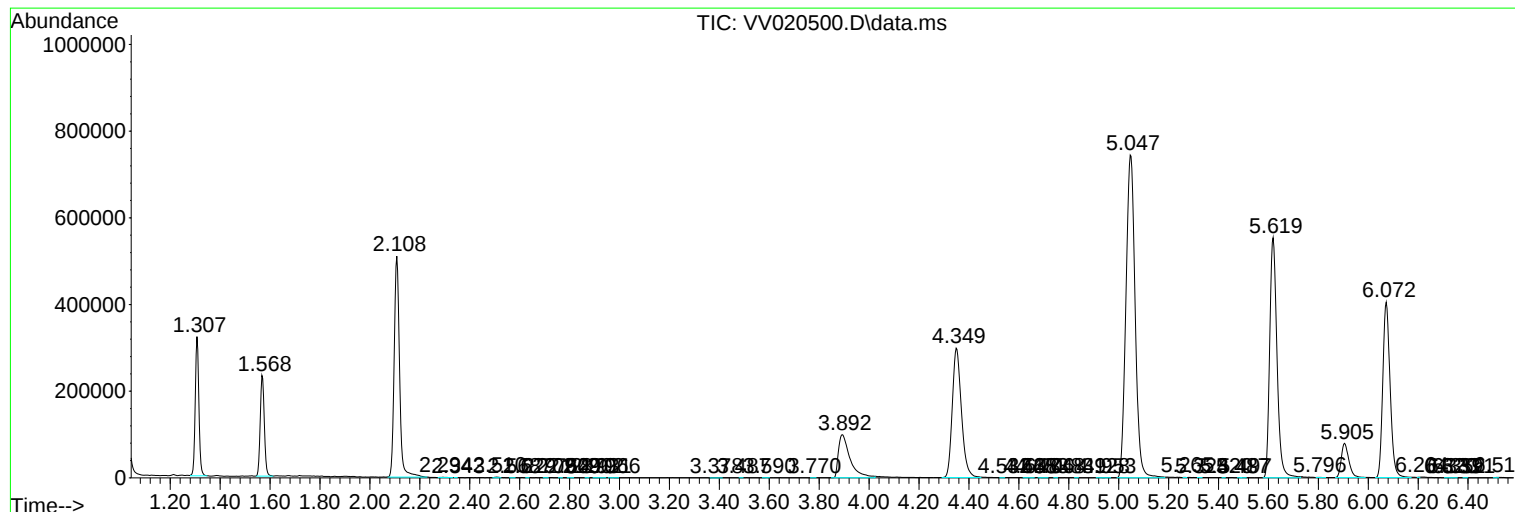

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020500.D
Acq On : 10 Mar 2021 17:07
Operator : SY/MD
Sample : M1610-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG506

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020500.D
Acq On : 10 Mar 2021 17:07
Operator : SY/MD
Sample : M1610-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG506

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
