

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031121\
 Data File : VW020502.D
 Acq On : 10 Mar 2021 17:54
 Operator : SY/MD
 Sample : M1610-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VW020502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	51	54	62	rVB3	6756	6539	0.33%	0.043%
2	1.307	75	83	99	rVB	329690	334185	17.02%	2.204%
3	1.571	156	165	180	rBV	245392	279207	14.22%	1.842%
4	2.108	319	332	374	rVB	523945	792749	40.38%	5.229%
5	2.288	383	388	391	rBV3	529	417	0.02%	0.003%
6	2.468	442	444	447	rVB2	361	201	0.01%	0.001%
7	2.513	447	458	465	rBV4	1473	2294	0.12%	0.015%
8	2.873	564	570	572	rBV	263	167	0.01%	0.001%
9	3.088	631	637	640	rVB	216	212	0.01%	0.001%
10	3.214	672	676	679	rVB	323	202	0.01%	0.001%
11	3.558	776	783	785	rBV2	211	178	0.01%	0.001%
12	3.593	789	794	800	rVB2	158	184	0.01%	0.001%
13	3.638	800	808	809	rBV2	147	177	0.01%	0.001%
14	3.892	876	887	926	rBV	109879	344466	17.54%	2.272%
15	4.236	991	994	998	rBB2	288	219	0.01%	0.001%
16	4.352	1013	1030	1060	rBV	307249	776900	39.57%	5.125%
17	4.584	1100	1102	1109	rVB4	422	465	0.02%	0.003%
18	4.629	1109	1116	1119	rBV3	338	534	0.03%	0.004%
19	4.757	1150	1156	1159	rVV2	231	208	0.01%	0.001%
20	4.802	1166	1170	1173	rBV3	238	192	0.01%	0.001%
21	4.867	1183	1190	1194	rBV2	152	198	0.01%	0.001%
22	4.957	1211	1218	1222	rBV2	165	188	0.01%	0.001%
23	5.050	1224	1247	1284	rBV2	770604	1963337	100.00%	12.951%
24	5.410	1355	1359	1366	rVB4	501	612	0.03%	0.004%
25	5.445	1366	1370	1375	rVB3	530	411	0.02%	0.003%
26	5.622	1411	1425	1459	rBV	580071	1164345	59.30%	7.681%
27	5.908	1502	1514	1540	rBV	82657	170013	8.66%	1.121%
28	6.075	1552	1566	1600	rBV	417581	846019	43.09%	5.581%
29	6.281	1627	1630	1633	rVB3	626	413	0.02%	0.003%
30	6.307	1636	1638	1640	rVV	299	174	0.01%	0.001%
31	6.352	1648	1652	1656	rVB	304	235	0.01%	0.002%
32	6.487	1690	1694	1699	rBV2	162	175	0.01%	0.001%
33	6.571	1715	1720	1721	rBV2	534	321	0.02%	0.002%
34	6.741	1770	1773	1780	rVB2	251	230	0.01%	0.002%
35	6.873	1811	1814	1818	rVB2	297	198	0.01%	0.001%
36	6.989	1838	1850	1882	rBV	227707	414879	21.13%	2.737%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020502.D
 Acq On : 10 Mar 2021 17:54
 Operator : SY/MD
 Sample : M1610-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	7.320	1939	1953	1984	rBV	979270	1680679	85.60%	11.087%
38	7.625	2038	2048	2081	rBV	158841	278807	14.20%	1.839%
39	7.818	2105	2108	2112	rVB2	305	183	0.01%	0.001%
40	7.879	2123	2127	2130	rBV2	259	190	0.01%	0.001%
41	7.937	2138	2145	2146	rBV2	1054	730	0.04%	0.005%
42	7.989	2155	2161	2166	rVB5	751	996	0.05%	0.007%
43	8.095	2183	2194	2229	rBV2	371231	791860	40.33%	5.223%
44	8.397	2285	2288	2292	rBV3	353	294	0.01%	0.002%
45	8.506	2319	2322	2328	rVV3	397	444	0.02%	0.003%
46	8.577	2338	2344	2346	rBV2	229	191	0.01%	0.001%
47	8.628	2355	2360	2363	rBV3	260	244	0.01%	0.002%
48	8.857	2419	2431	2456	rBV	894864	1439887	73.34%	9.498%
49	9.075	2498	2499	2503	rVB	324	210	0.01%	0.001%
50	9.101	2503	2507	2510	rBV2	283	277	0.01%	0.002%
51	9.152	2518	2523	2524	rBV2	272	235	0.01%	0.002%
52	9.185	2528	2533	2535	rBV2	254	198	0.01%	0.001%
53	9.567	2647	2652	2654	rBV2	263	272	0.01%	0.002%
54	9.616	2662	2667	2670	rBV2	304	225	0.01%	0.001%
55	9.886	2747	2751	2755	rBV2	264	188	0.01%	0.001%
56	10.181	2838	2843	2844	rBV	295	178	0.01%	0.001%
57	10.223	2844	2856	2873	rBV	498807	780317	39.74%	5.147%
58	10.326	2885	2888	2894	rVB2	576	519	0.03%	0.003%
59	10.390	2898	2908	2920	rVB4	2012	3174	0.16%	0.021%
60	10.439	2920	2923	2931	rVB2	180	231	0.01%	0.002%
61	10.542	2953	2955	2957	rBV	437	254	0.01%	0.002%
62	10.612	2973	2977	2980	rVB2	219	171	0.01%	0.001%
63	10.895	3062	3065	3070	rBV2	313	340	0.02%	0.002%
64	10.956	3082	3084	3091	rVB	395	337	0.02%	0.002%
65	11.069	3112	3119	3122	rBV	463	437	0.02%	0.003%
66	11.181	3150	3154	3157	rVV3	369	291	0.01%	0.002%
67	11.255	3165	3177	3208	rBV	952910	1434167	73.05%	9.460%
68	11.477	3242	3246	3248	rBV2	242	195	0.01%	0.001%
69	11.490	3248	3250	3256	rVB3	396	282	0.01%	0.002%
70	11.535	3260	3264	3267	rBV3	354	263	0.01%	0.002%
71	11.558	3267	3271	3273	rBV3	300	227	0.01%	0.001%
72	11.632	3281	3294	3322	rBV	1060892	1632430	83.15%	10.768%
73	11.837	3353	3358	3360	rBV3	394	358	0.02%	0.002%
74	11.850	3360	3362	3370	rVB3	498	423	0.02%	0.003%
75	11.886	3370	3373	3376	rBV	348	229	0.01%	0.002%
76	12.004	3407	3410	3415	rVB4	369	293	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020502.D
 Acq On : 10 Mar 2021 17:54
 Operator : SY/MD
 Sample : M1610-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	12.255	3484	3488	3490	rBV3	248	212	0.01%	0.001%
78	12.496	3561	3563	3567	rBV2	279	226	0.01%	0.001%
79	12.654	3610	3612	3613	rBV	429	176	0.01%	0.001%
80	12.747	3635	3641	3643	rBV	271	293	0.01%	0.002%
81	12.786	3649	3653	3655	rBV2	233	199	0.01%	0.001%
82	12.921	3693	3695	3698	rVB	377	174	0.01%	0.001%
83	12.947	3698	3703	3706	rBV2	267	276	0.01%	0.002%
84	12.992	3714	3717	3722	rVB2	333	249	0.01%	0.002%
85	13.078	3739	3744	3747	rBV2	305	327	0.02%	0.002%
86	13.146	3761	3765	3767	rBV2	201	176	0.01%	0.001%
87	13.275	3800	3805	3806	rBV2	660	463	0.02%	0.003%
88	13.365	3830	3833	3835	rBV	437	318	0.02%	0.002%
89	13.406	3841	3846	3850	rBV3	341	441	0.02%	0.003%
90	13.439	3853	3856	3857	rBV2	302	203	0.01%	0.001%
91	13.567	3893	3896	3898	rBV3	345	208	0.01%	0.001%
92	13.593	3901	3904	3906	rBV2	253	181	0.01%	0.001%
93	13.808	3969	3971	3974	rBV2	216	178	0.01%	0.001%
94	14.226	4097	4101	4105	rBV2	477	482	0.02%	0.003%
95	14.268	4111	4114	4119	rVB	572	349	0.02%	0.002%
96	14.397	4151	4154	4157	rBV	334	271	0.01%	0.002%
97	15.136	4382	4384	4386	rBV	481	218	0.01%	0.001%
98	15.249	4416	4419	4422	rBV	499	421	0.02%	0.003%
99	15.647	4541	4543	4548	rVB3	998	593	0.03%	0.004%
100	15.673	4549	4551	4554	rVV3	610	307	0.02%	0.002%




Sum of corrected areas: 15159611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020502.D
Acq On : 10 Mar 2021 17:54
Operator : SY/MD
Sample : M1610-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

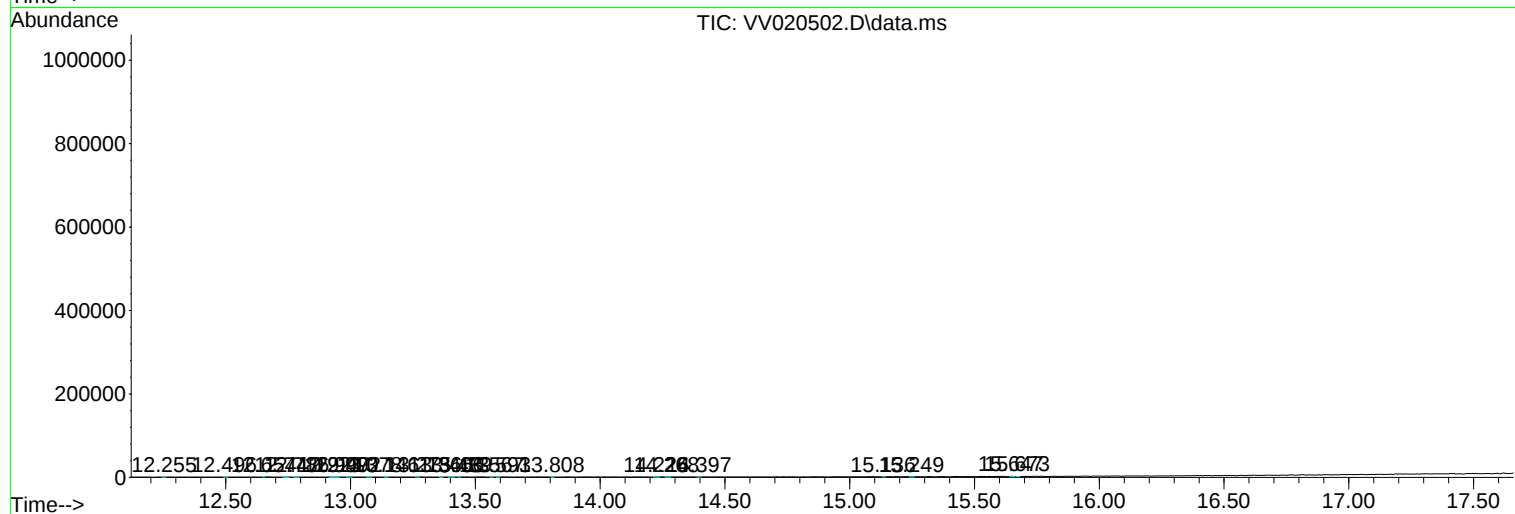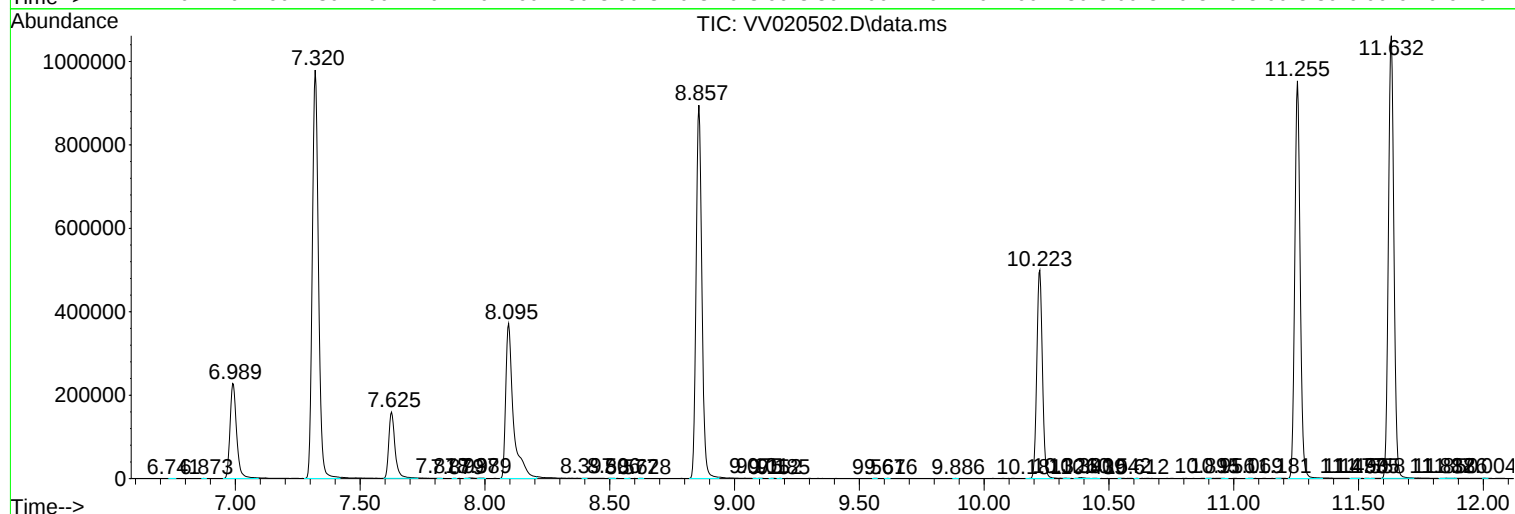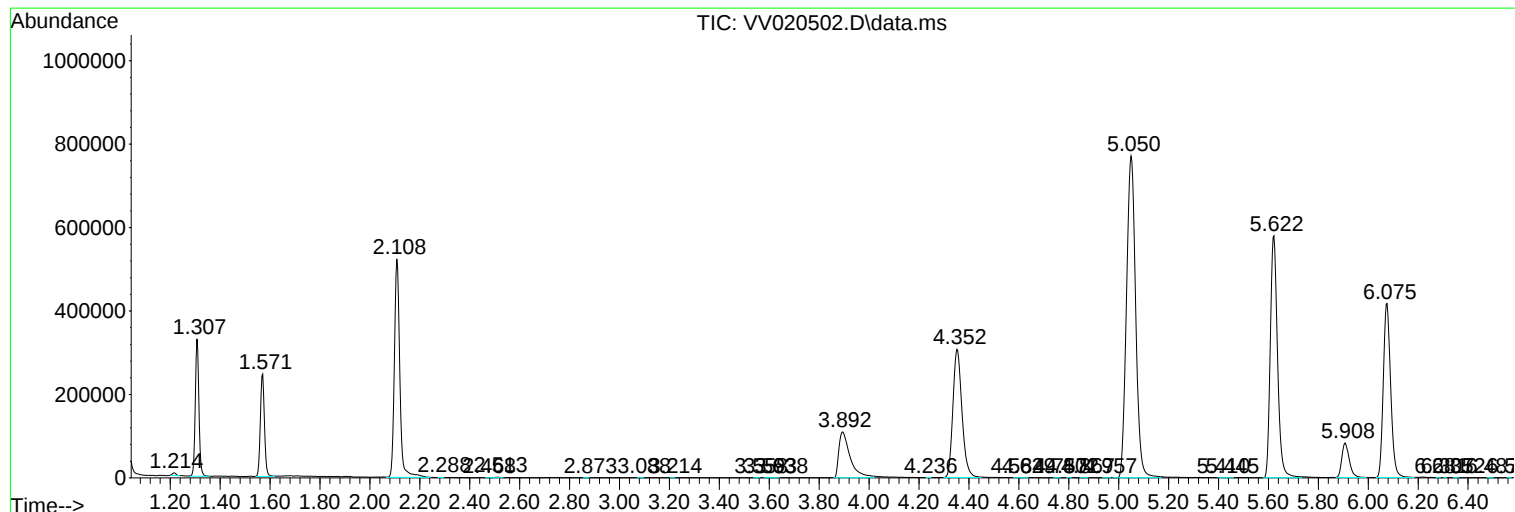

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020502.D
Acq On : 10 Mar 2021 17:54
Operator : SY/MD
Sample : M1610-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020502.D
Acq On : 10 Mar 2021 17:54
Operator : SY/MD
Sample : M1610-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
