

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020505.D
 Acq On : 10 Mar 2021 19:05
 Operator : SY/MD
 Sample : M1632-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	47	51	58	rVB2	21924	19841	1.03%	0.134%
2	1.307	77	83	102	rVB	321456	322040	16.76%	2.178%
3	1.568	157	164	182	rVB	242381	274159	14.27%	1.854%
4	2.108	321	332	364	rVB	513818	761417	39.62%	5.149%
5	2.667	504	506	508	rBV2	269	174	0.01%	0.001%
6	2.712	516	520	525	rBV2	232	235	0.01%	0.002%
7	2.812	547	551	554	rBV2	249	232	0.01%	0.002%
8	2.851	559	563	567	rBV3	211	238	0.01%	0.002%
9	2.896	574	577	579	rBV2	214	121	0.01%	0.001%
10	2.944	590	592	594	rVB2	167	36	0.00%	0.000%
11	3.008	608	612	614	rBV	242	142	0.01%	0.001%
12	3.047	621	624	626	rBV	116	64	0.00%	0.000%
13	3.146	653	655	658	rVB	188	103	0.01%	0.001%
14	3.166	659	661	663	rVB	204	88	0.00%	0.001%
15	3.355	718	720	725	rVB2	135	76	0.00%	0.001%
16	3.381	725	728	730	rBV	108	62	0.00%	0.000%
17	3.397	730	733	735	rBV	100	57	0.00%	0.000%
18	3.445	745	748	750	rBV	136	99	0.01%	0.001%
19	3.519	769	771	775	rVB	214	130	0.01%	0.001%
20	3.548	777	780	783	rVB2	131	76	0.00%	0.001%
21	3.596	793	795	800	rVB	187	115	0.01%	0.001%
22	3.683	814	822	826	rBV	177	204	0.01%	0.001%
23	3.706	826	829	834	rBV2	190	141	0.01%	0.001%
24	3.732	834	837	839	rBV	88	48	0.00%	0.000%
25	3.764	844	847	850	rBV2	75	49	0.00%	0.000%
26	3.783	850	853	856	rBV	266	171	0.01%	0.001%
27	3.825	863	866	869	rBV	95	70	0.00%	0.000%
28	3.857	873	876	877	rBV	78	38	0.00%	0.000%
29	3.895	877	888	919	rBV	106466	344348	17.92%	2.328%
30	4.352	1012	1030	1061	rBV	303234	763865	39.75%	5.165%
31	4.619	1111	1113	1114	rBV	258	64	0.00%	0.000%
32	4.645	1119	1121	1124	rVB3	393	215	0.01%	0.001%
33	4.712	1138	1142	1145	rBV2	390	317	0.02%	0.002%
34	4.738	1148	1150	1154	rVB2	150	91	0.00%	0.001%
35	4.770	1154	1160	1161	rBV2	363	263	0.01%	0.002%
36	4.812	1170	1173	1174	rBV	192	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031121\
 Data File : VW020505.D
 Acq On : 10 Mar 2021 19:05
 Operator : SY/MD
 Sample : M1632-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	4.847	1182	1184	1187	rVB	75	40	0.00%	0.000%
38	4.870	1187	1191	1194	rBV	98	72	0.00%	0.000%
39	4.892	1194	1198	1201	rBV2	91	83	0.00%	0.001%
40	5.050	1230	1247	1282	rBV2	756776	1921681	100.00%	12.994%
41	5.420	1357	1362	1367	rVB4	449	527	0.03%	0.004%
42	5.487	1377	1383	1389	rBV2	431	645	0.03%	0.004%
43	5.622	1412	1425	1450	rBV	562431	1127432	58.67%	7.623%
44	5.908	1503	1514	1535	rBV	57608	117508	6.11%	0.795%
45	6.072	1552	1565	1593	rBV	405355	827250	43.05%	5.594%
46	6.297	1632	1635	1636	rBV	161	76	0.00%	0.001%
47	6.342	1647	1649	1654	rBV	281	222	0.01%	0.002%
48	6.365	1654	1656	1658	rVV	102	63	0.00%	0.000%
49	6.381	1659	1661	1664	rVV2	261	129	0.01%	0.001%
50	6.397	1664	1666	1667	rVV	85	40	0.00%	0.000%
51	6.410	1667	1670	1673	rVB	188	118	0.01%	0.001%
52	6.429	1673	1676	1679	rBV2	157	119	0.01%	0.001%
53	6.538	1703	1710	1712	rBV2	288	295	0.02%	0.002%
54	6.577	1721	1722	1723	rVB2	100	19	0.00%	0.000%
55	6.590	1723	1726	1728	rBV	112	62	0.00%	0.000%
56	6.606	1728	1731	1736	rVB2	151	130	0.01%	0.001%
57	6.628	1736	1738	1740	rBV	113	59	0.00%	0.000%
58	6.696	1758	1759	1760	rBV	111	35	0.00%	0.000%
59	6.786	1784	1787	1789	rBV2	184	103	0.01%	0.001%
60	6.825	1796	1799	1800	rBV2	106	62	0.00%	0.000%
61	6.892	1817	1820	1821	rBV	137	81	0.00%	0.001%
62	6.921	1825	1829	1833	rBV2	151	125	0.01%	0.001%
63	6.989	1839	1850	1871	rBV	217896	397832	20.70%	2.690%
64	7.201	1912	1916	1917	rBV	304	187	0.01%	0.001%
65	7.233	1923	1926	1934	rBV2	330	434	0.02%	0.003%
66	7.320	1940	1953	1985	rBV	957301	1643071	85.50%	11.110%
67	7.625	2038	2048	2069	rBV	156560	267235	13.91%	1.807%
68	7.844	2112	2116	2117	rBV2	243	136	0.01%	0.001%
69	7.879	2124	2127	2128	rBV2	125	57	0.00%	0.000%
70	7.947	2139	2148	2155	rBV3	944	1382	0.07%	0.009%
71	8.005	2163	2166	2168	rBV	131	97	0.01%	0.001%
72	8.095	2183	2194	2228	rBV2	383245	771384	40.14%	5.216%
73	8.567	2337	2341	2343	rBV	212	184	0.01%	0.001%
74	8.638	2361	2363	2366	rBV	212	110	0.01%	0.001%
75	8.792	2407	2411	2412	rBV	198	136	0.01%	0.001%
76	8.857	2419	2431	2455	rBV	876295	1402527	72.98%	9.484%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020505.D
 Acq On : 10 Mar 2021 19:05
 Operator : SY/MD
 Sample : M1632-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	9.143	2516	2520	2524	rBV2	426	412	0.02%	0.003%
78	9.181	2530	2532	2534	rBV2	195	100	0.01%	0.001%
79	9.255	2550	2555	2557	rBV2	287	229	0.01%	0.002%
80	9.339	2579	2581	2582	rBV2	168	82	0.00%	0.001%
81	9.513	2633	2635	2638	rBV2	284	138	0.01%	0.001%
82	9.728	2701	2702	2703	rVB	233	45	0.00%	0.000%
83	9.744	2705	2707	2711	rVB	213	103	0.01%	0.001%
84	10.223	2843	2856	2876	rBV	521356	825343	42.95%	5.581%
85	10.342	2890	2893	2895	rBV	273	158	0.01%	0.001%
86	10.397	2903	2910	2917	rVB3	1180	1707	0.09%	0.012%
87	10.448	2923	2926	2931	rBV2	205	165	0.01%	0.001%
88	10.860	3052	3054	3055	rBV	211	60	0.00%	0.000%
89	11.255	3165	3177	3199	rBV	912701	1394528	72.57%	9.429%
90	11.442	3233	3235	3236	rBV2	379	152	0.01%	0.001%
91	11.632	3281	3294	3317	rBV	1017214	1593835	82.94%	10.777%
92	11.812	3347	3350	3354	rBV2	475	406	0.02%	0.003%
93	12.905	3687	3690	3694	rBV	393	294	0.02%	0.002%




Sum of corrected areas: 14789004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020505.D
Acq On : 10 Mar 2021 19:05
Operator : SY/MD
Sample : M1632-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

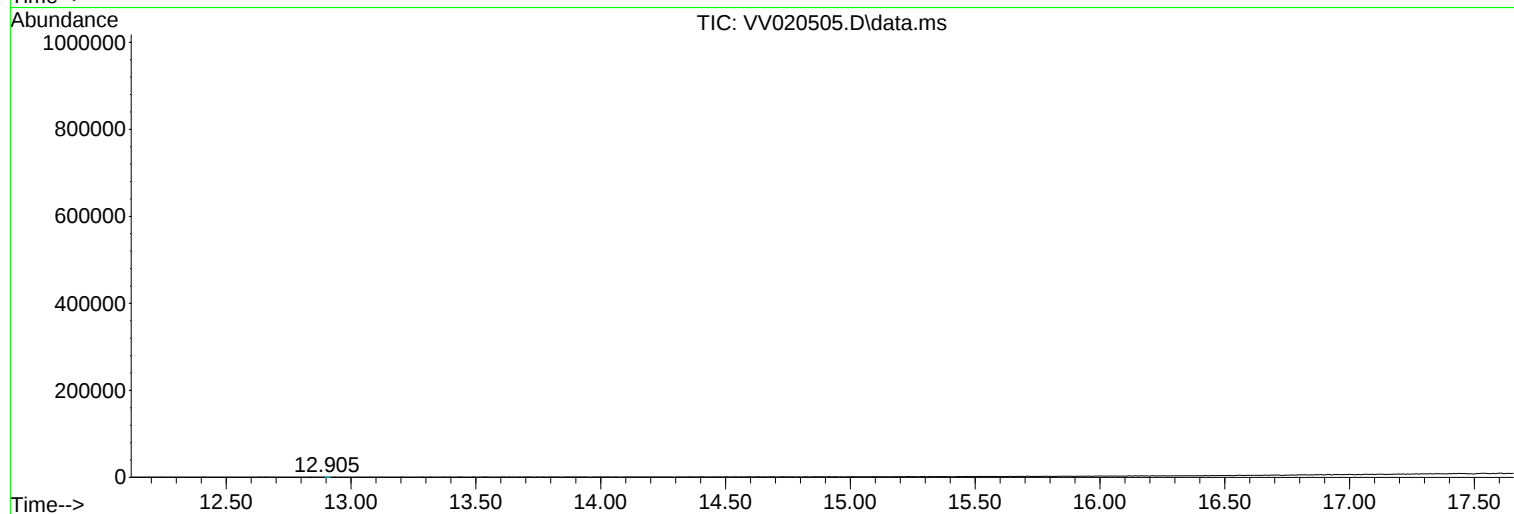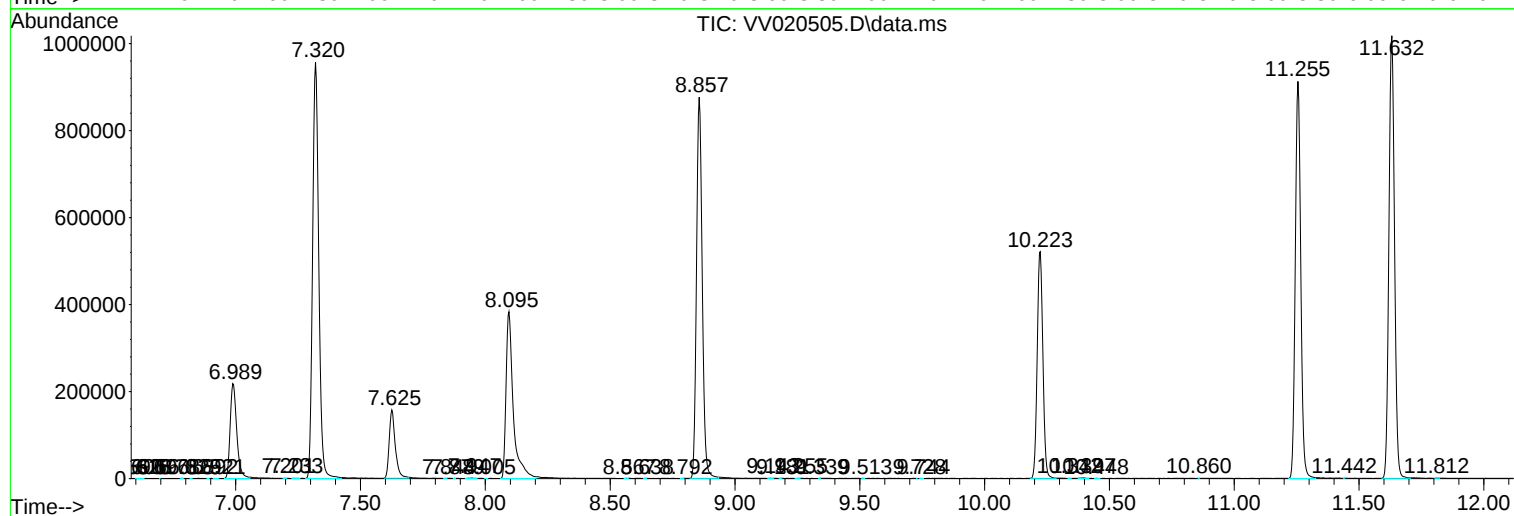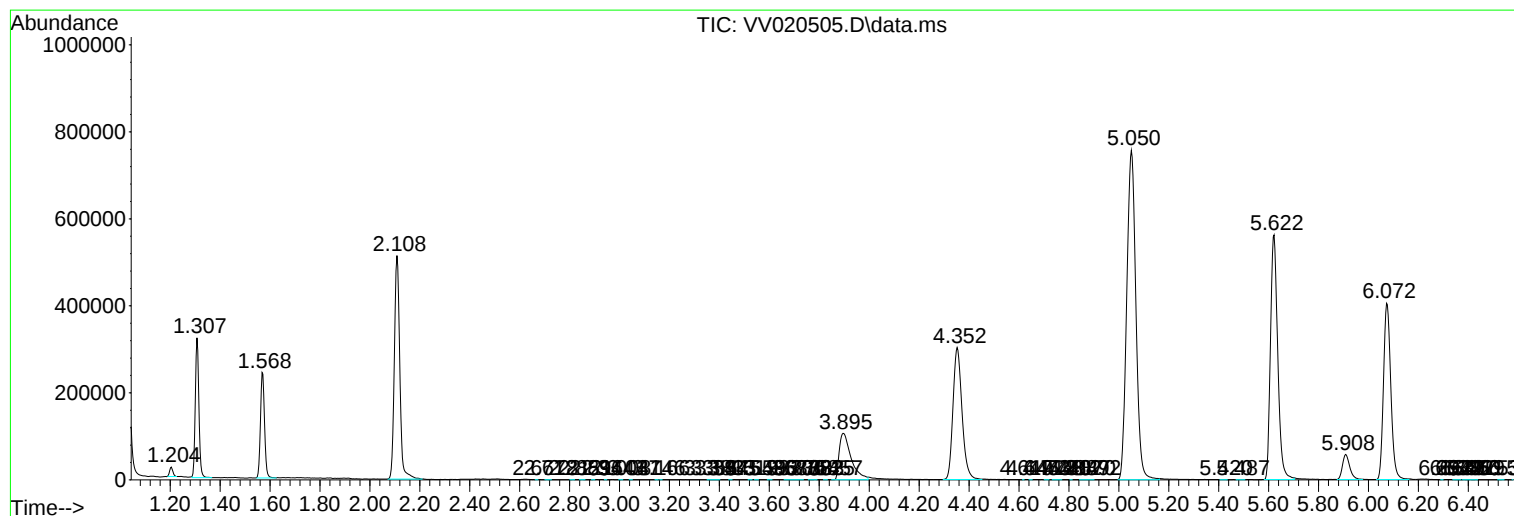

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020505.D
Acq On : 10 Mar 2021 19:05
Operator : SY/MD
Sample : M1632-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020505.D
Acq On : 10 Mar 2021 19:05
Operator : SY/MD
Sample : M1632-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
