

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020507.D
 Acq On : 10 Mar 2021 19:52
 Operator : SY/MD
 Sample : M1632-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020507.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	312138	314036	16.76%	2.162%
2	1.568	157	164	177	rVB	231175	261836	13.97%	1.803%
3	2.108	321	332	382	rVB	505953	770517	41.12%	5.305%
4	2.291	386	389	392	rBV2	247	209	0.01%	0.001%
5	2.513	451	458	465	rBV5	1087	1725	0.09%	0.012%
6	2.565	472	474	476	rBV2	247	171	0.01%	0.001%
7	2.613	483	489	497	rBV2	327	445	0.02%	0.003%
8	2.667	501	506	512	rBV2	188	233	0.01%	0.002%
9	2.812	545	551	554	rVV2	303	291	0.02%	0.002%
10	2.873	565	570	575	rBV2	205	201	0.01%	0.001%
11	2.976	599	602	607	rVB2	303	274	0.01%	0.002%
12	3.005	607	611	612	rBV	324	271	0.01%	0.002%
13	3.040	620	622	627	rVB2	264	191	0.01%	0.001%
14	3.069	627	631	638	rBV	255	301	0.02%	0.002%
15	3.166	657	661	666	rBV2	188	202	0.01%	0.001%
16	3.304	696	704	708	rBV2	185	224	0.01%	0.002%
17	3.401	729	734	737	rBV2	263	245	0.01%	0.002%
18	3.436	742	745	749	rBV2	221	172	0.01%	0.001%
19	3.597	791	795	798	rBV2	221	171	0.01%	0.001%
20	3.854	870	875	878	rBV2	170	160	0.01%	0.001%
21	3.899	878	889	926	rBV	98278	330158	17.62%	2.273%
22	4.288	1006	1010	1013	rBV2	280	301	0.02%	0.002%
23	4.352	1013	1030	1063	rVV	293016	738090	39.39%	5.082%
24	4.609	1099	1110	1122	rBV6	2771	6110	0.33%	0.042%
25	5.050	1229	1247	1292	rBV2	736090	1873933	100.00%	12.903%
26	5.246	1304	1308	1317	rVB3	592	738	0.04%	0.005%
27	5.423	1361	1363	1367	rBV2	239	158	0.01%	0.001%
28	5.490	1381	1384	1386	rBV2	313	213	0.01%	0.001%
29	5.619	1411	1424	1462	rBV	557878	1134032	60.52%	7.808%
30	5.863	1498	1500	1503	rVV3	325	172	0.01%	0.001%
31	5.912	1503	1515	1540	rVV5	66734	151208	8.07%	1.041%
32	5.998	1540	1542	1545	rVB	604	297	0.02%	0.002%
33	6.027	1548	1551	1552	rBV	349	190	0.01%	0.001%
34	6.072	1552	1565	1594	rBV	397013	802627	42.83%	5.527%
35	6.256	1620	1622	1626	rVB2	356	179	0.01%	0.001%
36	6.314	1638	1640	1644	rVB2	297	192	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020507.D
 Acq On : 10 Mar 2021 19:52
 Operator : SY/MD
 Sample : M1632-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.346	1647	1650	1655	rBV3	428	360	0.02%	0.002%
38	6.670	1747	1751	1754	rBV2	207	195	0.01%	0.001%
39	6.719	1760	1766	1769	rBV2	208	205	0.01%	0.001%
40	6.770	1779	1782	1787	rVB2	255	239	0.01%	0.002%

41	6.989	1839	1850	1878	rBV	210893	386290	20.61%	2.660%
42	7.249	1928	1931	1936	rVB3	327	359	0.02%	0.002%
43	7.320	1940	1953	1989	rBV	918941	1592224	84.97%	10.963%
44	7.625	2037	2048	2071	rBV	149938	258354	13.79%	1.779%
45	7.796	2099	2101	2104	rBV	283	157	0.01%	0.001%

46	7.844	2113	2116	2118	rBV3	262	182	0.01%	0.001%
47	7.937	2140	2145	2146	rBV2	310	257	0.01%	0.002%
48	7.947	2146	2148	2155	rVV	515	622	0.03%	0.004%
49	7.995	2158	2163	2164	rVV2	310	246	0.01%	0.002%
50	8.095	2183	2194	2235	rBV2	356063	739348	39.45%	5.091%

51	8.304	2257	2259	2266	rVB4	778	801	0.04%	0.006%
52	8.500	2316	2320	2323	rBV2	248	210	0.01%	0.001%
53	8.603	2350	2352	2356	rBV2	254	180	0.01%	0.001%
54	8.625	2356	2359	2365	rVB3	303	243	0.01%	0.002%
55	8.667	2370	2372	2377	rBV	232	175	0.01%	0.001%

56	8.731	2388	2392	2396	rBV2	282	199	0.01%	0.001%
57	8.857	2418	2431	2452	rBV	883007	1404530	74.95%	9.671%
58	9.130	2513	2516	2519	rBV2	231	181	0.01%	0.001%
59	9.243	2549	2551	2555	rVB3	304	204	0.01%	0.001%
60	9.397	2595	2599	2601	rBV2	258	192	0.01%	0.001%

61	9.548	2641	2646	2649	rBV2	179	183	0.01%	0.001%
62	9.587	2655	2658	2664	rVB2	228	221	0.01%	0.002%
63	9.648	2670	2677	2683	rVB2	266	362	0.02%	0.002%
64	9.895	2751	2754	2759	rVV2	205	182	0.01%	0.001%
65	9.944	2765	2769	2772	rBV	244	176	0.01%	0.001%

66	10.050	2799	2802	2807	rVB2	215	157	0.01%	0.001%
67	10.223	2843	2856	2885	rBV	500449	792732	42.30%	5.458%
68	10.378	2902	2904	2906	rVV	340	224	0.01%	0.002%
69	10.397	2906	2910	2914	rVB2	784	618	0.03%	0.004%
70	10.722	3008	3011	3017	rBV2	215	226	0.01%	0.002%

71	10.857	3049	3053	3059	rBV	269	391	0.02%	0.003%
72	11.069	3116	3119	3123	rBV2	261	221	0.01%	0.002%
73	11.104	3127	3130	3134	rBV	213	224	0.01%	0.002%
74	11.175	3148	3152	3160	rBV3	330	354	0.02%	0.002%
75	11.256	3165	3177	3202	rBV	912882	1387916	74.06%	9.557%

76	11.580	3273	3278	3281	rBV3	213	235	0.01%	0.002%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020507.D
 Acq On : 10 Mar 2021 19:52
 Operator : SY/MD
 Sample : M1632-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.632	3281	3294	3320	rBV	981494	1544243	82.41%	10.633%
78	11.944	3388	3391	3394	rVV	264	163	0.01%	0.001%
79	11.989	3401	3405	3408	rBV3	274	232	0.01%	0.002%
80	12.387	3525	3529	3531	rBV2	256	199	0.01%	0.001%
81	12.436	3539	3544	3550	rBV3	359	465	0.02%	0.003%
82	12.590	3590	3592	3595	rVB	321	197	0.01%	0.001%
83	12.612	3595	3599	3600	rBV	312	198	0.01%	0.001%
84	12.715	3627	3631	3633	rBV	208	185	0.01%	0.001%
85	12.918	3685	3694	3697	rBV2	296	506	0.03%	0.003%
86	13.037	3727	3731	3733	rBV	397	298	0.02%	0.002%
87	13.056	3735	3737	3741	rVB	313	208	0.01%	0.001%
88	13.194	3773	3780	3783	rBV3	385	520	0.03%	0.004%
89	13.220	3786	3788	3791	rBV	220	171	0.01%	0.001%
90	13.281	3804	3807	3811	rVV3	336	293	0.02%	0.002%
91	13.416	3845	3849	3853	rBV2	319	310	0.02%	0.002%
92	13.484	3867	3870	3873	rBV2	411	342	0.02%	0.002%
93	13.583	3898	3901	3904	rBV	280	209	0.01%	0.001%
94	13.689	3930	3934	3936	rBV	317	234	0.01%	0.002%
95	13.722	3941	3944	3947	rBV2	255	203	0.01%	0.001%
96	13.908	4000	4002	4003	rBV	383	190	0.01%	0.001%
97	14.014	4032	4035	4039	rBV2	334	301	0.02%	0.002%
98	14.683	4240	4243	4246	rBV2	410	325	0.02%	0.002%
99	15.837	4600	4602	4610	rBV6	811	810	0.04%	0.006%
100	15.966	4638	4642	4653	rVB	16164	11490	0.61%	0.079%




Sum of corrected areas: 14523140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020507.D
Acq On : 10 Mar 2021 19:52
Operator : SY/MD
Sample : M1632-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

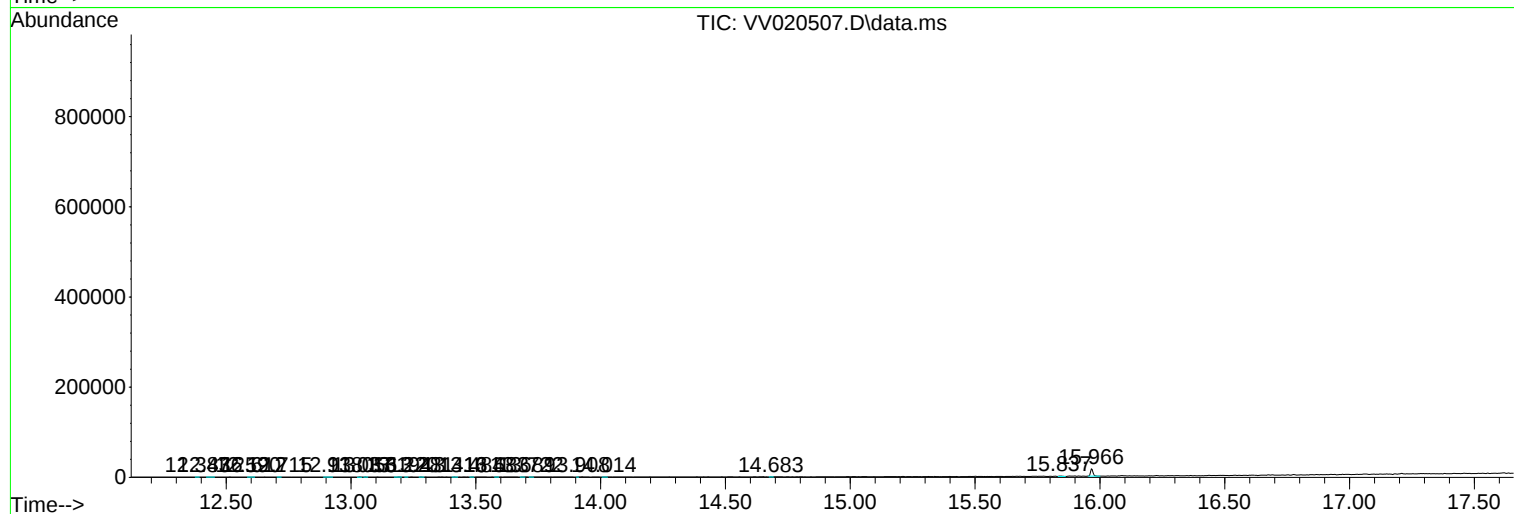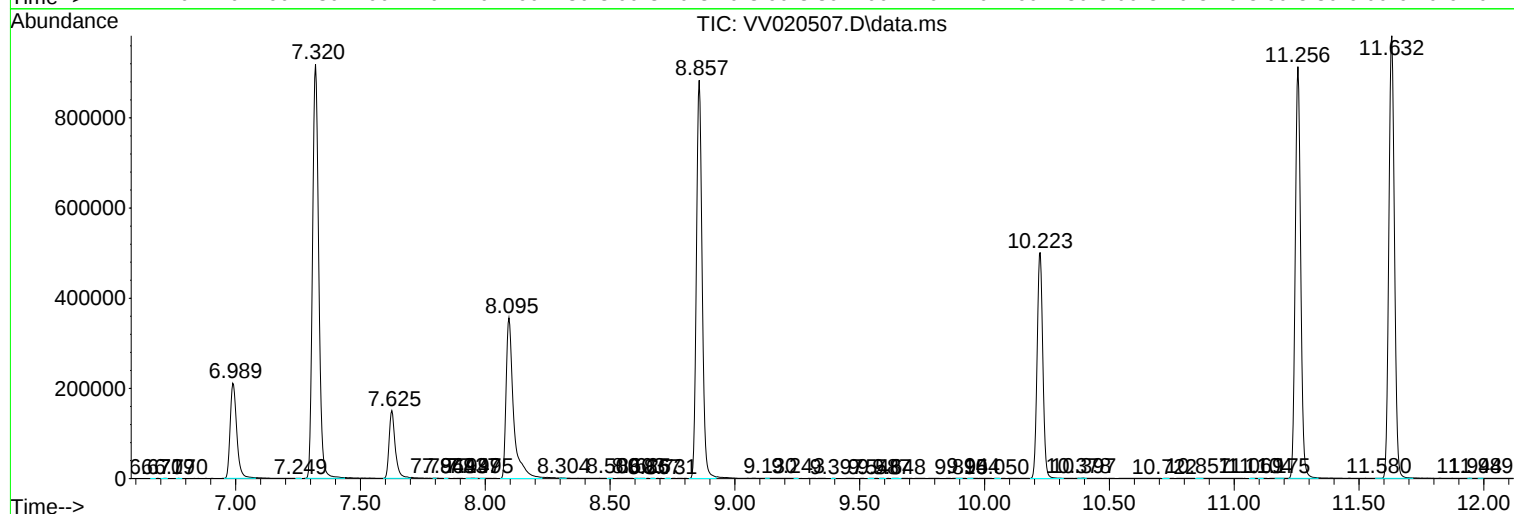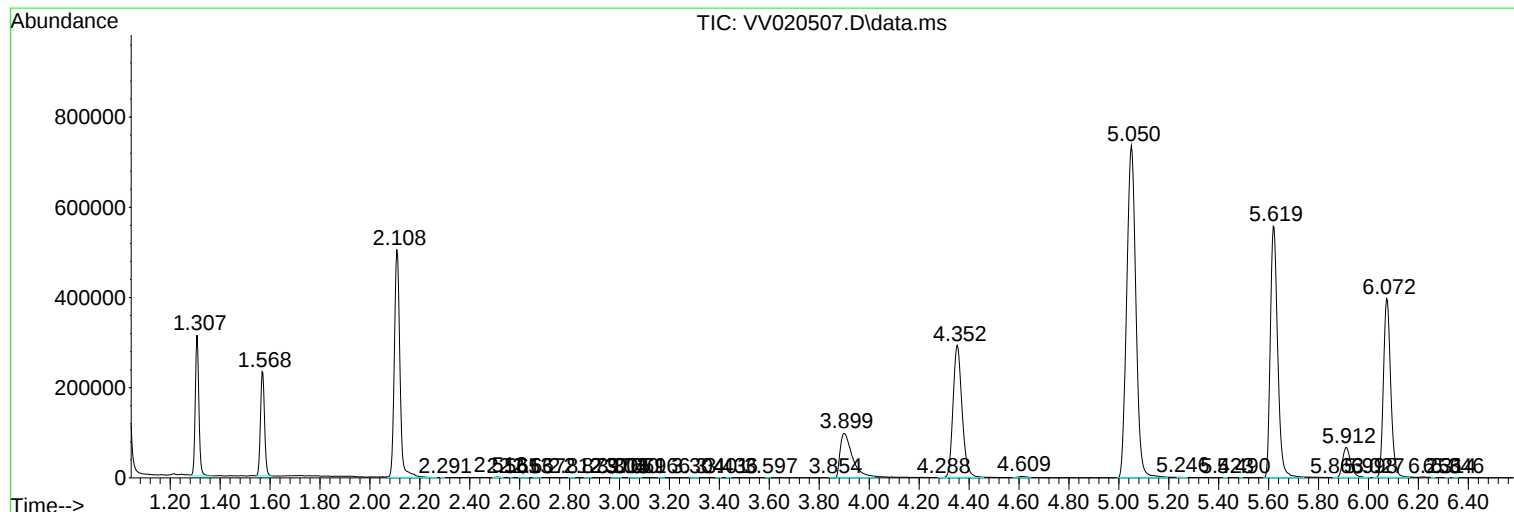

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020507.D
Acq On : 10 Mar 2021 19:52
Operator : SY/MD
Sample : M1632-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020507.D
Acq On : 10 Mar 2021 19:52
Operator : SY/MD
Sample : M1632-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
