

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020509.D
 Acq On : 10 Mar 2021 20:39
 Operator : SY/MD
 Sample : M1632-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

Signal : TIC: VV020509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	101	rVB	316512	317961	16.58%	2.134%
2	1.568	157	164	180	rVB	234503	268558	14.01%	1.802%
3	2.108	321	332	364	rBV	507697	756815	39.47%	5.079%
4	2.503	452	455	457	rBV4	1081	847	0.04%	0.006%
5	2.590	479	482	484	rBV	292	160	0.01%	0.001%
6	2.757	532	534	535	rBV	142	40	0.00%	0.000%
7	2.912	580	582	583	rBV	151	62	0.00%	0.000%
8	3.121	645	647	650	rBV2	315	164	0.01%	0.001%
9	3.153	654	657	661	rVB2	136	90	0.00%	0.001%
10	3.294	698	701	703	rBV2	106	59	0.00%	0.000%
11	3.484	758	760	763	rBV	81	35	0.00%	0.000%
12	3.500	763	765	766	rBV	229	57	0.00%	0.000%
13	3.551	779	781	784	rBV2	88	46	0.00%	0.000%
14	3.584	788	791	792	rBV	76	40	0.00%	0.000%
15	3.596	792	795	797	rVB	183	104	0.01%	0.001%
16	3.616	799	801	803	rBV2	82	41	0.00%	0.000%
17	3.632	803	806	808	rBV2	49	29	0.00%	0.000%
18	3.648	808	811	812	rBV	87	47	0.00%	0.000%
19	3.703	826	828	833	rVB2	265	165	0.01%	0.001%
20	3.744	833	841	845	rBV2	243	292	0.02%	0.002%
21	3.770	845	849	852	rBV	248	178	0.01%	0.001%
22	3.786	852	854	856	rVB	108	47	0.00%	0.000%
23	3.799	856	858	860	rBV2	71	41	0.00%	0.000%
24	3.812	860	862	864	rVB	150	56	0.00%	0.000%
25	3.825	864	866	869	rBV	92	56	0.00%	0.000%
26	3.841	869	871	873	rVB2	58	23	0.00%	0.000%
27	3.854	873	875	878	rBV2	143	78	0.00%	0.001%
28	3.899	878	889	934	rBV	103568	358320	18.69%	2.404%
29	4.352	1013	1030	1056	rBV	302761	764556	39.87%	5.130%
30	4.558	1091	1094	1096	rBV2	292	221	0.01%	0.001%
31	4.641	1117	1120	1121	rBV	102	65	0.00%	0.000%
32	4.654	1121	1124	1127	rVB4	364	270	0.01%	0.002%
33	4.699	1136	1138	1139	rVB4	138	33	0.00%	0.000%
34	4.789	1161	1166	1168	rBV2	154	143	0.01%	0.001%
35	4.841	1180	1182	1184	rBV	62	28	0.00%	0.000%
36	4.857	1184	1187	1191	rVV	181	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020509.D
 Acq On : 10 Mar 2021 20:39
 Operator : SY/MD
 Sample : M1632-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	4.873	1191	1192	1195	rVB	133	37	0.00%	0.000%
38	4.886	1195	1196	1197	rVB	112	22	0.00%	0.000%
39	4.905	1197	1202	1205	rBV2	315	193	0.01%	0.001%
40	4.950	1214	1216	1220	rBV	278	198	0.01%	0.001%
41	4.966	1220	1221	1223	rVB	182	67	0.00%	0.000%
42	5.050	1230	1247	1283	rBV2	753906	1917446	100.00%	12.867%
43	5.423	1359	1363	1368	rVB2	549	494	0.03%	0.003%
44	5.448	1368	1371	1375	rBV2	291	218	0.01%	0.001%
45	5.484	1380	1382	1384	rBV2	249	94	0.00%	0.001%
46	5.532	1395	1397	1399	rBV	211	97	0.01%	0.001%
47	5.548	1400	1402	1406	rVB2	278	153	0.01%	0.001%
48	5.619	1412	1424	1454	rBV	567336	1141905	59.55%	7.663%
49	5.911	1503	1515	1538	rVB3	66237	146043	7.62%	0.980%
50	6.072	1552	1565	1595	rBV	407197	825745	43.06%	5.541%
51	6.307	1635	1638	1641	rVB3	206	131	0.01%	0.001%
52	6.320	1641	1642	1647	rBV2	279	146	0.01%	0.001%
53	6.346	1647	1650	1652	rBV2	396	230	0.01%	0.002%
54	6.397	1662	1666	1670	rVB2	167	123	0.01%	0.001%
55	6.432	1674	1677	1678	rBV	165	72	0.00%	0.000%
56	6.519	1701	1704	1706	rVB	54	28	0.00%	0.000%
57	6.529	1706	1707	1708	rBV	136	40	0.00%	0.000%
58	6.558	1714	1716	1720	rBV	130	71	0.00%	0.000%
59	6.580	1720	1723	1725	rBV2	128	76	0.00%	0.001%
60	6.619	1732	1735	1738	rBV	170	116	0.01%	0.001%
61	6.728	1768	1769	1770	rBV	185	41	0.00%	0.000%
62	6.892	1817	1820	1824	rBV	171	171	0.01%	0.001%
63	6.989	1838	1850	1875	rBV	219229	397992	20.76%	2.671%
64	7.255	1931	1933	1938	rVB2	234	191	0.01%	0.001%
65	7.320	1939	1953	1984	rBV	958814	1641217	85.59%	11.013%
66	7.625	2037	2048	2070	rBV	152232	266432	13.90%	1.788%
67	7.792	2097	2100	2103	rBV3	289	206	0.01%	0.001%
68	7.863	2121	2122	2124	rBV	155	74	0.00%	0.000%
69	7.876	2124	2126	2127	rVB	264	77	0.00%	0.001%
70	7.937	2140	2145	2146	rBV2	418	351	0.02%	0.002%
71	7.982	2155	2159	2160	rBV2	319	207	0.01%	0.001%
72	8.008	2165	2167	2169	rBV	160	62	0.00%	0.000%
73	8.095	2183	2194	2234	rBV2	397917	811289	42.31%	5.444%
74	8.513	2323	2324	2330	rVB3	424	213	0.01%	0.001%
75	8.561	2337	2339	2342	rBV	349	147	0.01%	0.001%
76	8.606	2351	2353	2355	rVB	187	90	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020509.D
 Acq On : 10 Mar 2021 20:39
 Operator : SY/MD
 Sample : M1632-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	8.654	2366	2368	2370	rVB2	191	79	0.00%	0.001%
78	8.683	2370	2377	2384	rBV2	256	424	0.02%	0.003%
79	8.857	2418	2431	2463	rBV	890458	1430412	74.60%	9.599%
80	9.095	2502	2505	2506	rBV2	291	186	0.01%	0.001%
81	9.146	2519	2521	2525	rBV2	485	294	0.02%	0.002%
82	9.246	2550	2552	2559	rVB3	331	289	0.02%	0.002%
83	9.294	2564	2567	2570	rBV	225	150	0.01%	0.001%
84	9.426	2605	2608	2613	rBV2	162	141	0.01%	0.001%
85	9.760	2711	2712	2713	rVB	222	43	0.00%	0.000%
86	9.779	2713	2718	2720	rBV2	219	183	0.01%	0.001%
87	9.799	2721	2724	2729	rVV	286	232	0.01%	0.002%
88	9.879	2745	2749	2753	rBV	212	240	0.01%	0.002%
89	9.911	2756	2759	2763	rVV2	242	184	0.01%	0.001%
90	10.149	2829	2833	2834	rBV	211	163	0.01%	0.001%
91	10.223	2843	2856	2877	rBV	528952	835874	43.59%	5.609%
92	10.587	2967	2969	2970	rBV	204	70	0.00%	0.000%
93	10.812	3036	3039	3043	rBV	246	187	0.01%	0.001%
94	11.027	3105	3106	3107	rBV	160	58	0.00%	0.000%
95	11.255	3165	3177	3204	rBV	937772	1416134	73.86%	9.503%
96	11.632	3281	3294	3315	rBV	1020259	1593653	83.11%	10.694%
97	11.882	3369	3372	3375	rBV3	476	370	0.02%	0.002%
98	12.937	3698	3700	3701	rBV	553	145	0.01%	0.001%
99	13.538	3883	3887	3889	rBV	567	364	0.02%	0.002%




Sum of corrected areas: 14902217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020509.D
Acq On : 10 Mar 2021 20:39
Operator : SY/MD
Sample : M1632-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

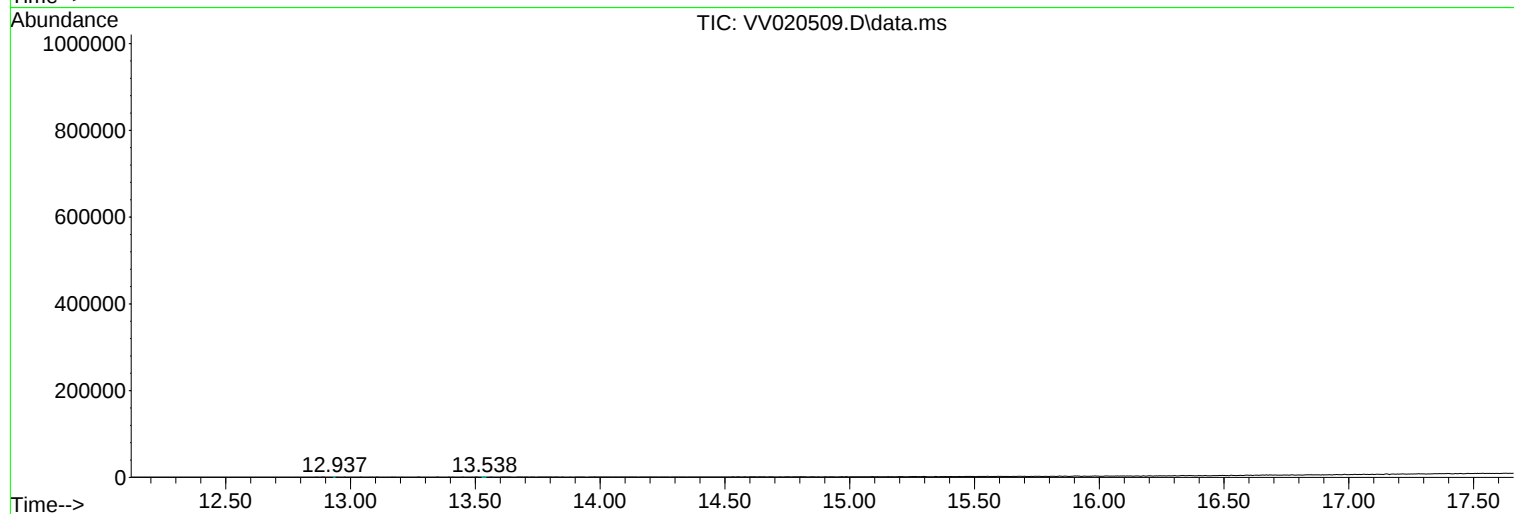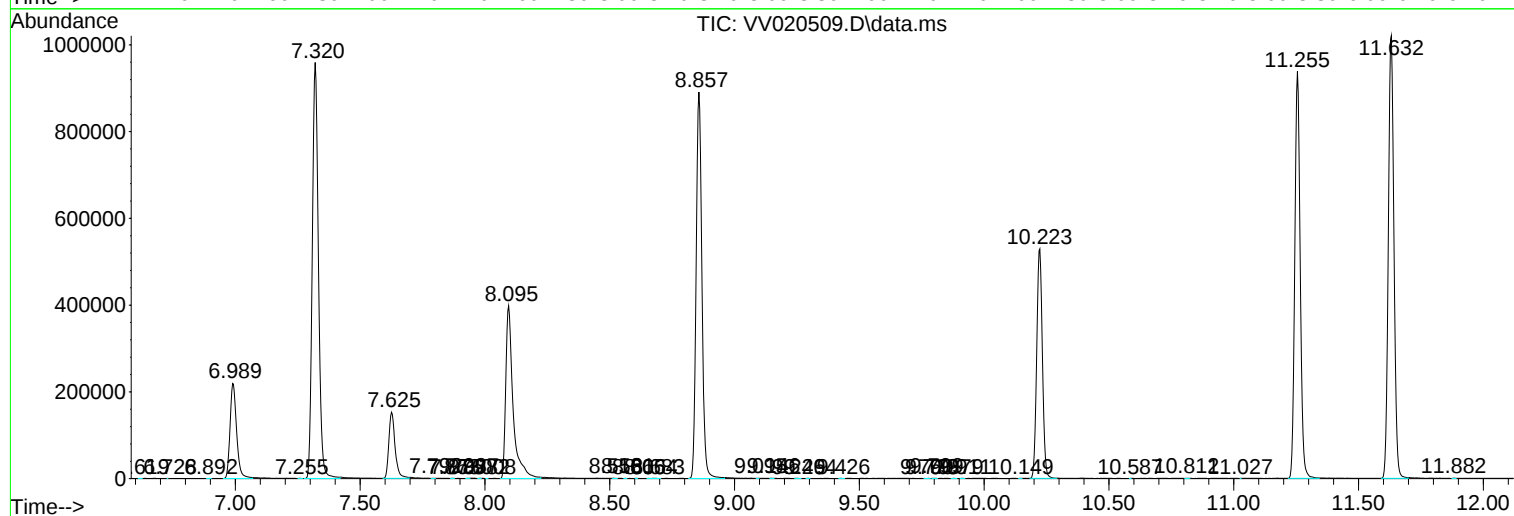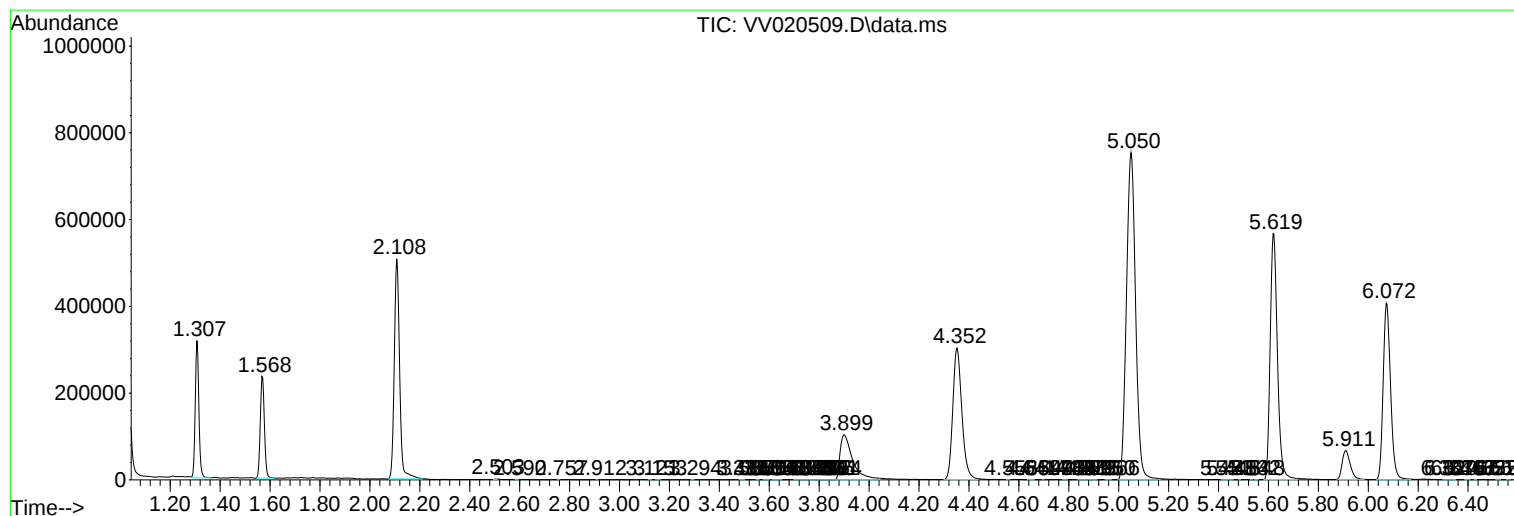

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020509.D
Acq On : 10 Mar 2021 20:39
Operator : SY/MD
Sample : M1632-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020509.D
Acq On : 10 Mar 2021 20:39
Operator : SY/MD
Sample : M1632-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------