

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020510.D
 Acq On : 10 Mar 2021 21:03
 Operator : SY/MD
 Sample : M1632-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	316109	318247	16.49%	2.135%
2	1.571	156	165	178	rBV	241014	273293	14.16%	1.834%
3	2.108	320	332	361	rBV	507234	750609	38.89%	5.036%
4	2.400	420	423	426	rBV3	238	194	0.01%	0.001%
5	2.436	429	434	438	rVV2	453	503	0.03%	0.003%
6	2.455	438	440	443	rVV2	285	175	0.01%	0.001%
7	2.478	444	447	451	rVV2	400	325	0.02%	0.002%
8	2.513	451	458	467	rVB5	1132	1661	0.09%	0.011%
9	2.558	467	472	474	rBV2	270	218	0.01%	0.001%
10	2.696	512	515	520	rVB2	229	192	0.01%	0.001%
11	2.732	522	526	527	rVV2	245	140	0.01%	0.001%
12	2.767	535	537	541	rVB2	270	159	0.01%	0.001%
13	2.828	551	556	557	rBV	292	172	0.01%	0.001%
14	3.043	621	623	625	rBV2	191	134	0.01%	0.001%
15	3.307	700	705	706	rBV	310	201	0.01%	0.001%
16	3.317	706	708	711	rVB2	242	147	0.01%	0.001%
17	3.503	760	766	770	rBV2	240	340	0.02%	0.002%
18	3.609	794	799	805	rVB	248	268	0.01%	0.002%
19	3.648	805	811	813	rBV2	191	170	0.01%	0.001%
20	3.683	819	822	827	rVB	313	294	0.02%	0.002%
21	3.709	827	830	834	rBV2	240	252	0.01%	0.002%
22	3.899	878	889	940	rBV	102125	350824	18.17%	2.354%
23	4.352	1012	1030	1060	rBV	300357	757970	39.27%	5.085%
24	5.050	1229	1247	1284	rBV2	766431	1930258	100.00%	12.951%
25	5.272	1314	1316	1320	rVB3	431	265	0.01%	0.002%
26	5.320	1329	1331	1334	rVB3	321	153	0.01%	0.001%
27	5.339	1334	1337	1339	rBV2	221	138	0.01%	0.001%
28	5.404	1352	1357	1360	rBV3	228	230	0.01%	0.002%
29	5.423	1361	1363	1370	rVB3	371	380	0.02%	0.003%
30	5.452	1370	1372	1375	rVB2	306	189	0.01%	0.001%
31	5.474	1376	1379	1384	rBV4	406	407	0.02%	0.003%
32	5.542	1395	1400	1404	rVB3	272	238	0.01%	0.002%
33	5.622	1411	1425	1454	rBV	572632	1150506	59.60%	7.719%
34	5.818	1483	1486	1492	rVB4	399	346	0.02%	0.002%
35	5.908	1502	1514	1542	rVB2	59626	123960	6.42%	0.832%
36	6.072	1549	1565	1595	rBV	408513	826190	42.80%	5.543%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020510.D
 Acq On : 10 Mar 2021 21:03
 Operator : SY/MD
 Sample : M1632-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

37	6.288	1628	1632	1636	rBV3	305	291	0.02%	0.002%
38	6.493	1694	1696	1702	rBV2	138	147	0.01%	0.001%
39	6.551	1709	1714	1717	rBV2	144	176	0.01%	0.001%
40	6.609	1725	1732	1733	rBV2	271	257	0.01%	0.002%
41	6.651	1743	1745	1748	rVV2	204	140	0.01%	0.001%
42	6.799	1787	1791	1793	rBV	266	218	0.01%	0.001%
43	6.937	1831	1834	1838	rVB	235	137	0.01%	0.001%
44	6.989	1838	1850	1880	rBV	217580	399231	20.68%	2.679%
45	7.127	1891	1893	1898	rBV3	466	353	0.02%	0.002%
46	7.175	1905	1908	1911	rVB2	404	194	0.01%	0.001%
47	7.188	1911	1912	1915	rVB2	356	133	0.01%	0.001%
48	7.227	1920	1924	1927	rBV3	212	192	0.01%	0.001%
49	7.320	1940	1953	1984	rBV	962367	1652755	85.62%	11.089%
50	7.625	2038	2048	2069	rBV2	154496	266944	13.83%	1.791%
51	7.879	2124	2127	2130	rBV	186	147	0.01%	0.001%
52	7.918	2137	2139	2141	rVB	446	215	0.01%	0.001%
53	7.940	2141	2146	2148	rBV	554	546	0.03%	0.004%
54	7.979	2155	2158	2162	rBV3	386	262	0.01%	0.002%
55	8.018	2167	2170	2175	rVB2	245	230	0.01%	0.002%
56	8.095	2183	2194	2234	rBV2	394736	805837	41.75%	5.407%
57	8.448	2300	2304	2308	rVB	353	290	0.02%	0.002%
58	8.500	2315	2320	2324	rVB3	350	346	0.02%	0.002%
59	8.532	2324	2330	2333	rBV3	293	318	0.02%	0.002%
60	8.622	2353	2358	2361	rBV2	439	383	0.02%	0.003%
61	8.857	2418	2431	2454	rBV	884013	1429390	74.05%	9.590%
62	9.091	2501	2504	2509	rBV2	163	188	0.01%	0.001%
63	9.185	2529	2533	2535	rBV3	392	317	0.02%	0.002%
64	9.313	2569	2573	2574	rBV	267	141	0.01%	0.001%
65	9.326	2574	2577	2580	rVB	196	131	0.01%	0.001%
66	9.368	2588	2590	2594	rVB2	266	143	0.01%	0.001%
67	9.474	2619	2623	2626	rBV2	186	143	0.01%	0.001%
68	9.516	2633	2636	2639	rBV2	195	157	0.01%	0.001%
69	9.818	2728	2730	2734	rVB2	310	153	0.01%	0.001%
70	9.892	2750	2753	2759	rVB	195	177	0.01%	0.001%
71	9.956	2770	2773	2777	rVB2	237	168	0.01%	0.001%
72	10.223	2844	2856	2884	rVB	526153	828705	42.93%	5.560%
73	10.390	2901	2908	2915	rVB3	675	927	0.05%	0.006%
74	10.580	2964	2967	2971	rBV2	340	274	0.01%	0.002%
75	10.628	2978	2982	2987	rBV	300	284	0.01%	0.002%
76	10.744	3014	3018	3023	rBV	352	381	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020510.D
 Acq On : 10 Mar 2021 21:03
 Operator : SY/MD
 Sample : M1632-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	10.905	3066	3068	3073	rVB2	304	218	0.01%	0.001%
78	10.953	3079	3083	3086	rVB2	283	181	0.01%	0.001%
79	11.175	3146	3152	3156	rBV3	334	433	0.02%	0.003%
80	11.255	3165	3177	3201	rBV	939683	1416561	73.39%	9.504%
81	11.564	3270	3273	3275	rBV	327	209	0.01%	0.001%
82	11.632	3280	3294	3320	rBV	1038302	1601496	82.97%	10.745%
83	11.815	3348	3351	3356	rBV2	331	263	0.01%	0.002%
84	11.863	3363	3366	3370	rVB2	346	213	0.01%	0.001%
85	11.911	3379	3381	3384	rBV	246	143	0.01%	0.001%
86	11.966	3394	3398	3401	rVB	443	351	0.02%	0.002%
87	11.988	3402	3405	3409	rBV	306	259	0.01%	0.002%
88	12.033	3416	3419	3425	rVB2	284	229	0.01%	0.002%
89	12.490	3559	3561	3565	rBV2	234	131	0.01%	0.001%
90	12.564	3582	3584	3587	rVB3	372	205	0.01%	0.001%
91	12.664	3613	3615	3620	rBV2	249	159	0.01%	0.001%
92	12.979	3710	3713	3717	rBV	244	174	0.01%	0.001%
93	13.120	3754	3757	3759	rBV	196	138	0.01%	0.001%
94	13.278	3803	3806	3808	rBV	306	191	0.01%	0.001%
95	13.522	3880	3882	3887	rVB3	393	217	0.01%	0.001%
96	13.725	3943	3945	3947	rBV2	267	144	0.01%	0.001%
97	13.837	3976	3980	3990	rBV3	413	813	0.04%	0.005%
98	14.162	4078	4081	4084	rBV	397	304	0.02%	0.002%
99	14.567	4205	4207	4208	rBV	367	156	0.01%	0.001%
100	15.059	4358	4360	4363	rBV2	460	319	0.02%	0.002%




Sum of corrected areas: 14904676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020510.D
Acq On : 10 Mar 2021 21:03
Operator : SY/MD
Sample : M1632-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

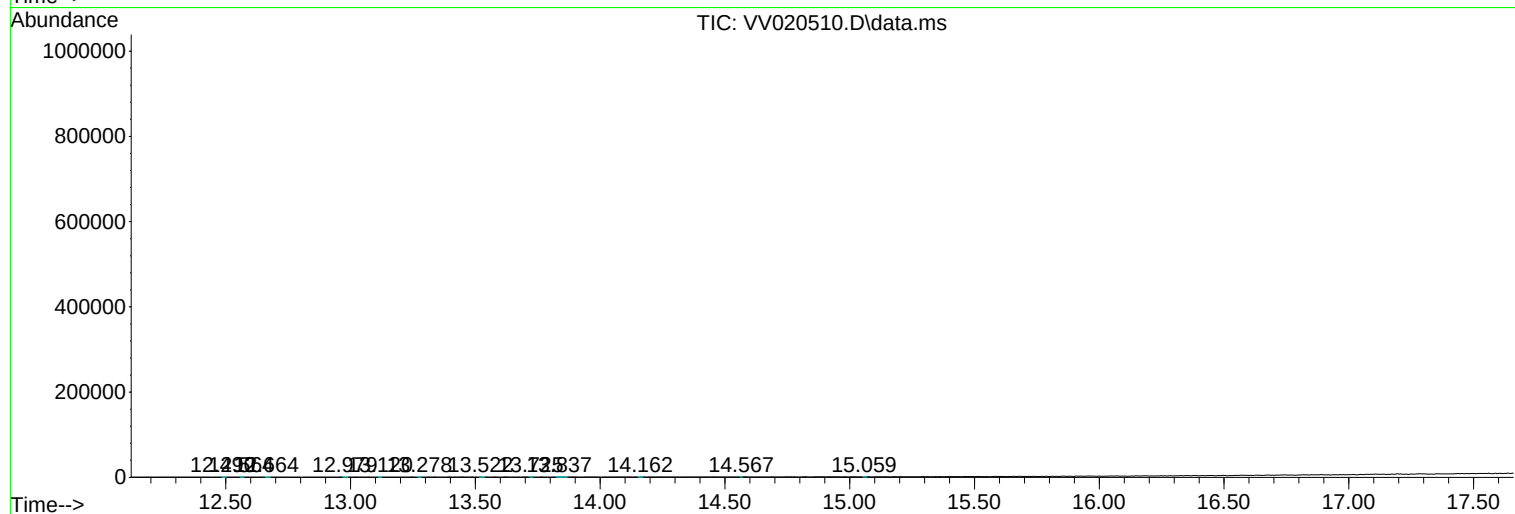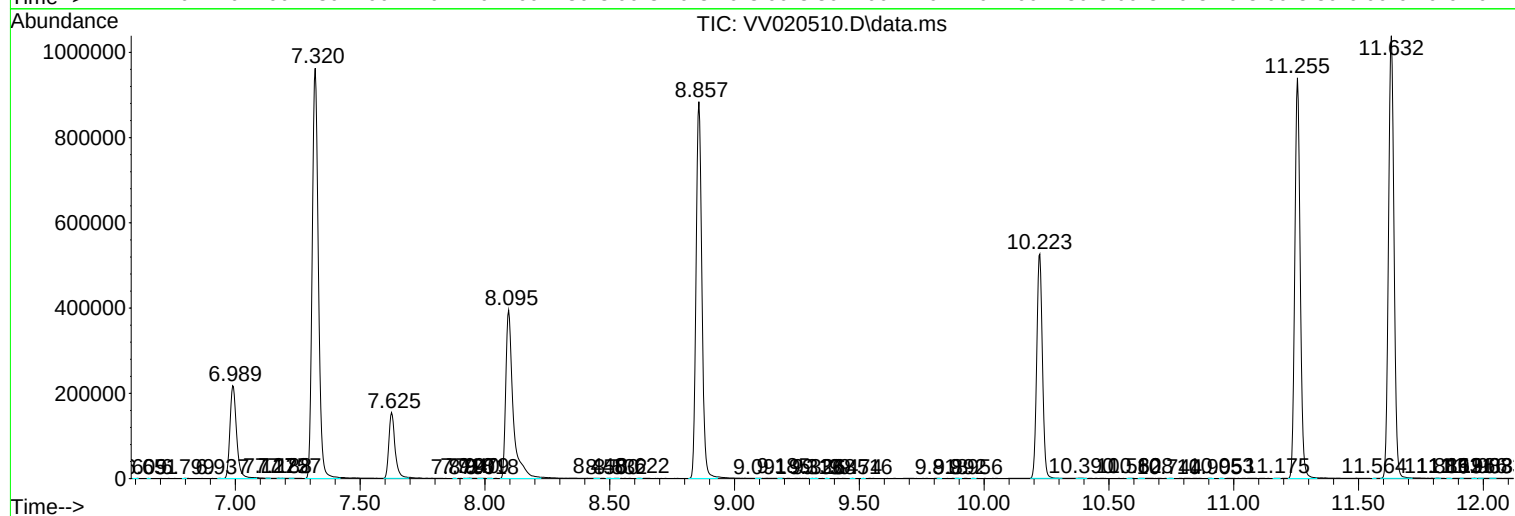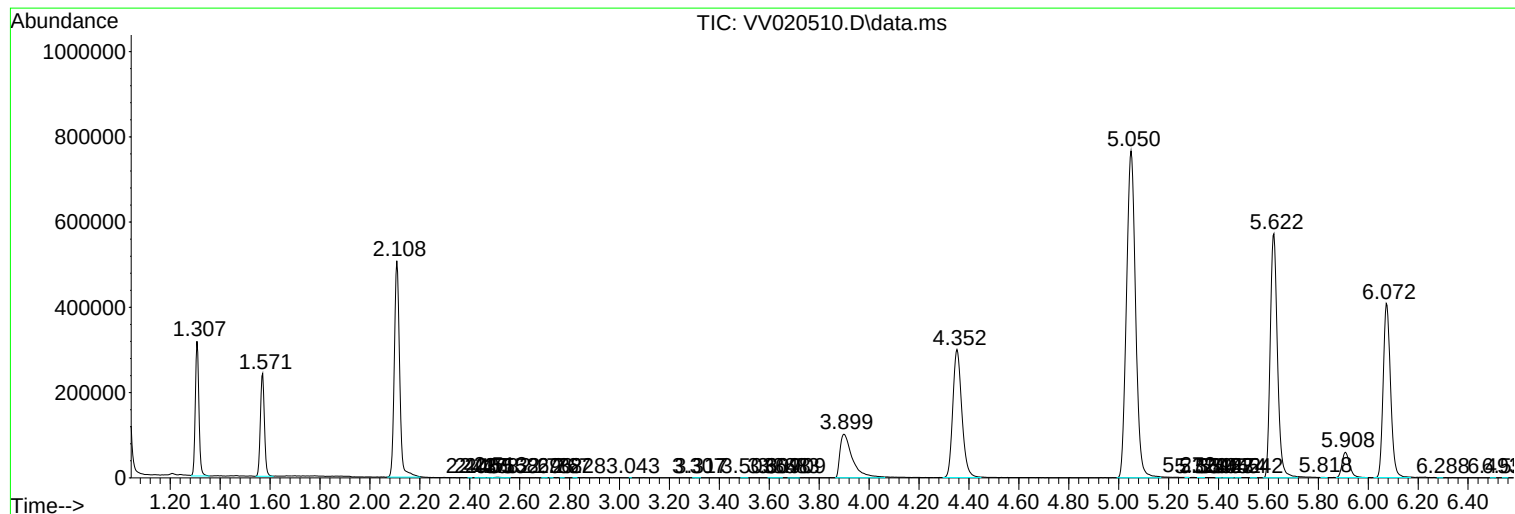

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020510.D
Acq On : 10 Mar 2021 21:03
Operator : SY/MD
Sample : M1632-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020510.D
Acq On : 10 Mar 2021 21:03
Operator : SY/MD
Sample : M1632-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
